

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
 Data File : BP010534.D
 Acq On : 25 May 2022 14:12
 Operator : CG/JU
 Sample : N2918-12DL 20X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTH0DL

Quant Time: May 25 23:26:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	74687	20.000	ng/u1	# 0.00
20) Naphthalene-d8	10.681	136	310024	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.516	164	214823	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.269	188	475892	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.351	240	389294	20.000	ng/u1	# 0.00
88) Perylene-d12	23.768	264	318276	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	661	0.377	ng/uL	0.01
4) Pyridine-d5	3.740	84	898	0.180	ng/u1	-0.02
7) Phenol-d5	7.058	99	3121	0.498	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.099	67	94	0.022	ng/u1	-0.12
11) 2-Chlorophenol-d4	7.422	132	10355	2.159	ng/u1	0.00
15) 4-Methylphenol-d8	8.610	113	6585	1.236	ng/u1	0.01
21) Nitrobenzene-d5	9.052	128	7062	2.943	ng/u1	0.00
24) 2-Nitrophenol-d4	9.769	143	6474	2.546	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	12	0.002	ng/u1	-0.09
31) 4-Chloroaniline-d4	10.840	131	12017	1.681	ng/u1	0.01
46) Dimethylphthalate-d6	13.928	166	59390	3.752	ng/u1	0.00
49) Acenaphthylene-d8	14.334	160	164	0.009	ng/u1	0.12
54) 4-Nitrophenol-d4	14.734	143	19	0.007	ng/u1	0.01
60) Fluorene-d10	15.510	176	50458	3.664	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	4719	1.696	ng/u1	0.01
73) Anthracene-d10	17.369	188	78977	3.665	ng/u1	0.00
81) Pyrene-d10	19.604	212	99982	4.836	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.615	264	56344	3.526	ng/u1	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.734	128	966009	59.656	ng/u1	96
36) 2-Methylnaphthalene	12.345	142	56004	4.885	ng/u1	94
43) 1,1'-Biphenyl	13.357	154	16238	1.030	ng/u1	92
52) Acenaphthene	14.581	153	48401	3.757	ng/u1	91
56) Dibenzofuran	14.916	168	65835	3.487	ng/u1	98
61) Fluorene	15.563	166	42142	2.729	ng/u1	98
72) Phenanthrene	17.310	178	62513	2.461	ng/u1	99
74) Anthracene	17.310	178	62513	2.454	ng/u1	98
77) Carbazole	17.675	167	133271	5.952	ng/u1#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010534.D
Acq On : 25 May 2022 14:12
Operator : CG/JU
Sample : N2918-12DL 20X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTH0DL

Quant Time: May 25 23:26:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 24 05:50:40 2022
Response via : Initial Calibration




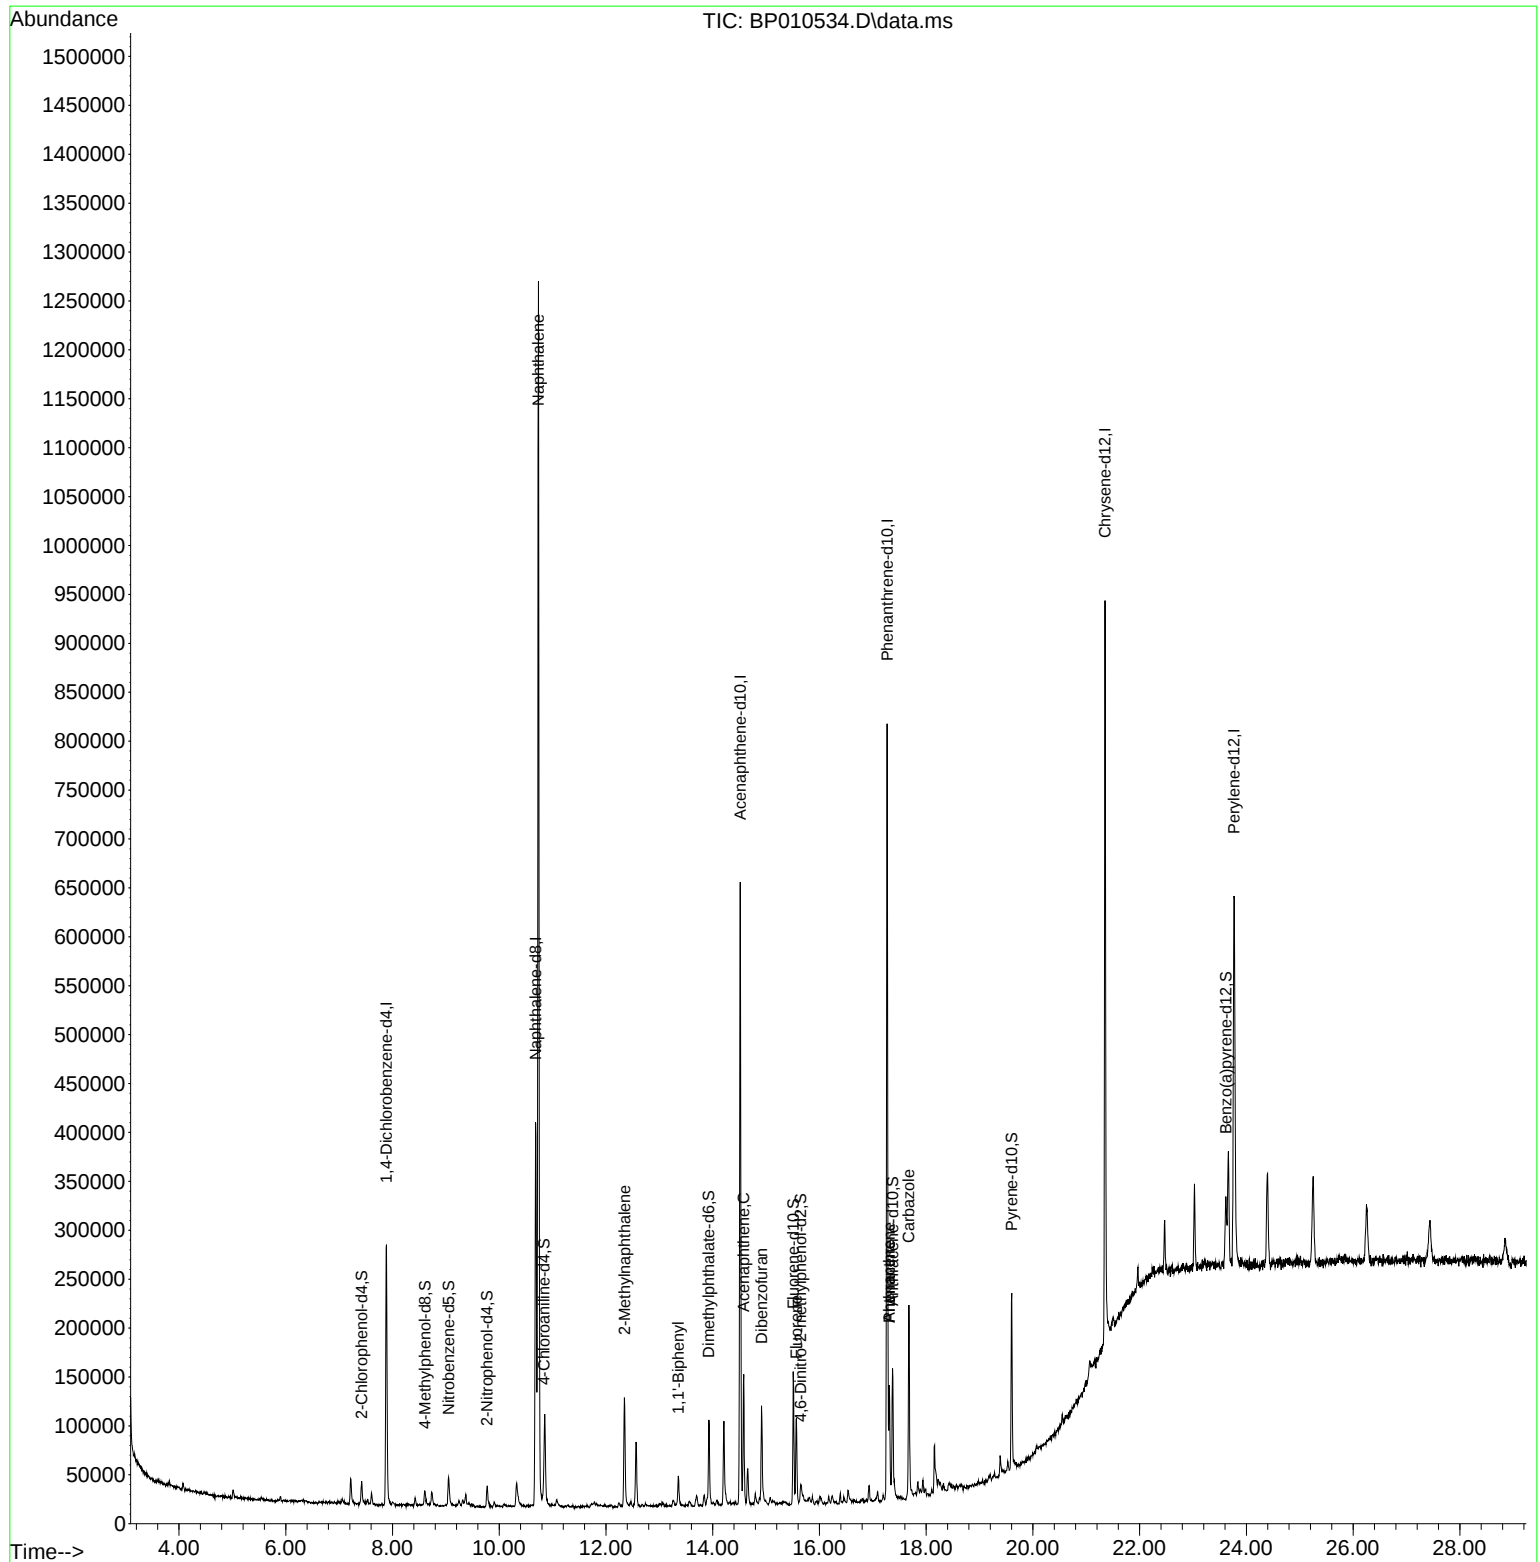


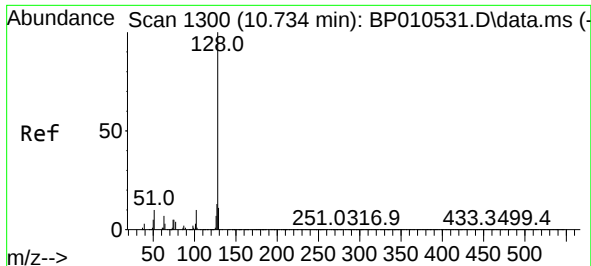

#30
Naphthalene
Concen: 59.656 ng/ul
RT: 10.734 min Scan# 1300
Delta R.T. -0.006 min
Lab File: BP010534.D
Acq: 25 May 2022 14:12




Instrument :
BNA_P
ClientSampleId :
DBTH0DL


Tgt Ion:128 Resp: 966009
Ion Ratio Lower Upper
128 100
129 11.1 8.6 13.0
127 12.9 12.2 18.4

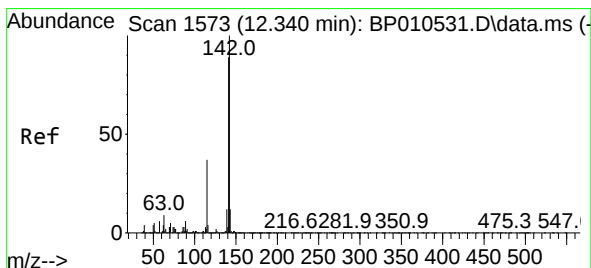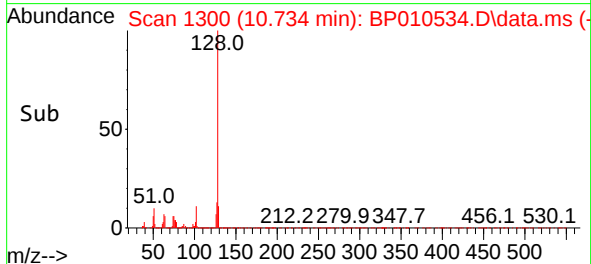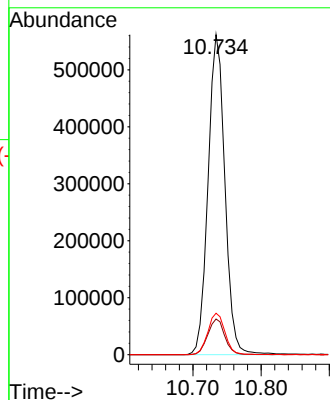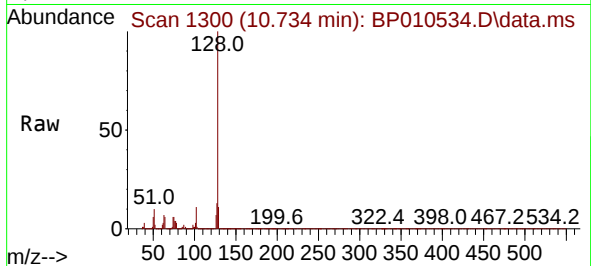

#36
2-Methylnaphthalene
Concen: 4.885 ng/ul
RT: 12.345 min Scan# 1574
Delta R.T. -0.000 min
Lab File: BP010534.D
Acq: 25 May 2022 14:12

Tgt Ion:142 Resp: 56004
Ion Ratio Lower Upper
142 100
141 85.9 64.3 96.5


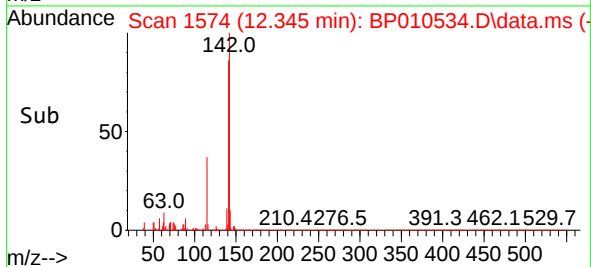
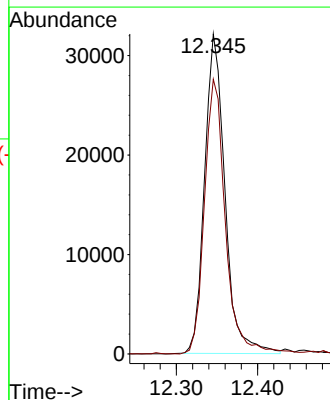
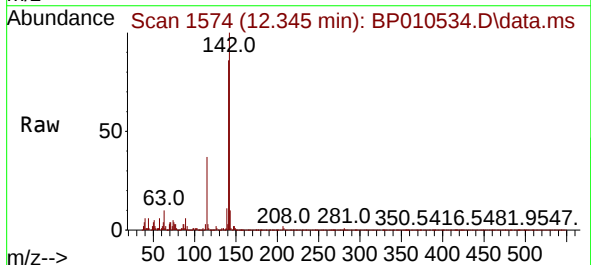


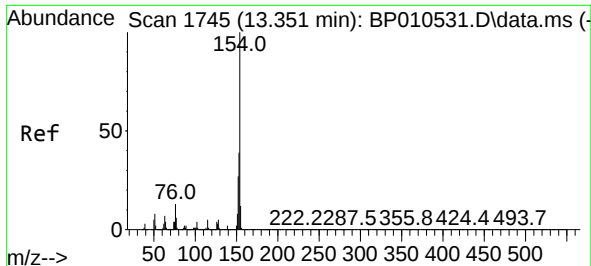

#43
1,1'-Biphenyl
Concen: 1.030 ng/ul
RT: 13.357 min Scan# 1746
Delta R.T. 0.006 min
Lab File: BP010534.D
Acq: 25 May 2022 14:12




Instrument :
BNA_P
ClientSampleId :
DBTH0DL


Tgt Ion:154 Resp: 16238
Ion Ratio Lower Upper
154 100
153 41.1 28.6 43.0
76 12.0 8.5 12.7

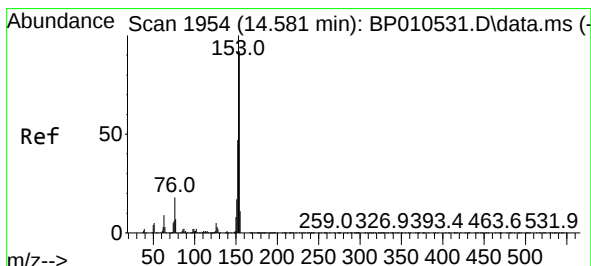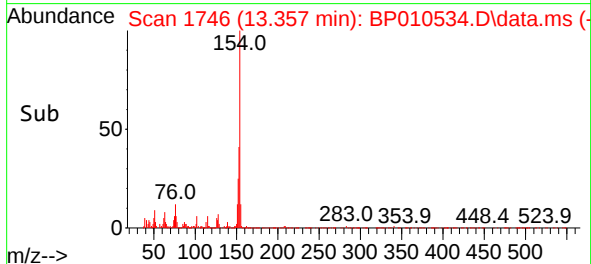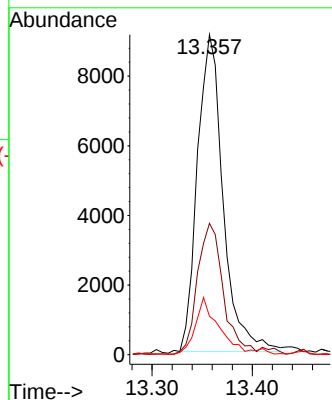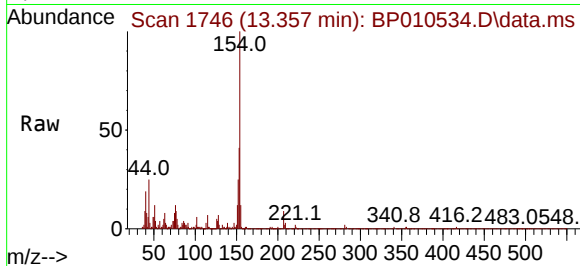

#52
Acenaphthene
Concen: 3.757 ng/ul
RT: 14.581 min Scan# 1954
Delta R.T. -0.000 min
Lab File: BP010534.D
Acq: 25 May 2022 14:12

Tgt Ion:153 Resp: 48401
Ion Ratio Lower Upper
153 100
152 49.4 34.3 51.5
154 95.3 70.0 105.0


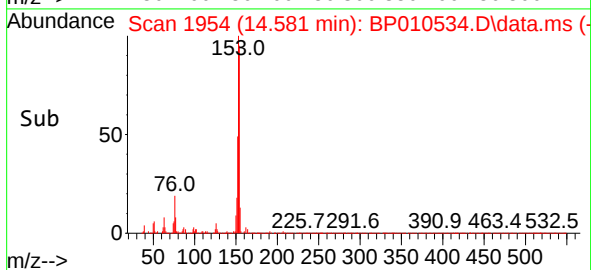
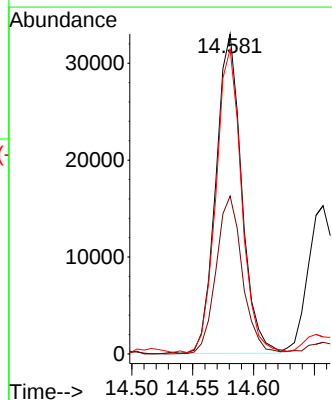
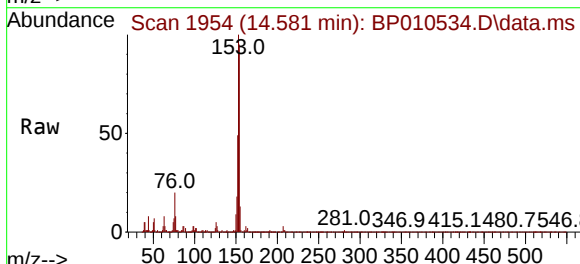


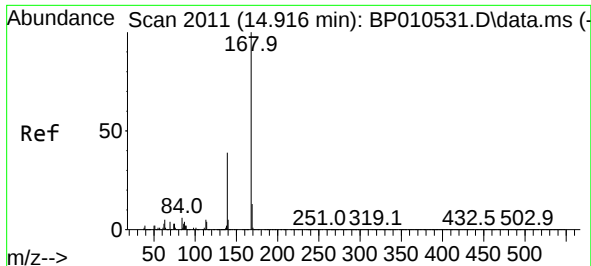

#56
Dibenzofuran
Concen: 3.487 ng/ul
RT: 14.916 min Scan# 2011
Delta R.T. -0.000 min
Lab File: BP010534.D
Acq: 25 May 2022 14:12




Instrument :
BNA_P
ClientSampleId :
DBTH0DL


Tgt Ion:168 Resp: 65835
Ion Ratio Lower Upper
168 100
139 39.0 30.1 45.1

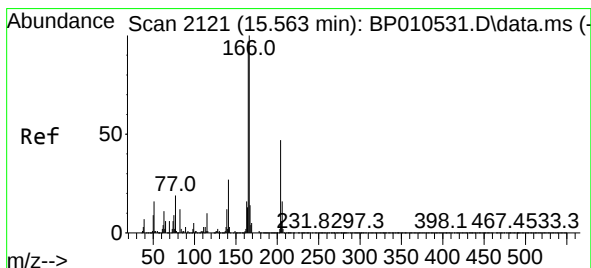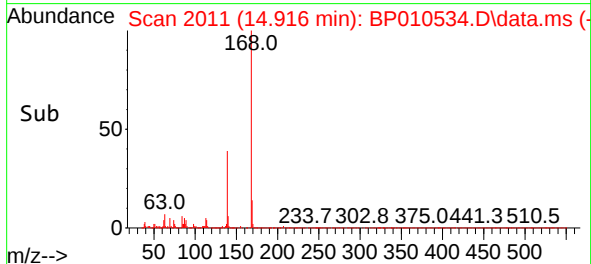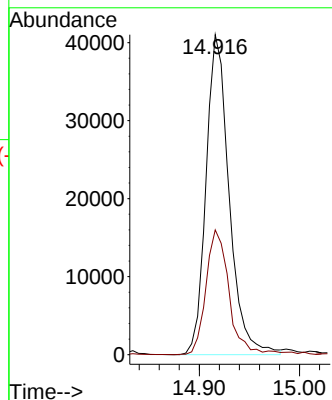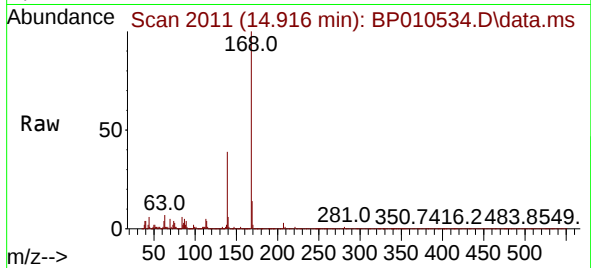

#61
Fluorene
Concen: 2.729 ng/ul
RT: 15.563 min Scan# 2121
Delta R.T. -0.006 min
Lab File: BP010534.D
Acq: 25 May 2022 14:12

Tgt Ion:166 Resp: 42142
Ion Ratio Lower Upper
166 100
165 85.7 70.3 105.5
167 12.6 9.5 14.3

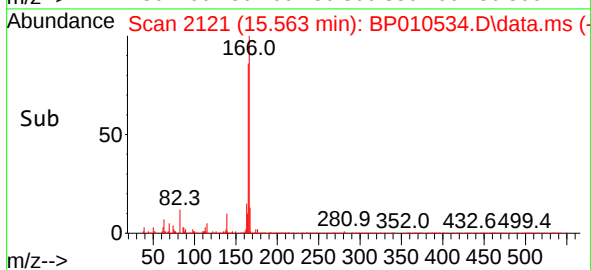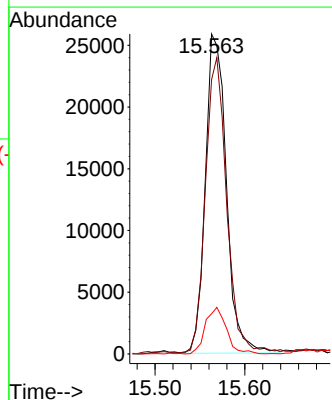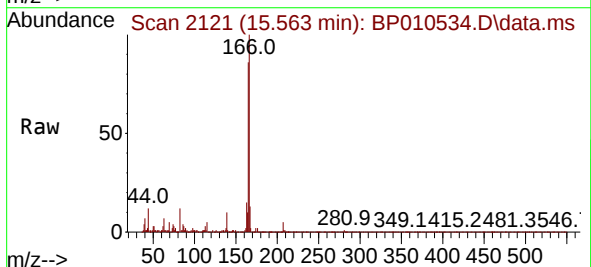

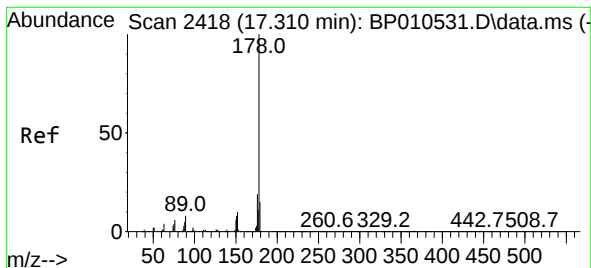

#72

Phenanthrene

Concen: 2.461 ng/ul

RT: 17.310 min Scan# 2418

Delta R.T. -0.006 min

Lab File: BP010534.D

Acq: 25 May 2022 14:12

Instrument :

BNA_P

ClientSampleId :

DBTH0DL





Tgt Ion:178 Resp: 62513

Ion Ratio Lower Upper

178 100

179 14.4 11.7 17.5

176 17.5 14.5 21.7

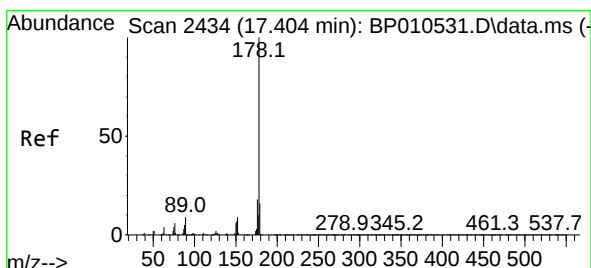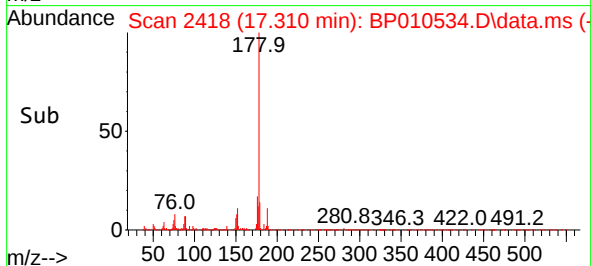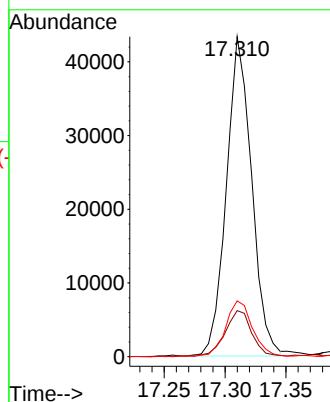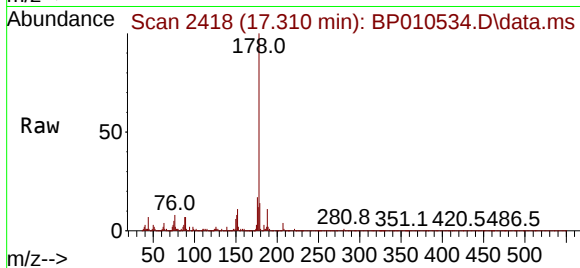

#74

Anthracene

Concen: 2.454 ng/ul

RT: 17.310 min Scan# 2418

Delta R.T. -0.094 min

Lab File: BP010534.D

Acq: 25 May 2022 14:12




Tgt Ion:178 Resp: 62513


Ion Ratio Lower Upper

178 100

179 14.4 12.3 18.5


176 17.5 13.4 20.2

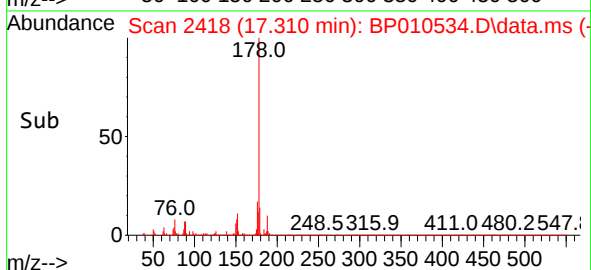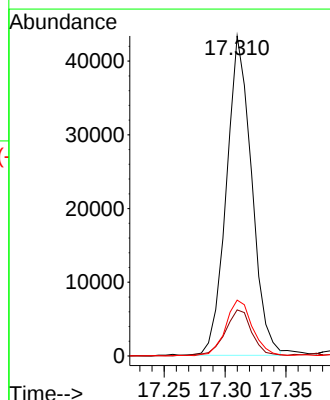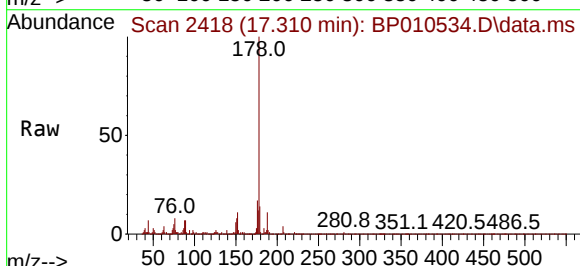

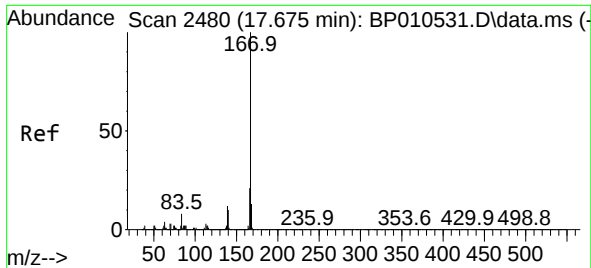

#77
 Carbazole
 Concen: 5.952 ng/ul
 RT: 17.675 min Scan# 24
 Delta R.T. -0.000 min
 Lab File: BP010534.D
 Acq: 25 May 2022 14:12

Instrument :
 BNA_P
 ClientSampleId :
 DBTH0DL

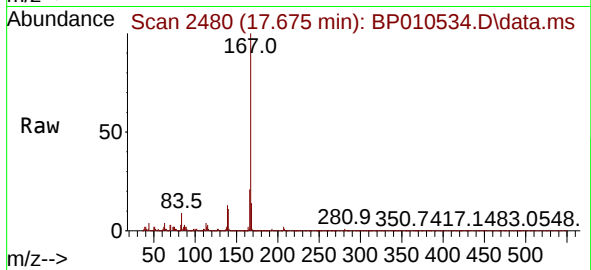

Tgt Ion:167 Resp: 133271
 Ion Ratio Lower Upper
 167 100
 166 21.2 15.8 23.8
 139 13.4 8.3 12.5#

