




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
 Data File : BP010532.D
 Acq On : 25 May 2022 11:53
 Operator : CG/JU
 Sample : PB145008BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK008

Manual IntegrationsAPPROVED

Quant Time: May 25 23:25:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/26/2022
 Supervised By :mohammad ahmed 05/27/2022

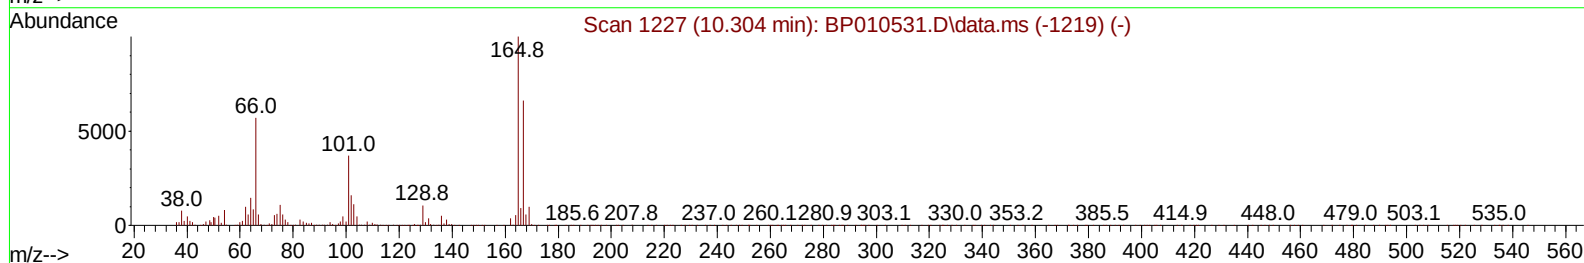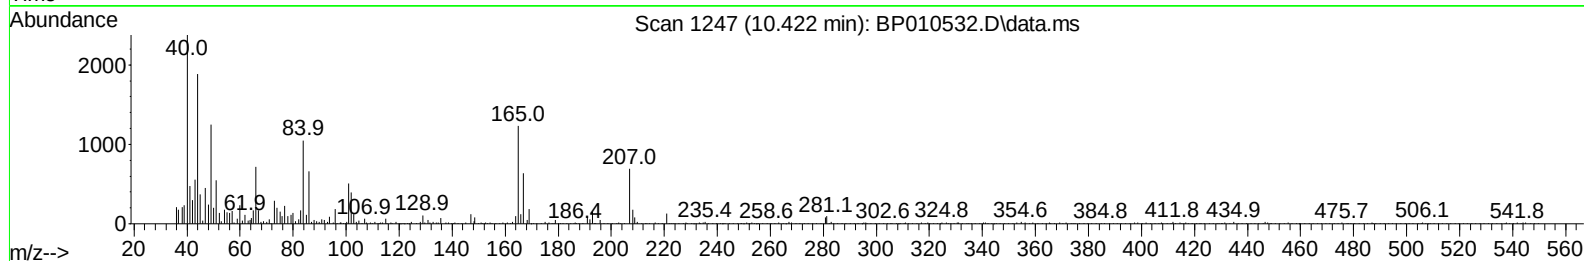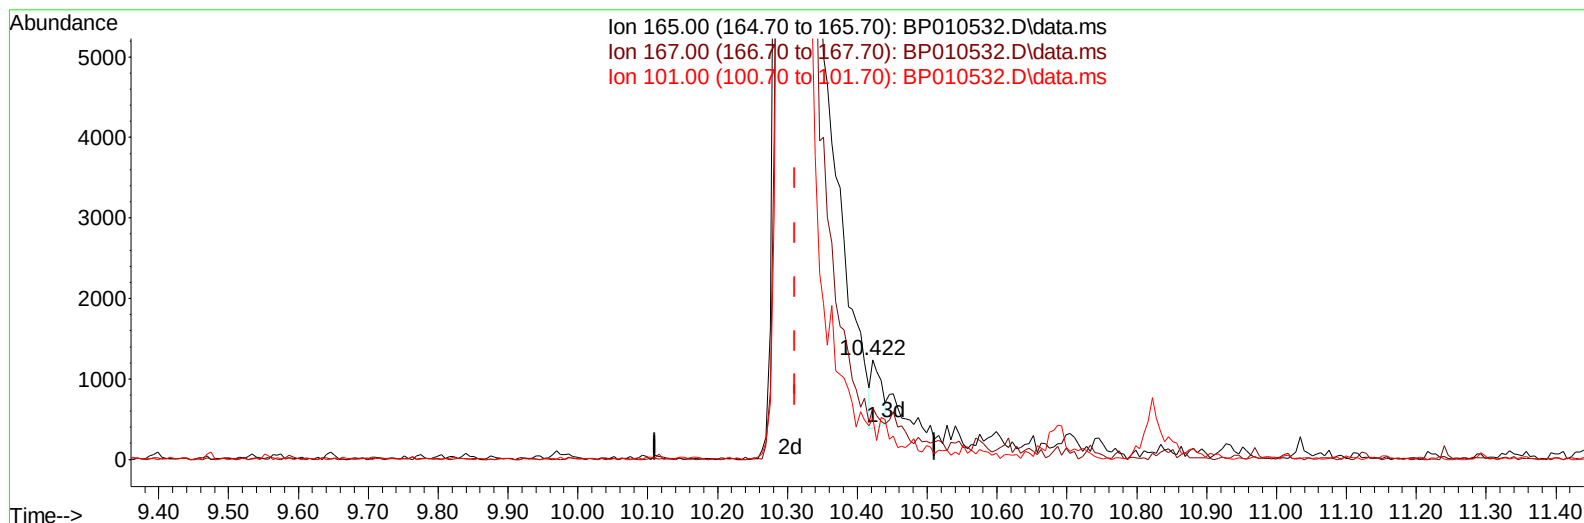

TIC: BP010532.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.422min (+ 0.112) 0.10 ng/ul

response 842

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	51.70
101.00	49.80	41.26
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010532.D
Acq On : 25 May 2022 11:53
Operator : CG/JU
Sample : PB145008BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK008

Manual IntegrationsAPPROVED

Quant Time: May 25 23:25:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 24 05:50:40 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/26/2022
Supervised By :mohammad ahmed 05/27/2022

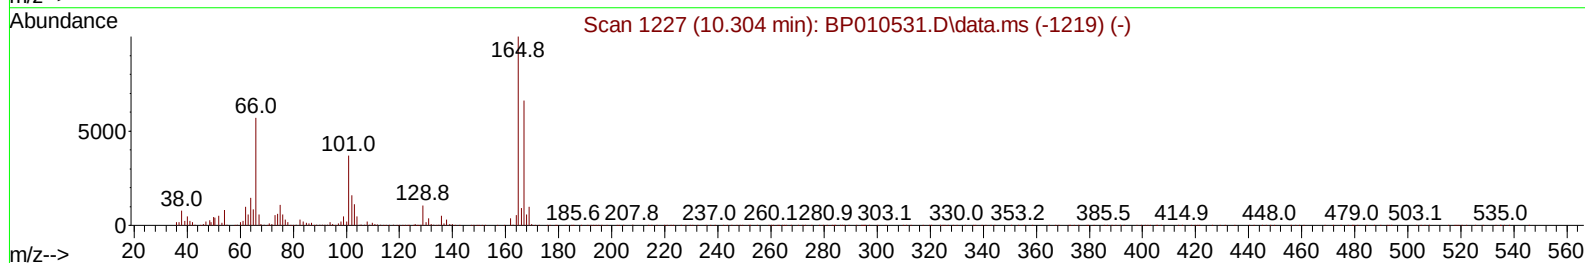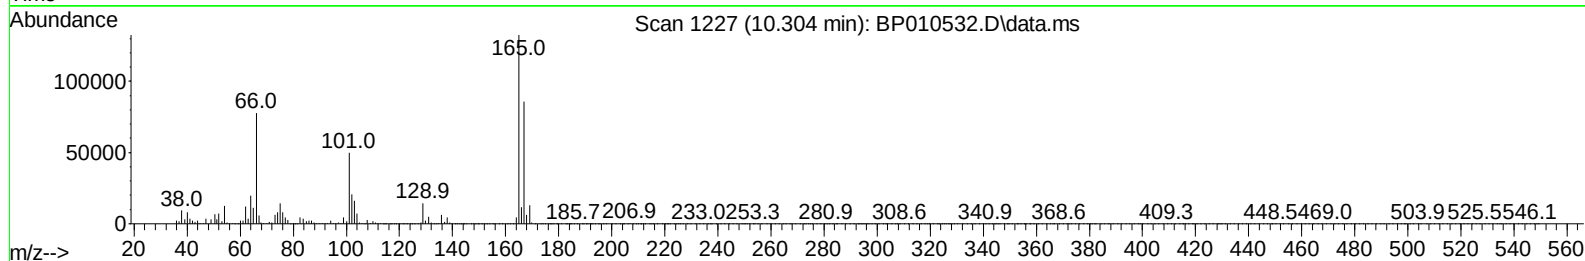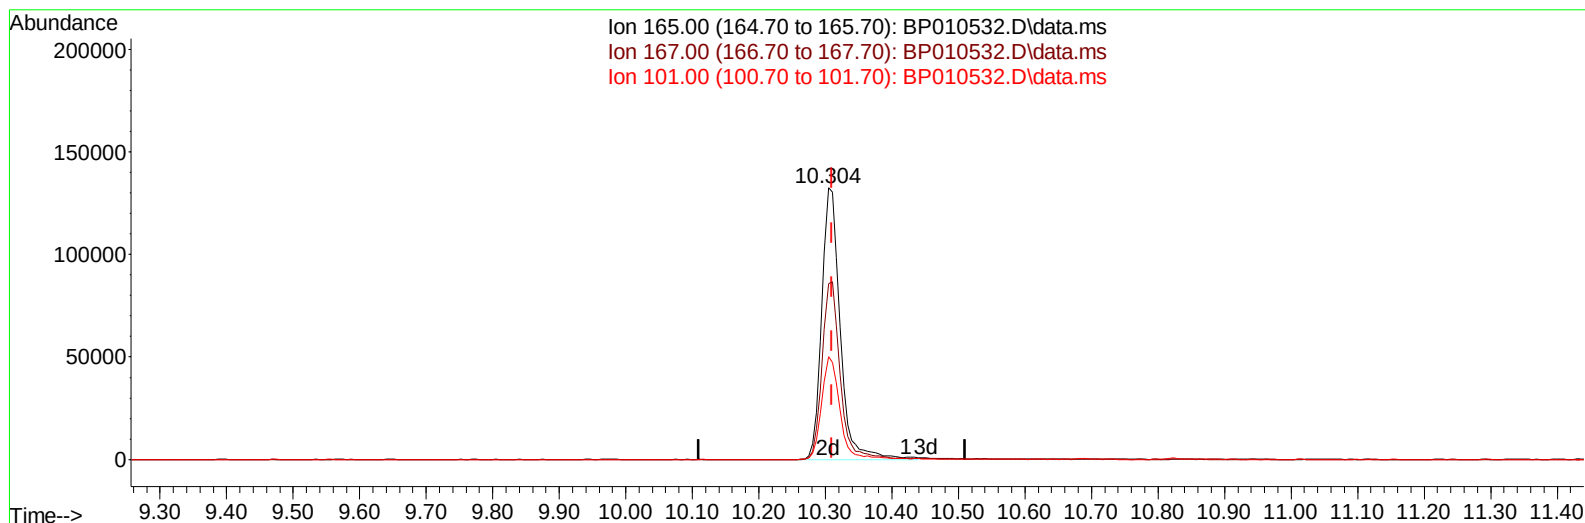

TIC: BP010532.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.304min (-0.006) 28.92 ng/ul m

response 254759

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	64.82
101.00	49.80	37.78#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
 Data File : BP010532.D
 Acq On : 25 May 2022 11:53
 Operator : CG/JU
 Sample : PB145008BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK008

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/26/2022
 Supervised By :mohammad ahmed 05/27/2022

Quant Time: May 25 23:25:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.881	152	131854	20.000	ng/ul	0.00
20) Naphthalene-d8	10.681	136	568016	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.516	164	391919	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.269	188	870858	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.351	240	796456	20.000	ng/ul	0.00
88) Perylene-d12	23.768	264	665269	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	18610	6.016	ng/uL	0.00
4) Pyridine-d5	3.752	84	257215	29.285	ng/ul	0.00
7) Phenol-d5	7.052	99	322176	29.112	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.216	67	230991	31.066	ng/ul	0.00
11) 2-Chlorophenol-d4	7.416	132	263342	31.098	ng/ul	0.00
15) 4-Methylphenol-d8	8.593	113	274727	29.211	ng/ul	0.00
21) Nitrobenzene-d5	9.046	128	140682	32.002	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	153216	32.888	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.304	165	254759m	28.920	ng/ul	0.00
31) 4-Chloroaniline-d4	10.822	131	370955	28.322	ng/ul	0.00
46) Dimethylphthalate-d6	13.928	166	979157	33.910	ng/ul	0.00
49) Acenaphthylene-d8	14.210	160	1063896	31.942	ng/ul	0.00
54) 4-Nitrophenol-d4	14.716	143	138305	26.910	ng/ul	0.00
60) Fluorene-d10	15.510	176	812707	32.352	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	141234	27.730	ng/ul	0.00
73) Anthracene-d10	17.369	188	1333267	33.810	ng/ul	0.00
81) Pyrene-d10	19.598	212	1595162	37.713	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.610	264	1199214	35.899	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010532.D
Acq On : 25 May 2022 11:53
Operator : CG/JU
Sample : PB145008BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK008

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/26/2022
Supervised By :mohammad ahmed 05/27/2022

Quant Time: May 25 23:25:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 24 05:50:40 2022
Response via : Initial Calibration

