

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
 Data File : BP010532.D
 Acq On : 25 May 2022 11:53
 Operator : CG/JU
 Sample : PB145008BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK008

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010532.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	55	rVB	43230	73157	1.76%	0.178%
2	3.752	110	113	129	rBV	454305	836860	20.18%	2.040%
3	5.928	482	483	487	rBV3	4004	4735	0.11%	0.012%
4	6.122	512	516	518	rBV5	2885	4149	0.10%	0.010%
5	7.052	667	674	688	rBV	591904	1011952	24.40%	2.467%
6	7.216	696	702	718	rVB	479998	806054	19.44%	1.965%
7	7.416	729	736	747	rBV	626923	1047729	25.27%	2.554%
8	7.881	807	815	829	rVB	502860	836113	20.16%	2.038%
9	8.593	928	936	951	rBV	763704	1302769	31.42%	3.176%
10	9.040	1005	1012	1024	rBV	640127	1117836	26.96%	2.725%
11	9.763	1128	1135	1147	rBV	517989	922350	22.24%	2.249%
12	10.304	1220	1227	1247	rBV	668507	1294785	31.22%	3.156%
13	10.681	1283	1291	1307	rBV	708258	1252287	30.20%	3.053%
14	10.822	1307	1315	1335	rBV	664755	1339001	32.29%	3.264%
15	12.287	1558	1564	1570	rVB5	11375	24833	0.60%	0.061%
16	12.957	1674	1678	1682	rBV7	2366	4278	0.10%	0.010%
17	13.487	1765	1768	1774	rVB7	2105	4237	0.10%	0.010%
18	13.804	1817	1822	1826	rBV7	2739	5616	0.14%	0.014%
19	13.928	1835	1843	1856	rBV	1513830	2232225	53.83%	5.442%
20	14.022	1856	1859	1865	rVB8	4498	10586	0.26%	0.026%
21	14.210	1882	1891	1904	rBV	1560546	2403721	57.96%	5.860%
22	14.516	1935	1943	1954	rBV	1133074	1742021	42.01%	4.247%
23	14.716	1971	1977	2001	rBV	436713	1036101	24.99%	2.526%
24	14.945	2011	2016	2023	rVB10	9964	19969	0.48%	0.049%
25	15.510	2105	2112	2126	rBV	2103955	3083700	74.36%	7.518%
26	15.634	2126	2133	2144	rVV	712847	1100466	26.54%	2.683%
27	15.751	2148	2153	2159	rVB2	25385	44567	1.07%	0.109%
28	16.298	2242	2246	2252	rVB8	11118	19139	0.46%	0.047%
29	16.610	2295	2299	2302	rBV5	3424	5764	0.14%	0.014%
30	16.939	2352	2355	2359	rVB6	5179	7529	0.18%	0.018%
31	17.051	2370	2374	2375	rBV4	4821	6264	0.15%	0.015%
32	17.269	2402	2411	2421	rBV	1472417	2169600	52.32%	5.289%
33	17.369	2421	2428	2442	rVV	2317758	3486062	84.06%	8.498%
34	17.886	2513	2516	2520	rBV4	6902	10275	0.25%	0.025%
35	18.151	2556	2561	2570	rBV2	83047	167407	4.04%	0.408%
36	18.228	2571	2574	2578	rVB	13992	20994	0.51%	0.051%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010532.D
Acq On : 25 May 2022 11:53
Operator : CG/JU
Sample : PB145008BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK008

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Title : SVOA CALIBRATION

37	19.180	2731	2736	2740	rBV2	38266	52346	1.26%	0.128%
38	19.245	2743	2747	2752	rBV	26815	43818	1.06%	0.107%
39	19.386	2767	2771	2779	rBV5	30697	58950	1.42%	0.144%
40	19.598	2801	2807	2820	rBV	3176513	4146892	100.00%	10.109%
41	21.351	3100	3105	3117	rBV	1555833	2186873	52.74%	5.331%
42	23.610	3482	3489	3505	rBV2	1538366	3269094	78.83%	7.970%
43	23.768	3509	3516	3530	rVB2	814810	1806936	43.57%	4.405%




Sum of corrected areas: 41020040

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010532.D
Acq On : 25 May 2022 11:53
Operator : CG/JU
Sample : PB145008BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK008

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

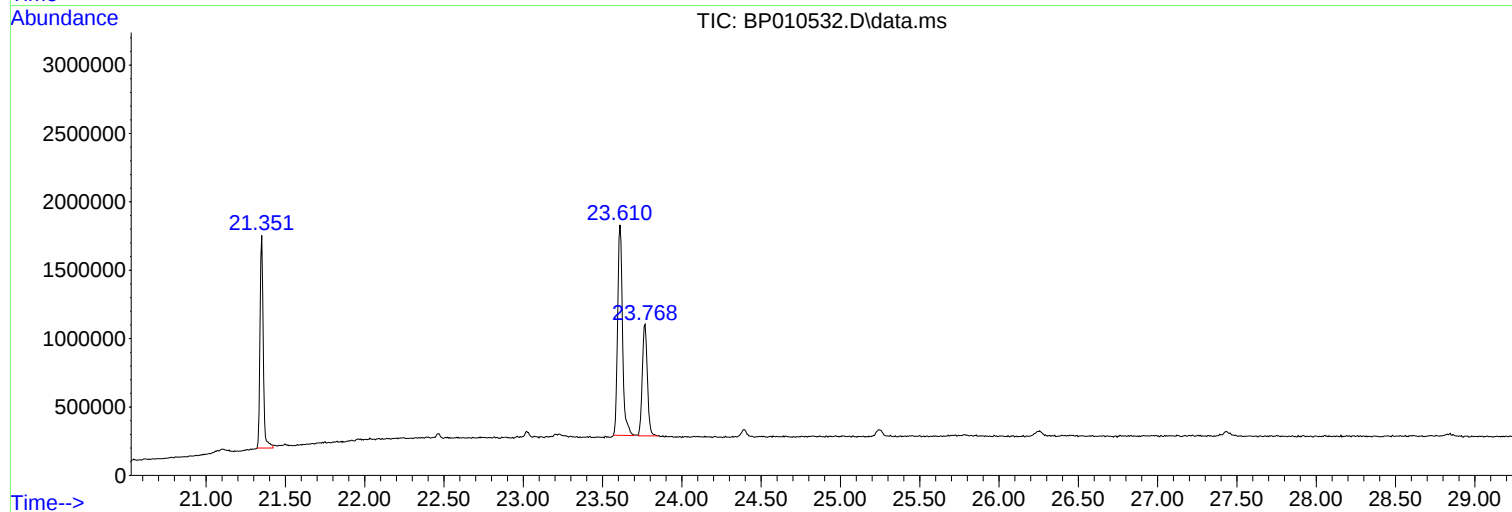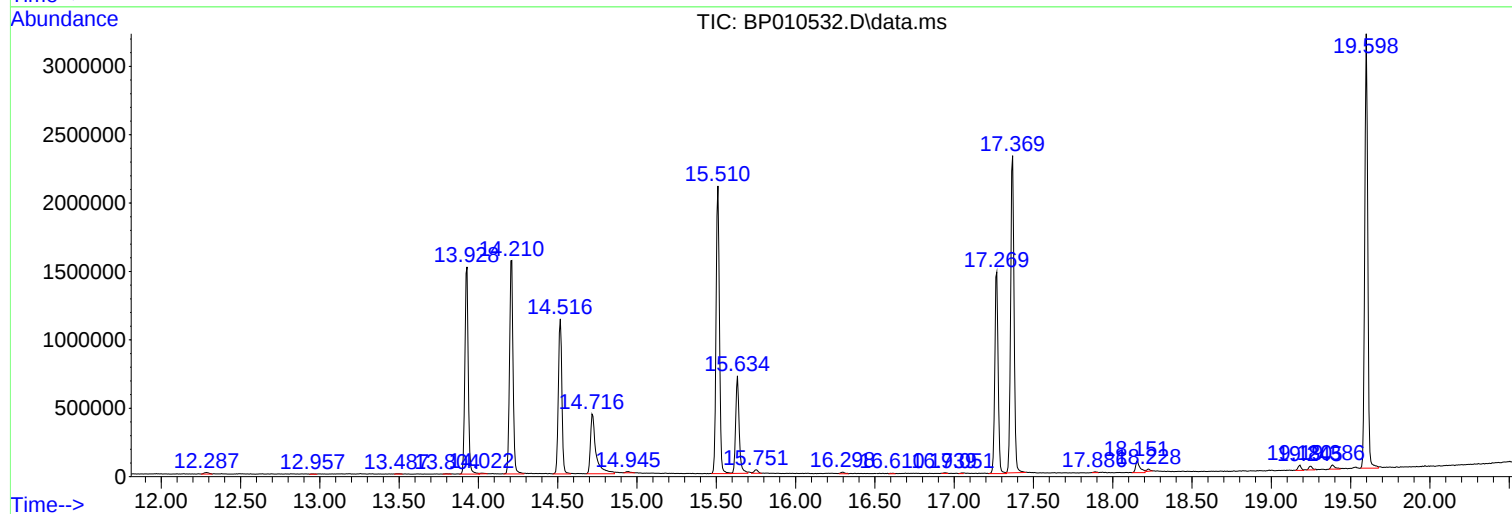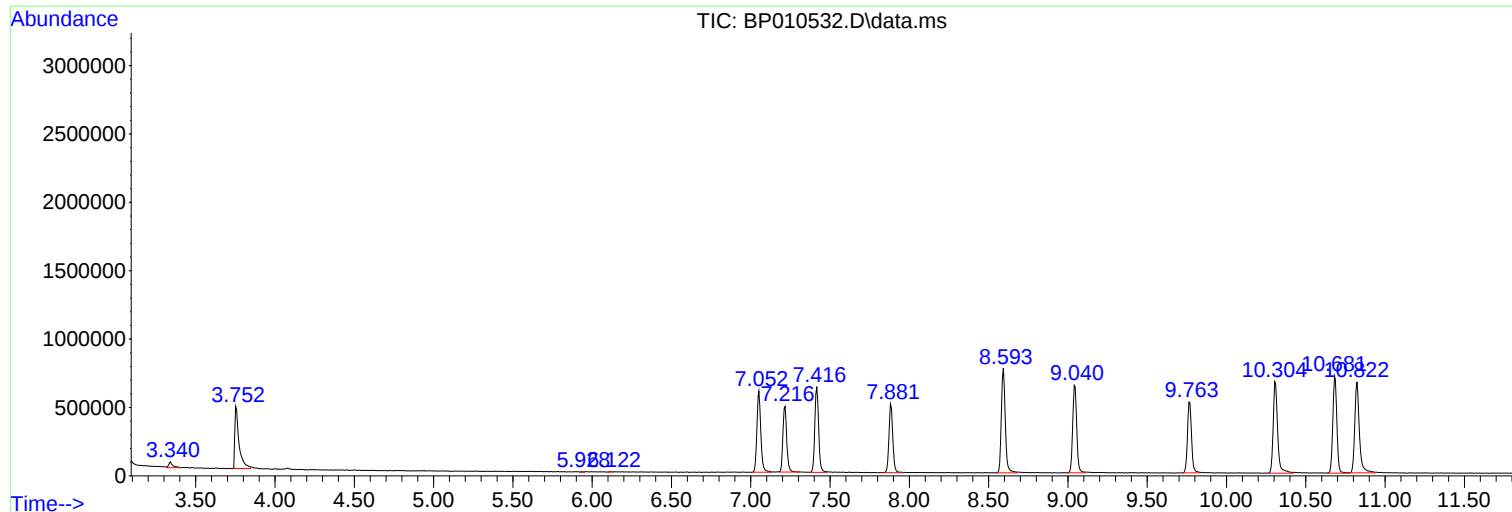

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010532.D
Acq On : 25 May 2022 11:53
Operator : CG/JU
Sample : PB145008BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK008

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010532.D
Acq On : 25 May 2022 11:53
Operator : CG/JU
Sample : PB145008BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK008

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
