

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
 Data File : BP010534.D
 Acq On : 25 May 2022 14:12
 Operator : CG/JU
 Sample : N2918-12DL 20X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTH0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010534.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.075	165	168	174	rVB5	8376	13991	0.65%	0.124%
2	4.122	174	176	180	rBV5	3168	3450	0.16%	0.031%
3	4.864	300	302	308	rBV7	3185	4219	0.20%	0.038%
4	5.011	324	327	332	rBV3	8341	14641	0.68%	0.130%
5	5.899	475	478	482	rVV5	5613	8576	0.40%	0.076%
6	6.328	549	551	554	rVB4	3509	3745	0.17%	0.033%
7	7.058	671	675	676	rBV4	4627	4725	0.22%	0.042%
8	7.216	697	702	710	rBV	26061	48831	2.28%	0.434%
9	7.422	730	737	742	rVV2	24395	44227	2.06%	0.393%
10	7.463	742	744	747	rVV4	3943	4634	0.22%	0.041%
11	7.534	752	756	759	rVV6	4582	6563	0.31%	0.058%
12	7.605	764	768	774	rVB2	11817	17629	0.82%	0.157%
13	7.887	808	816	826	rBV	266354	471085	21.99%	4.190%
14	7.999	832	835	841	rBV6	3110	6331	0.30%	0.056%
15	8.422	902	907	914	rBV6	9506	19899	0.93%	0.177%
16	8.604	932	938	947	rBV3	14469	31805	1.48%	0.283%
17	8.734	954	960	967	rVV3	14182	30075	1.40%	0.268%
18	9.052	1009	1014	1023	rVB2	28197	56081	2.62%	0.499%
19	9.246	1043	1047	1054	rVB8	5352	9454	0.44%	0.084%
20	9.316	1054	1059	1062	rBV7	6067	10742	0.50%	0.096%
21	9.375	1064	1069	1073	rVB6	9869	15575	0.73%	0.139%
22	9.434	1078	1079	1083	rVB4	3880	3535	0.17%	0.031%
23	9.775	1131	1137	1144	rVV2	21592	41074	1.92%	0.365%
24	9.904	1154	1159	1163	rBV8	5812	10741	0.50%	0.096%
25	10.081	1185	1189	1191	rBV5	3077	4055	0.19%	0.036%
26	10.328	1224	1231	1242	rBV6	23686	63725	2.97%	0.567%
27	10.404	1242	1244	1246	rVV3	3343	3624	0.17%	0.032%
28	10.681	1284	1291	1295	rBV	391117	670332	31.29%	5.962%
29	10.734	1295	1300	1310	rVV	1250901	2142046	100.00%	19.052%
30	10.851	1312	1320	1330	rVV2	93257	198586	9.27%	1.766%
31	11.081	1354	1359	1366	rBV10	6306	13034	0.61%	0.116%
32	11.293	1389	1395	1396	rVV6	2406	3613	0.17%	0.032%
33	11.381	1408	1410	1414	rVB5	3648	4031	0.19%	0.036%
34	11.728	1462	1469	1472	rBV9	4077	9407	0.44%	0.084%
35	11.787	1476	1479	1481	rVV4	4939	6533	0.30%	0.058%
36	12.104	1532	1533	1538	rVB5	3207	3749	0.18%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
 Data File : BP010534.D
 Acq On : 25 May 2022 14:12
 Operator : CG/JU
 Sample : N2918-12DL 20X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTH0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	12.240	1551	1556	1561	rBV7	4652	9551	0.45%	0.085%
38	12.345	1567	1574	1588	rBV	111611	205045	9.57%	1.824%
39	12.469	1593	1595	1601	rVB6	5712	6924	0.32%	0.062%
40	12.563	1603	1611	1618	rBV	66308	124107	5.79%	1.104%
41	12.675	1627	1630	1634	rBV6	2278	3417	0.16%	0.030%
42	12.740	1637	1641	1643	rBV5	3536	4026	0.19%	0.036%
43	13.004	1681	1686	1687	rBV5	2822	4009	0.19%	0.036%
44	13.051	1692	1694	1696	rVV3	4257	4147	0.19%	0.037%
45	13.069	1696	1697	1701	rVB4	3956	3572	0.17%	0.032%
46	13.251	1725	1728	1730	rBV4	5574	7187	0.34%	0.064%
47	13.357	1740	1746	1752	rBV2	29367	49593	2.32%	0.441%
48	13.563	1777	1781	1783	rBV5	4636	8111	0.38%	0.072%
49	13.698	1796	1804	1811	rBV7	11135	27572	1.29%	0.245%
50	13.845	1822	1829	1833	rBV4	11843	24297	1.13%	0.216%
51	13.928	1833	1843	1851	rVV	87344	151622	7.08%	1.349%
52	14.010	1854	1857	1861	rVB6	2968	3981	0.19%	0.035%
53	14.075	1864	1868	1873	rBV6	4722	8973	0.42%	0.080%
54	14.210	1885	1891	1904	rBV	85514	152837	7.14%	1.359%
55	14.434	1924	1929	1930	rVB5	2946	3559	0.17%	0.032%
56	14.516	1935	1943	1949	rVV	636366	956608	44.66%	8.508%
57	14.581	1949	1954	1961	rVV2	133266	207772	9.70%	1.848%
58	14.657	1963	1967	1973	rVV	36884	63786	2.98%	0.567%
59	14.798	1986	1991	1995	rBV5	11102	17985	0.84%	0.160%
60	14.875	2000	2004	2006	rBV5	6120	8131	0.38%	0.072%
61	14.916	2006	2011	2023	rVB	98220	163688	7.64%	1.456%
62	15.081	2032	2039	2044	rBV	7546	16053	0.75%	0.143%
63	15.122	2044	2046	2051	rVV6	4342	7670	0.36%	0.068%
64	15.510	2105	2112	2117	rVV	136186	205999	9.62%	1.832%
65	15.569	2117	2122	2129	rVB	87010	144548	6.75%	1.286%
66	15.651	2129	2136	2148	rBV9	18924	57888	2.70%	0.515%
67	15.816	2160	2164	2169	rVB8	4847	8547	0.40%	0.076%
68	15.869	2169	2173	2180	rVB8	8926	14707	0.69%	0.131%
69	16.010	2191	2197	2208	rVV8	8271	24560	1.15%	0.218%
70	16.175	2221	2225	2231	rVB9	7112	10157	0.47%	0.090%
71	16.239	2231	2236	2243	rBV10	7623	16116	0.75%	0.143%
72	16.392	2258	2262	2265	rBV5	11190	14609	0.68%	0.130%
73	16.457	2269	2273	2281	rVV7	7106	12743	0.59%	0.113%
74	16.533	2282	2286	2294	rVV2	13313	29723	1.39%	0.264%
75	16.628	2298	2302	2304	rVV5	2796	3453	0.16%	0.031%
76	16.645	2304	2305	2311	rVV6	3493	5185	0.24%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
 Data File : BP010534.D
 Acq On : 25 May 2022 14:12
 Operator : CG/JU
 Sample : N2918-12DL 20X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTH0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

77	16.816	2331	2334	2336	rVB4	3610	3527	0.16%	0.031%
78	16.933	2348	2354	2360	rBV3	16621	29878	1.39%	0.266%
79	17.092	2377	2381	2385	rVB3	9783	14953	0.70%	0.133%
80	17.192	2392	2398	2402	rBV8	7082	12258	0.57%	0.109%
81	17.269	2402	2411	2416	rBV	793493	1199600	56.00%	10.670%
82	17.310	2416	2418	2423	rVV	116976	155451	7.26%	1.383%
83	17.369	2423	2428	2441	rVV	133867	247669	11.56%	2.203%
84	17.475	2445	2446	2450	rVV4	3242	3829	0.18%	0.034%
85	17.522	2452	2454	2458	rVB5	3470	4209	0.20%	0.037%
86	17.675	2470	2480	2488	rBV	199489	328612	15.34%	2.923%
87	17.845	2504	2509	2514	rBV3	13834	25031	1.17%	0.223%
88	17.886	2514	2516	2520	rVV5	4481	5814	0.27%	0.052%
89	17.939	2521	2525	2529	rVB6	12866	16025	0.75%	0.143%
90	18.104	2551	2553	2557	rBV5	4397	4242	0.20%	0.038%
91	18.157	2557	2562	2571	rBV3	48994	110160	5.14%	0.980%
92	18.222	2571	2573	2577	rVV4	6083	9631	0.45%	0.086%
93	18.328	2586	2591	2595	rBV7	6884	10233	0.48%	0.091%
94	18.422	2603	2607	2609	rBV4	6740	10295	0.48%	0.092%
95	18.710	2653	2656	2659	rBV5	4971	7285	0.34%	0.065%
96	18.980	2700	2702	2705	rBV4	4188	3794	0.18%	0.034%
97	19.386	2767	2771	2778	rBV9	20973	39089	1.82%	0.348%
98	19.604	2803	2808	2813	rBV	178618	255994	11.95%	2.277%
99	21.351	3100	3105	3114	rBV	759740	1110979	51.87%	9.882%
100	23.768	3510	3516	3529	rVB2	372531	837590	39.10%	7.450%




Sum of corrected areas: 11242969

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010534.D
Acq On : 25 May 2022 14:12
Operator : CG/JU
Sample : N2918-12DL 20X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTH0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

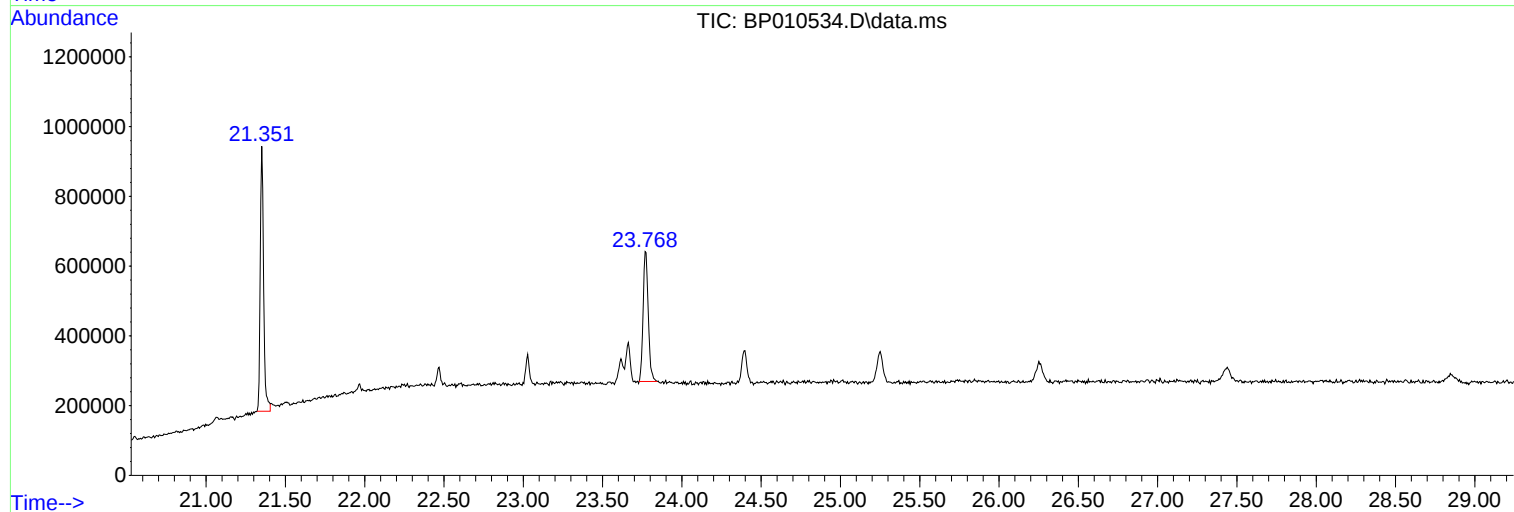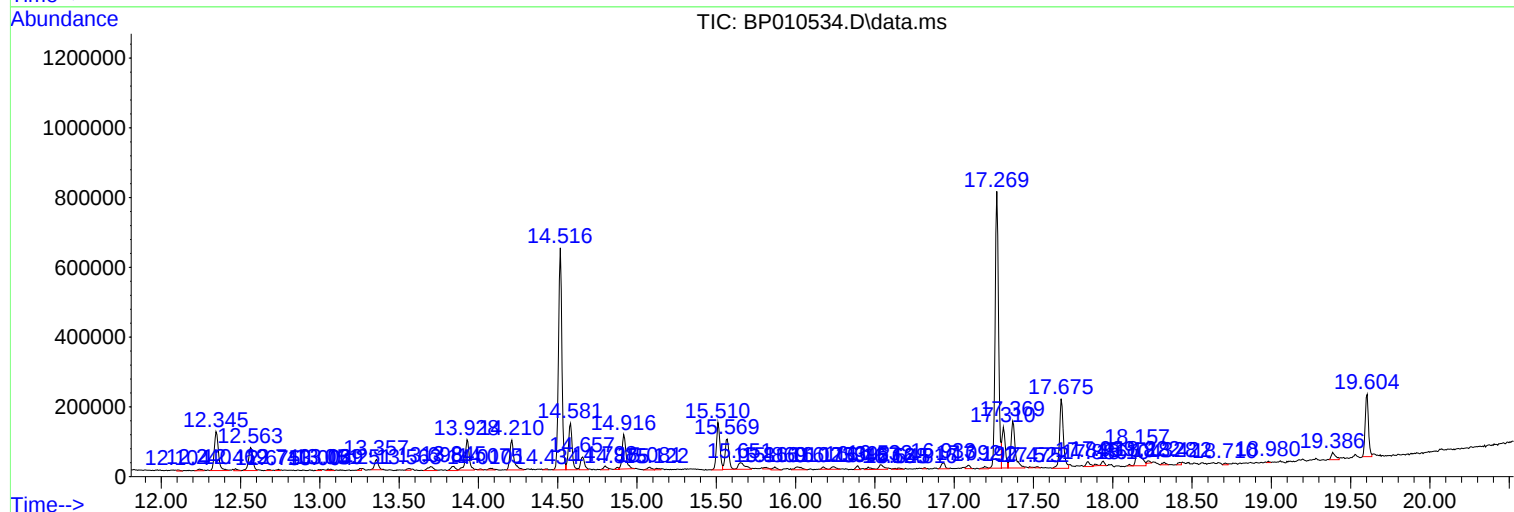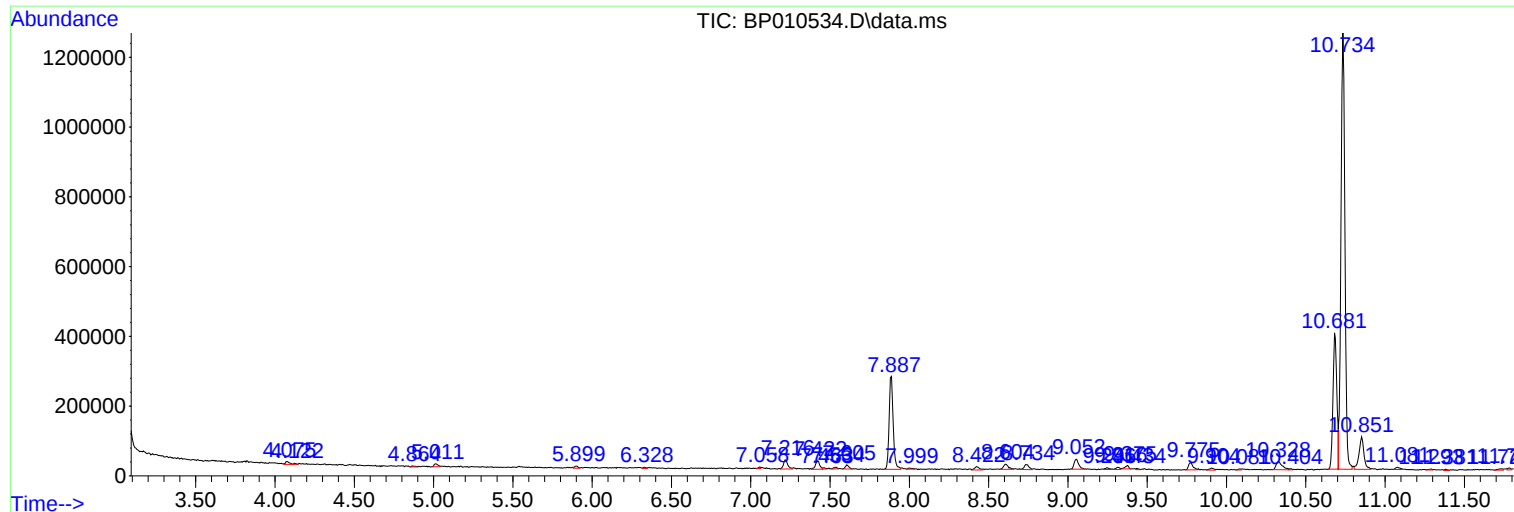

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010534.D
Acq On : 25 May 2022 14:12
Operator : CG/JU
Sample : N2918-12DL 20X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTH0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010534.D
Acq On : 25 May 2022 14:12
Operator : CG/JU
Sample : N2918-12DL 20X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTH0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc