

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
 Data File : BP010543.D
 Acq On : 25 May 2022 19:16
 Operator : CG/JU
 Sample : N2950-15DL2 25X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE2DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010543.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.075	164	168	172	rVB4	7177	9962	0.34%	0.066%
2	4.187	185	187	189	rBV2	3184	3280	0.11%	0.022%
3	5.522	411	414	417	rBV5	1941	2940	0.10%	0.019%
4	7.058	673	675	679	rBV5	3155	4010	0.14%	0.026%
5	7.216	696	702	708	rBV	18182	33690	1.16%	0.222%
6	7.416	731	736	746	rBV2	14610	30084	1.04%	0.199%
7	7.534	751	756	760	rBV5	3841	6739	0.23%	0.044%
8	7.599	765	767	774	rVV8	4902	8581	0.30%	0.057%
9	7.658	775	777	785	rVB8	1604	3535	0.12%	0.023%
10	7.881	809	815	828	rBV	409679	706078	24.35%	4.661%
11	8.263	875	880	883	rBV7	2863	3816	0.13%	0.025%
12	8.422	901	907	914	rVV	26752	52238	1.80%	0.345%
13	8.610	934	939	943	rBV5	7936	15374	0.53%	0.101%
14	8.999	1001	1005	1006	rVV4	2550	3287	0.11%	0.022%
15	9.058	1009	1015	1024	rVV2	20121	49530	1.71%	0.327%
16	9.246	1043	1047	1048	rBV4	4778	6506	0.22%	0.043%
17	9.375	1059	1069	1075	rBV7	9062	22556	0.78%	0.149%
18	9.434	1075	1079	1085	rVB7	2918	5421	0.19%	0.036%
19	9.693	1118	1123	1126	rBV6	3040	4423	0.15%	0.029%
20	9.775	1130	1137	1142	rVV5	15236	30803	1.06%	0.203%
21	9.834	1146	1147	1151	rVV4	2904	3173	0.11%	0.021%
22	9.934	1160	1164	1169	rBV8	3202	5752	0.20%	0.038%
23	10.099	1185	1192	1193	rBV6	5159	7550	0.26%	0.050%
24	10.193	1205	1208	1212	rBV6	2285	3685	0.13%	0.024%
25	10.328	1225	1231	1239	rBV5	14337	35156	1.21%	0.232%
26	10.681	1283	1291	1295	rBV	605163	1047776	36.14%	6.916%
27	10.734	1295	1300	1312	rVV	1671652	2899235	100.00%	19.138%
28	10.852	1313	1320	1334	rVB	105242	214563	7.40%	1.416%
29	11.069	1354	1357	1361	rVB4	3445	4820	0.17%	0.032%
30	11.799	1479	1481	1485	rVB6	2458	3268	0.11%	0.022%
31	11.975	1509	1511	1515	rVB4	2914	3109	0.11%	0.021%
32	12.240	1551	1556	1559	rBV5	7332	12359	0.43%	0.082%
33	12.346	1567	1574	1586	rBV	139242	266165	9.18%	1.757%
34	12.463	1589	1594	1599	rVB6	4903	9752	0.34%	0.064%
35	12.563	1601	1611	1619	rBV	127699	229957	7.93%	1.518%
36	12.998	1682	1685	1690	rVV6	4783	7565	0.26%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
 Data File : BP010543.D
 Acq On : 25 May 2022 19:16
 Operator : CG/JU
 Sample : N2950-15DL2 25X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE2DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	13.034	1690	1691	1697	rVB6	2316	3246	0.11%	0.021%
38	13.357	1737	1746	1753	rBV2	39429	70623	2.44%	0.466%
39	13.498	1766	1770	1774	rBV7	1850	3857	0.13%	0.025%
40	13.557	1776	1780	1782	rVV3	5972	9776	0.34%	0.065%

41	13.581	1782	1784	1792	rVB7	4962	7850	0.27%	0.052%
42	13.698	1798	1804	1812	rVB8	13579	28380	0.98%	0.187%
43	13.840	1822	1828	1833	rBV3	11483	18518	0.64%	0.122%
44	13.898	1833	1838	1839	rBV5	5969	8055	0.28%	0.053%
45	13.928	1839	1843	1851	rVB	60690	96930	3.34%	0.640%

46	14.081	1863	1869	1871	rBV7	3769	6679	0.23%	0.044%
47	14.104	1871	1873	1879	rVB7	3226	3951	0.14%	0.026%
48	14.210	1884	1891	1903	rBV2	64468	126319	4.36%	0.834%
49	14.516	1935	1943	1949	rBV	953254	1467047	50.60%	9.684%
50	14.581	1949	1954	1962	rVV	219073	361656	12.47%	2.387%

51	14.657	1962	1967	1982	rVB	54256	111057	3.83%	0.733%
52	14.828	1989	1996	1999	rBV9	2653	5326	0.18%	0.035%
53	14.916	2004	2011	2015	rBV	77227	126729	4.37%	0.837%
54	14.951	2015	2017	2031	rVV	25294	50235	1.73%	0.332%
55	15.081	2035	2039	2045	rVB8	5462	10633	0.37%	0.070%

56	15.510	2107	2112	2117	rVV	103256	153102	5.28%	1.011%
57	15.563	2117	2121	2131	rVB2	71689	120312	4.15%	0.794%
58	15.657	2133	2137	2140	rBV5	9633	18149	0.63%	0.120%
59	15.822	2162	2165	2170	rVB7	3188	4931	0.17%	0.033%
60	15.881	2170	2175	2180	rBV9	3432	6280	0.22%	0.041%

61	16.010	2194	2197	2202	rVV7	5127	9226	0.32%	0.061%
62	16.245	2232	2237	2241	rBV7	6018	8316	0.29%	0.055%
63	16.545	2286	2288	2291	rBV4	3378	4202	0.14%	0.028%
64	16.575	2291	2293	2295	rVB3	3829	3249	0.11%	0.021%
65	16.934	2348	2354	2359	rVV9	13563	24771	0.85%	0.164%

66	17.057	2372	2375	2376	rVV3	3793	3051	0.11%	0.020%
67	17.086	2376	2380	2385	rVB3	4054	6048	0.21%	0.040%
68	17.169	2391	2394	2395	rBV3	2659	2933	0.10%	0.019%
69	17.269	2401	2411	2417	rBV	1200107	1891412	65.24%	12.485%
70	17.369	2422	2428	2439	rVB2	96335	180111	6.21%	1.189%

71	17.675	2472	2480	2493	rBV	170804	302322	10.43%	1.996%
72	18.104	2550	2553	2557	rBV6	4064	6307	0.22%	0.042%
73	18.157	2557	2562	2566	rBV6	19543	40344	1.39%	0.266%
74	18.563	2628	2631	2636	rBV7	5123	6507	0.22%	0.043%
75	19.386	2768	2771	2775	rBV6	9518	15586	0.54%	0.103%

76	19.598	2802	2807	2818	rBV	133984	208084	7.18%	1.374%
----	--------	------	------	------	-----	--------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010543.D
Acq On : 25 May 2022 19:16
Operator : CG/JU
Sample : N2950-15DL2 25X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE2DL2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Title : SVOA CALIBRATION

77	21.345	3099	3104	3118	rBV	1420396	2132311	73.55%	14.075%
78	23.768	3509	3516	3528	rVB	783649	1728006	59.60%	11.407%




Sum of corrected areas: 15149165

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010543.D
Acq On : 25 May 2022 19:16
Operator : CG/JU
Sample : N2950-15DL2 25X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE2DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

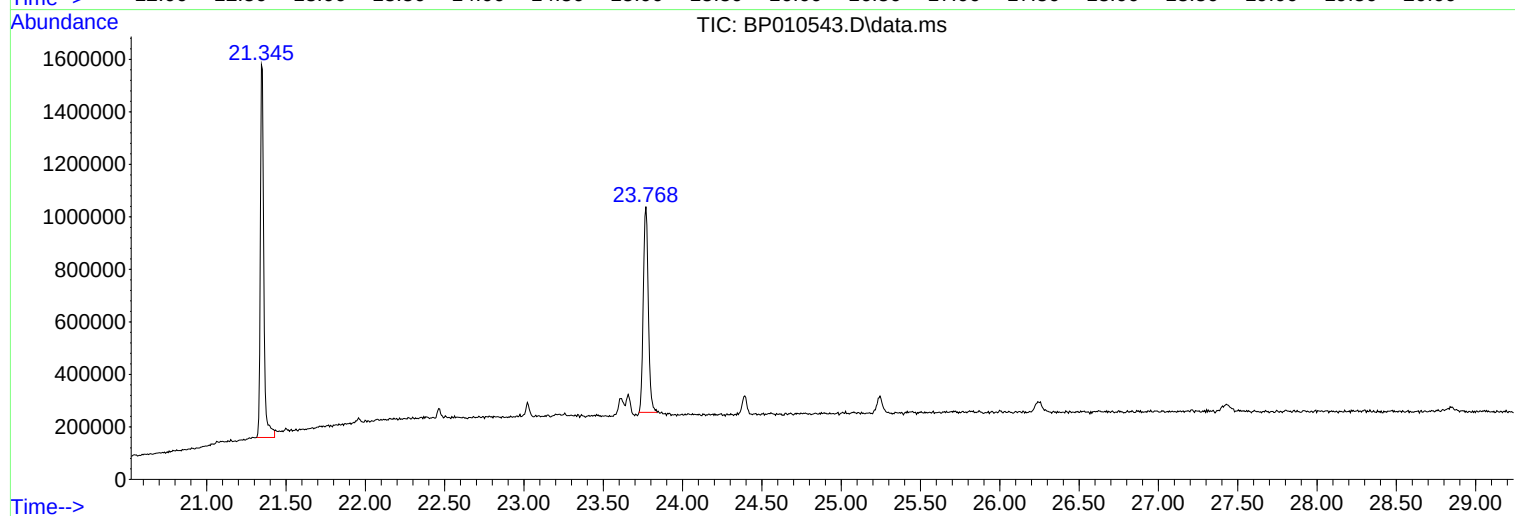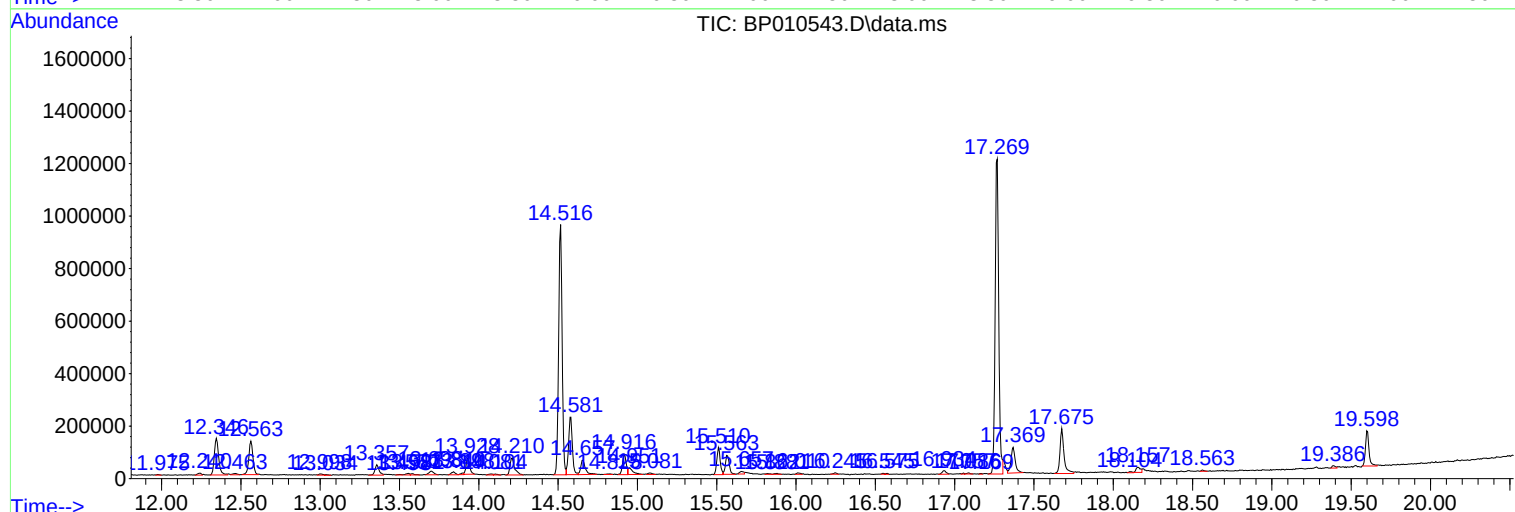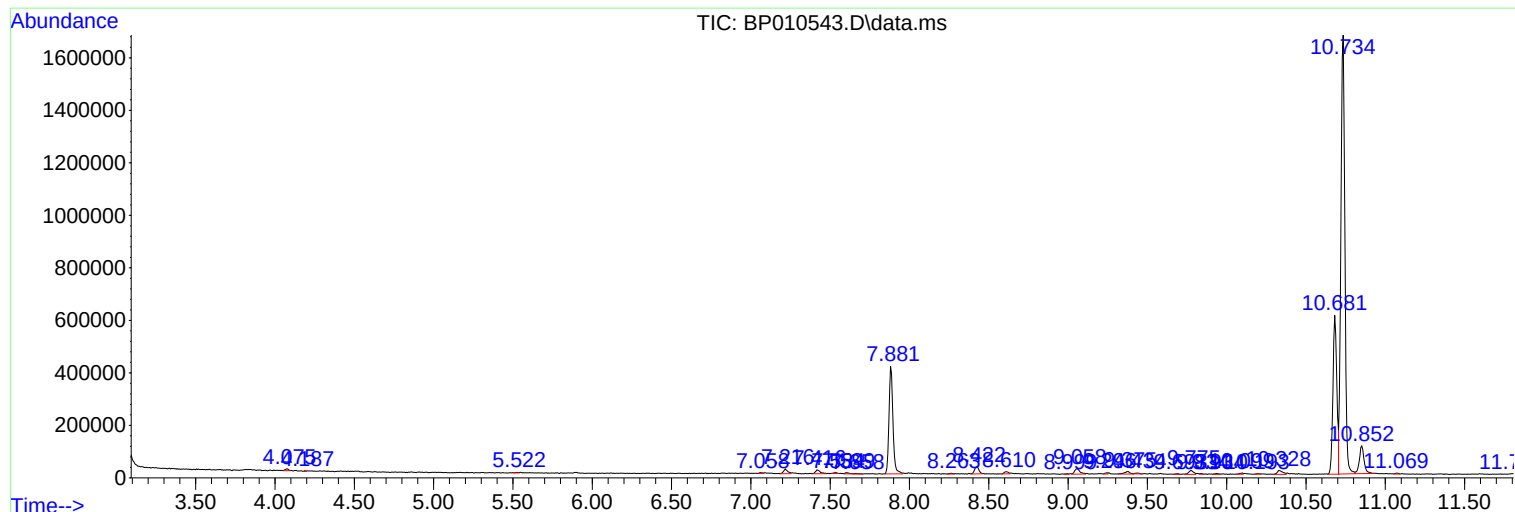

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010543.D
Acq On : 25 May 2022 19:16
Operator : CG/JU
Sample : N2950-15DL2 25X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE2DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010543.D
Acq On : 25 May 2022 19:16
Operator : CG/JU
Sample : N2950-15DL2 25X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE2DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------