

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
 Data File : BP010548.D
 Acq On : 25 May 2022 22:05
 Operator : CG/JU
 Sample : N2950-05DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTF1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010548.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.799	118	121	126	rBV4	8157	14828	0.58%	0.082%
2	3.981	149	152	154	rBV4	4044	4914	0.19%	0.027%
3	4.075	165	168	173	rVB2	9647	14399	0.57%	0.080%
4	5.528	412	415	418	rBV5	2081	2957	0.12%	0.016%
5	5.899	474	478	483	rVB3	5968	9080	0.36%	0.050%
6	6.569	590	592	596	rBV5	2155	2687	0.11%	0.015%
7	7.064	670	676	682	rBV5	8091	18614	0.73%	0.103%
8	7.216	697	702	715	rBV	46827	93378	3.68%	0.517%
9	7.422	730	737	747	rBV	39750	75385	2.97%	0.417%
10	7.540	755	757	761	rVB5	3118	3452	0.14%	0.019%
11	7.605	761	768	773	rBV2	18873	33422	1.32%	0.185%
12	7.881	807	815	827	rBV	536251	911439	35.94%	5.044%
13	7.963	827	829	832	rVV4	4547	5453	0.22%	0.030%
14	7.999	834	835	839	rVB4	3685	3789	0.15%	0.021%
15	8.205	863	870	871	rBV6	1965	3378	0.13%	0.019%
16	8.258	876	879	886	rVB9	2293	5338	0.21%	0.030%
17	8.422	902	907	912	rBV3	19740	33415	1.32%	0.185%
18	8.599	931	937	947	rBV3	27176	56549	2.23%	0.313%
19	8.740	955	961	970	rVB3	21861	38735	1.53%	0.214%
20	9.052	1007	1014	1023	rVV	55083	113860	4.49%	0.630%
21	9.193	1034	1038	1042	rBV7	2235	3511	0.14%	0.019%
22	9.240	1044	1046	1052	rVV7	5422	7769	0.31%	0.043%
23	9.305	1054	1057	1059	rBV4	2693	3048	0.12%	0.017%
24	9.369	1062	1068	1074	rVV6	11635	27767	1.10%	0.154%
25	9.440	1074	1080	1083	rVV7	4637	9691	0.38%	0.054%
26	9.469	1083	1085	1091	rVV7	3175	4893	0.19%	0.027%
27	9.522	1091	1094	1098	rVB6	2000	2869	0.11%	0.016%
28	9.769	1129	1136	1150	rBV2	40215	84248	3.32%	0.466%
29	10.093	1186	1191	1195	rBV7	3618	4680	0.18%	0.026%
30	10.181	1203	1206	1209	rBV4	3123	3523	0.14%	0.019%
31	10.322	1224	1230	1244	rBV2	45098	113116	4.46%	0.626%
32	10.446	1248	1251	1257	rVB8	2325	4100	0.16%	0.023%
33	10.610	1276	1279	1282	rBV4	2502	3544	0.14%	0.020%
34	10.681	1283	1291	1295	rVV	746433	1299393	51.24%	7.191%
35	10.734	1295	1300	1311	rVV	1478293	2535798	100.00%	14.033%
36	10.852	1311	1320	1335	rVB2	121578	293548	11.58%	1.624%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
 Data File : BP010548.D
 Acq On : 25 May 2022 22:05
 Operator : CG/JU
 Sample : N2950-05DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTF1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	11.075	1353	1358	1366	rVB2	5256	11111	0.44%	0.061%
38	11.387	1409	1411	1416	rVV6	2737	3652	0.14%	0.020%
39	11.463	1419	1424	1426	rBV6	1387	2813	0.11%	0.016%
40	11.663	1452	1458	1460	rVB7	2050	3782	0.15%	0.021%

41	11.728	1464	1469	1470	rBV5	3138	4022	0.16%	0.022%
42	11.793	1477	1480	1484	rVB6	4030	5210	0.21%	0.029%
43	12.240	1550	1556	1558	rBV3	6680	9647	0.38%	0.053%
44	12.346	1568	1574	1585	rVV	125553	218514	8.62%	1.209%
45	12.463	1590	1594	1601	rVB8	5104	9286	0.37%	0.051%

46	12.563	1601	1611	1619	rBV	77285	138542	5.46%	0.767%
47	12.681	1627	1631	1634	rBV5	2671	2786	0.11%	0.015%
48	12.740	1636	1641	1644	rBV7	4413	8961	0.35%	0.050%
49	12.857	1658	1661	1665	rBV6	1755	2678	0.11%	0.015%
50	12.999	1678	1685	1691	rBV6	4113	10500	0.41%	0.058%

51	13.051	1691	1694	1696	rBV4	2233	2863	0.11%	0.016%
52	13.257	1723	1729	1731	rBV6	4707	8895	0.35%	0.049%
53	13.357	1741	1746	1754	rVB	41914	71310	2.81%	0.395%
54	13.551	1776	1779	1781	rVV4	5223	6192	0.24%	0.034%
55	13.569	1781	1782	1786	rVB4	4198	4468	0.18%	0.025%

56	13.698	1796	1804	1811	rBV6	14111	36167	1.43%	0.200%
57	13.834	1821	1827	1833	rBV4	13202	24949	0.98%	0.138%
58	13.928	1833	1843	1854	rVV	166998	265355	10.46%	1.468%
59	14.075	1862	1868	1872	rVB8	5489	10540	0.42%	0.058%
60	14.110	1872	1874	1877	rVB4	3231	3029	0.12%	0.017%

61	14.204	1884	1890	1909	rBV	165349	284075	11.20%	1.572%
62	14.381	1916	1920	1922	rBV5	2608	3343	0.13%	0.018%
63	14.516	1936	1943	1949	rBV	1168026	1816611	71.64%	10.053%
64	14.575	1949	1953	1961	rVV	127325	205292	8.10%	1.136%
65	14.651	1961	1966	1976	rVB	49744	84772	3.34%	0.469%

66	14.798	1985	1991	1997	rBV4	13364	28196	1.11%	0.156%
67	14.916	2005	2011	2023	rVB	127076	212886	8.40%	1.178%
68	15.069	2029	2037	2044	rBV4	27174	52353	2.06%	0.290%
69	15.151	2048	2051	2062	rVB9	11384	21464	0.85%	0.119%
70	15.457	2098	2103	2105	rBV5	2556	3251	0.13%	0.018%

71	15.510	2105	2112	2117	rBV	244445	360402	14.21%	1.994%
72	15.569	2117	2122	2129	rVV2	100344	166123	6.55%	0.919%
73	15.640	2129	2134	2147	rVB3	35488	88641	3.50%	0.491%
74	15.751	2150	2153	2157	rVB5	5369	5974	0.24%	0.033%
75	15.792	2157	2160	2161	rBV3	2767	3133	0.12%	0.017%

76	15.863	2168	2172	2179	rVB6	9292	17077	0.67%	0.095%
----	--------	------	------	------	------	------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
 Data File : BP010548.D
 Acq On : 25 May 2022 22:05
 Operator : CG/JU
 Sample : N2950-05DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTF1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

77	16.010	2192	2197	2200	rBV7	7405	11422	0.45%	0.063%
78	16.245	2230	2237	2242	rVV7	14726	31286	1.23%	0.173%
79	16.298	2242	2246	2249	rVB3	7140	8319	0.33%	0.046%
80	16.457	2271	2273	2279	rVB5	6159	8503	0.34%	0.047%
81	16.534	2279	2286	2296	rBV2	25999	57257	2.26%	0.317%
82	16.922	2341	2352	2364	rBV3	60196	120860	4.77%	0.669%
83	17.034	2367	2371	2372	rBV4	4761	5618	0.22%	0.031%
84	17.087	2376	2380	2383	rVB4	10306	14916	0.59%	0.083%
85	17.175	2391	2395	2399	rVB7	2997	5219	0.21%	0.029%
86	17.269	2400	2411	2415	rBV	1512848	2273049	89.64%	12.579%
87	17.304	2415	2417	2422	rVV	107539	162611	6.41%	0.900%
88	17.369	2422	2428	2440	rVB	261075	435707	17.18%	2.411%
89	17.522	2451	2454	2458	rVB6	5177	7484	0.30%	0.041%
90	17.675	2471	2480	2489	rBV	226719	375812	14.82%	2.080%
91	17.769	2493	2496	2502	rBV8	5683	8874	0.35%	0.049%
92	17.839	2502	2508	2514	rBV3	24235	50204	1.98%	0.278%
93	17.981	2529	2532	2535	rVB5	5153	6195	0.24%	0.034%
94	18.151	2557	2561	2564	rBV5	21327	33865	1.34%	0.187%
95	18.386	2599	2601	2602	rBV2	2987	2910	0.11%	0.016%
96	19.386	2767	2771	2776	rBV6	13663	25859	1.02%	0.143%
97	19.598	2801	2807	2814	rBV	365097	496700	19.59%	2.749%
98	21.351	3099	3105	3112	rBV	1515351	2131370	84.05%	11.795%
99	23.610	3486	3489	3493	rVB2	85182	112802	4.45%	0.624%
100	23.763	3509	3515	3527	rVB2	747865	1618099	63.81%	8.954%



Sum of corrected areas: 18070376

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010548.D
Acq On : 25 May 2022 22:05
Operator : CG/JU
Sample : N2950-05DL 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTF1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

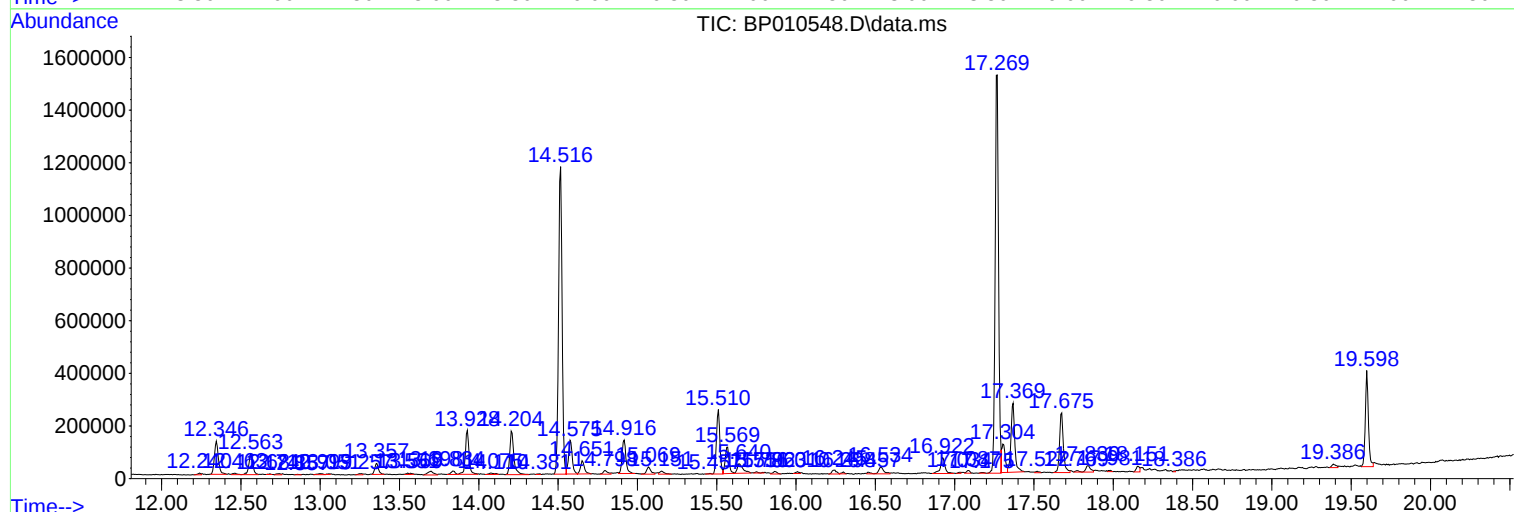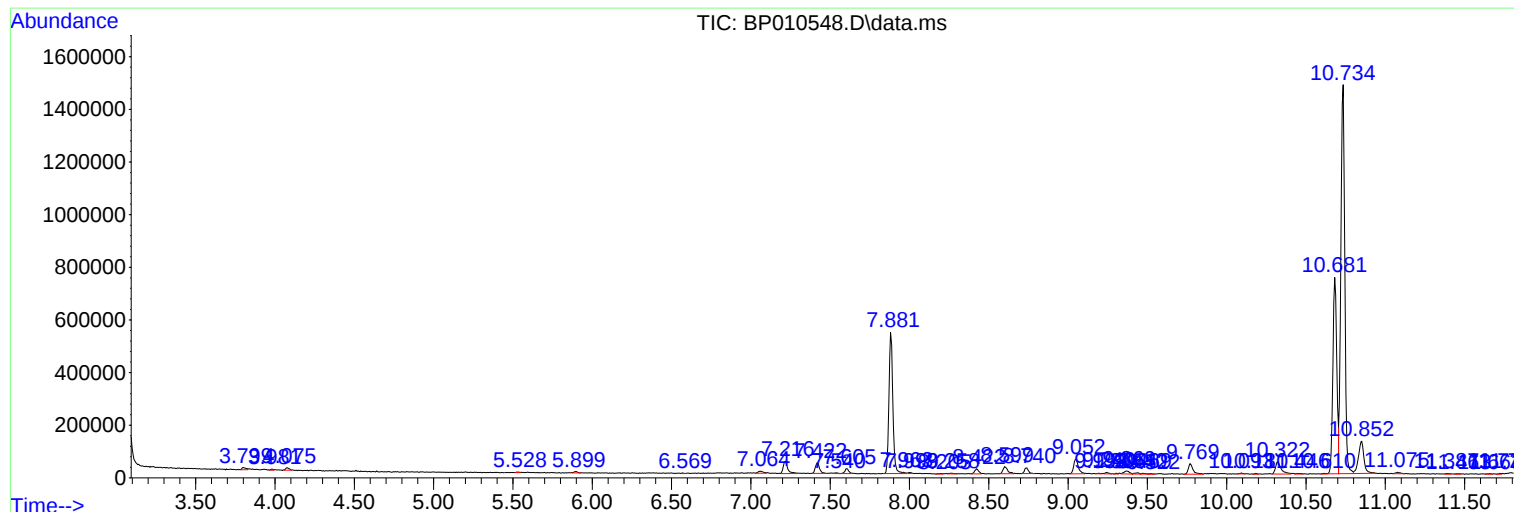

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010548.D
Acq On : 25 May 2022 22:05
Operator : CG/JU
Sample : N2950-05DL 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTF1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010548.D
Acq On : 25 May 2022 22:05
Operator : CG/JU
Sample : N2950-05DL 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTF1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------