

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
 Data File : BP010556.D
 Acq On : 26 May 2022 02:35
 Operator : CG/JU
 Sample : N2950-09DL 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTH2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010556.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.793	118	120	128	rBV6	8961	20139	0.79%	0.107%
2	4.075	165	168	172	rVB2	9790	11728	0.46%	0.062%
3	5.899	475	478	479	rBV3	4231	3455	0.14%	0.018%
4	7.058	672	675	676	rBV3	5401	5603	0.22%	0.030%
5	7.216	696	702	710	rBV	46076	80069	3.15%	0.424%
6	7.416	730	736	745	rBV2	36702	70924	2.79%	0.376%
7	7.605	760	768	778	rVB5	21163	44316	1.74%	0.235%
8	7.881	806	815	826	rBV	520717	882356	34.68%	4.673%
9	7.999	831	835	839	rVB6	3476	6298	0.25%	0.033%
10	8.369	895	898	901	rBV5	2356	4085	0.16%	0.022%
11	8.422	901	907	913	rVV2	17083	32541	1.28%	0.172%
12	8.599	932	937	944	rBV3	25200	48994	1.93%	0.259%
13	8.734	954	960	967	rBV	20281	37276	1.47%	0.197%
14	9.046	1006	1013	1022	rBV	53026	108105	4.25%	0.573%
15	9.181	1032	1036	1041	rBV8	8333	16086	0.63%	0.085%
16	9.310	1056	1058	1060	rBV3	2975	3020	0.12%	0.016%
17	9.369	1062	1068	1073	rVV6	9663	17894	0.70%	0.095%
18	9.440	1075	1080	1081	rBV4	4662	5026	0.20%	0.027%
19	9.640	1109	1114	1118	rBV7	1903	3350	0.13%	0.018%
20	9.769	1128	1136	1142	rBV2	37028	70688	2.78%	0.374%
21	10.093	1185	1191	1195	rBV7	3812	7486	0.29%	0.040%
22	10.322	1224	1230	1241	rBV2	42658	106641	4.19%	0.565%
23	10.681	1282	1291	1295	rBV	749949	1307925	51.41%	6.927%
24	10.728	1295	1299	1311	rVV	1419737	2453663	96.44%	12.995%
25	10.852	1312	1320	1334	rVV2	124160	285338	11.22%	1.511%
26	10.963	1337	1339	1342	rBV4	2507	2941	0.12%	0.016%
27	11.081	1353	1359	1363	rVB9	5288	10434	0.41%	0.055%
28	11.716	1463	1467	1468	rBV4	2842	3306	0.13%	0.018%
29	11.787	1473	1479	1481	rBV7	4504	7765	0.31%	0.041%
30	12.234	1549	1555	1560	rBV7	7054	13110	0.52%	0.069%
31	12.346	1566	1574	1584	rBV	123699	217279	8.54%	1.151%
32	12.446	1588	1591	1592	rBV2	3164	3442	0.14%	0.018%
33	12.563	1602	1611	1620	rVB	75134	135201	5.31%	0.716%
34	12.687	1624	1632	1633	rBV8	2703	4438	0.17%	0.024%
35	12.746	1636	1642	1644	rBV7	4021	6539	0.26%	0.035%
36	12.993	1681	1684	1685	rBV3	2735	3328	0.13%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
 Data File : BP010556.D
 Acq On : 26 May 2022 02:35
 Operator : CG/JU
 Sample : N2950-09DL 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTH2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	13.022	1687	1689	1693	rVV4	2523	3079	0.12%	0.016%
38	13.063	1693	1696	1699	rVB5	2858	3499	0.14%	0.019%
39	13.251	1722	1728	1730	rBV7	4703	8076	0.32%	0.043%
40	13.316	1736	1739	1741	rBV4	2311	3334	0.13%	0.018%
41	13.351	1741	1745	1753	rVV	42678	72121	2.83%	0.382%
42	13.498	1765	1770	1771	rBV5	1896	2977	0.12%	0.016%
43	13.557	1775	1780	1782	rBV6	4330	5824	0.23%	0.031%
44	13.698	1795	1804	1810	rBV10	13710	31019	1.22%	0.164%
45	13.834	1820	1827	1831	rBV7	12924	22714	0.89%	0.120%
46	13.893	1833	1837	1838	rVV4	7447	7536	0.30%	0.040%
47	13.922	1838	1842	1852	rVB	157258	246615	9.69%	1.306%
48	14.075	1864	1868	1871	rBV5	6153	7830	0.31%	0.041%
49	14.204	1883	1890	1903	rBV	162646	272797	10.72%	1.445%
50	14.510	1936	1942	1949	rBV	1214733	1845124	72.52%	9.772%
51	14.575	1949	1953	1960	rVV	126057	196076	7.71%	1.038%
52	14.651	1961	1966	1973	rVB	44727	72210	2.84%	0.382%
53	14.798	1985	1991	1995	rBV6	13147	27016	1.06%	0.143%
54	14.869	2000	2003	2004	rVV3	4223	4992	0.20%	0.026%
55	14.916	2006	2011	2023	rVB	128770	214577	8.43%	1.136%
56	15.069	2031	2037	2044	rBV6	29987	57393	2.26%	0.304%
57	15.151	2048	2051	2059	rVV9	11978	24116	0.95%	0.128%
58	15.440	2097	2100	2105	rBV5	2437	4873	0.19%	0.026%
59	15.510	2105	2112	2117	rBV	223762	354744	13.94%	1.879%
60	15.563	2117	2121	2129	rVB	105638	155740	6.12%	0.825%
61	15.645	2129	2135	2141	rBV4	35917	82073	3.23%	0.435%
62	15.745	2150	2152	2157	rVB5	4647	5000	0.20%	0.026%
63	15.787	2157	2159	2164	rVB6	3439	4602	0.18%	0.024%
64	15.863	2169	2172	2176	rVB5	7581	10922	0.43%	0.058%
65	16.004	2193	2196	2198	rBV3	9137	9610	0.38%	0.051%
66	16.240	2230	2236	2242	rBV5	13411	22478	0.88%	0.119%
67	16.457	2268	2273	2278	rBV7	5656	11753	0.46%	0.062%
68	16.534	2281	2286	2298	rVV	26792	54933	2.16%	0.291%
69	16.757	2321	2324	2327	rBV5	2605	4648	0.18%	0.025%
70	16.787	2327	2329	2332	rBV4	3134	3899	0.15%	0.021%
71	16.863	2339	2342	2343	rBV3	4958	4142	0.16%	0.022%
72	16.887	2343	2346	2347	rVV3	9939	10342	0.41%	0.055%
73	16.922	2347	2352	2360	rVB2	65041	112120	4.41%	0.594%
74	17.045	2370	2373	2375	rBV4	3180	3924	0.15%	0.021%
75	17.087	2376	2380	2387	rVB3	9908	15125	0.59%	0.080%
76	17.263	2400	2410	2415	rBV	1597283	2343874	92.13%	12.414%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
 Data File : BP010556.D
 Acq On : 26 May 2022 02:35
 Operator : CG/JU
 Sample : N2950-09DL 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTH2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

77	17.304	2415	2417	2422	rVV	116909	166355	6.54%	0.881%
78	17.363	2422	2427	2442	rVB2	277127	451194	17.73%	2.390%
79	17.522	2451	2454	2458	rVB6	3534	4605	0.18%	0.024%
80	17.669	2471	2479	2489	rBV	253499	405843	15.95%	2.149%
81	17.839	2504	2508	2514	rBV	27343	48291	1.90%	0.256%
82	17.928	2522	2523	2527	rBV4	2761	3987	0.16%	0.021%
83	17.975	2529	2531	2534	rVB4	6740	4913	0.19%	0.026%
84	18.098	2550	2552	2555	rBV4	3261	3298	0.13%	0.017%
85	18.151	2557	2561	2564	rBV5	20882	31111	1.22%	0.165%
86	18.257	2576	2579	2585	rVB7	9788	18485	0.73%	0.098%
87	18.328	2585	2591	2593	rBV7	5532	10815	0.43%	0.057%
88	18.422	2602	2607	2610	rBV7	5967	10790	0.42%	0.057%
89	18.469	2613	2615	2619	rVV3	5936	6625	0.26%	0.035%
90	18.551	2627	2629	2630	rBV2	3643	3299	0.13%	0.017%
91	18.622	2639	2641	2644	rBV4	5120	4483	0.18%	0.024%
92	18.663	2646	2648	2650	rBV3	3924	3654	0.14%	0.019%
93	18.834	2671	2677	2679	rBV7	4111	7634	0.30%	0.040%
94	19.110	2722	2724	2726	rBV3	4622	3688	0.14%	0.020%
95	19.275	2750	2752	2756	rBV5	7947	9571	0.38%	0.051%
96	19.386	2767	2771	2775	rBV7	12355	21048	0.83%	0.111%
97	19.598	2801	2807	2816	rBV	367380	516763	20.31%	2.737%
98	21.345	3099	3104	3118	rBV	1784329	2544225	100.00%	13.475%
99	23.610	3485	3489	3494	rVB2	124696	207953	8.17%	1.101%
100	23.763	3508	3515	3526	rBV2	923973	2007988	78.92%	10.635%




Sum of corrected areas: 18881134

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010556.D
Acq On : 26 May 2022 02:35
Operator : CG/JU
Sample : N2950-09DL 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTH2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

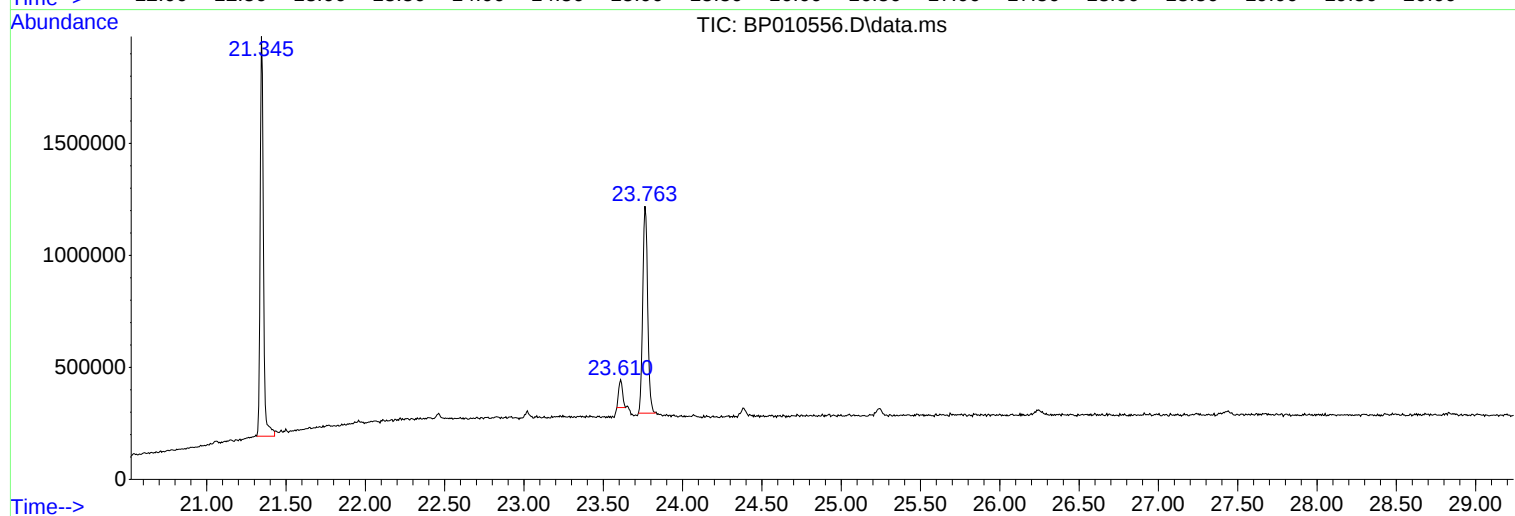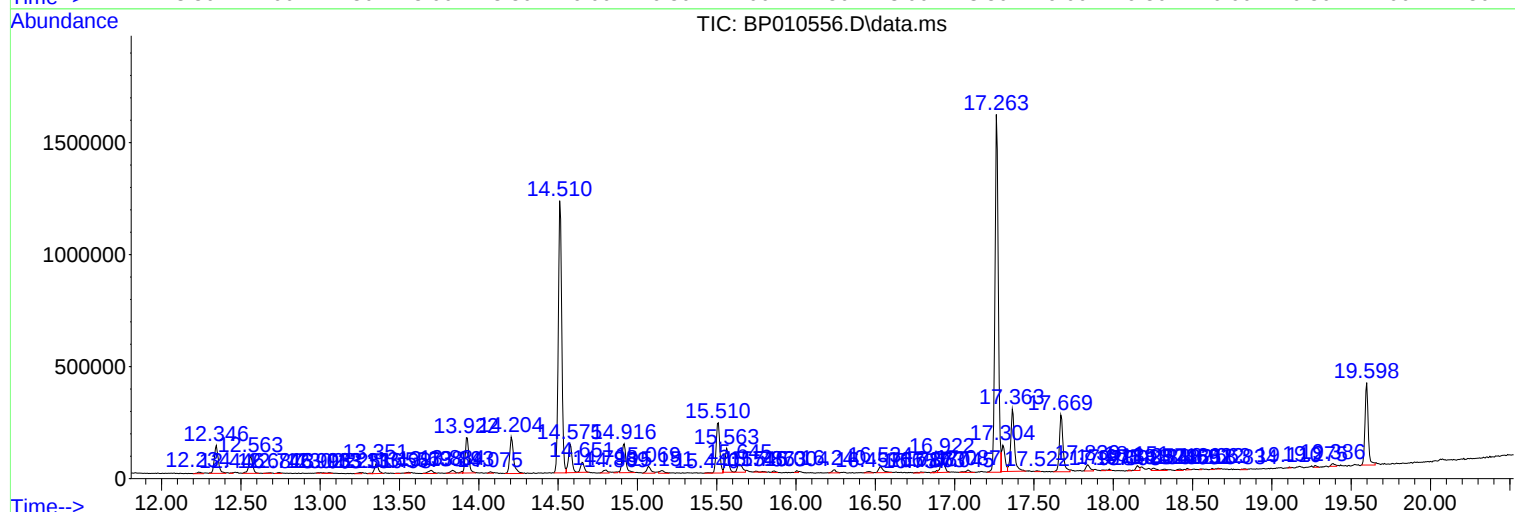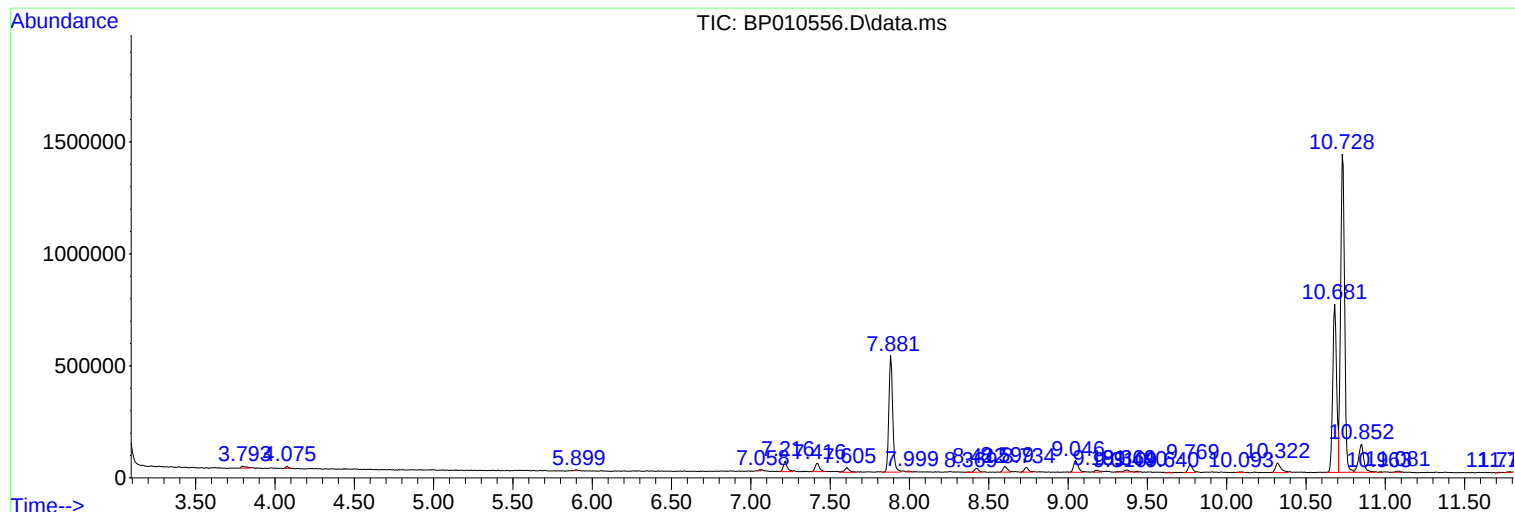

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010556.D
Acq On : 26 May 2022 02:35
Operator : CG/JU
Sample : N2950-09DL 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTH2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052522\
Data File : BP010556.D
Acq On : 26 May 2022 02:35
Operator : CG/JU
Sample : N2950-09DL 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTH2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------