
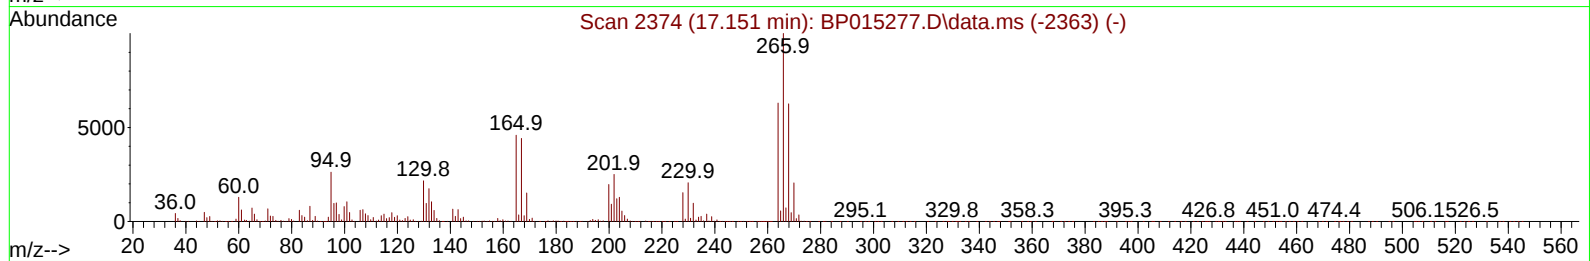
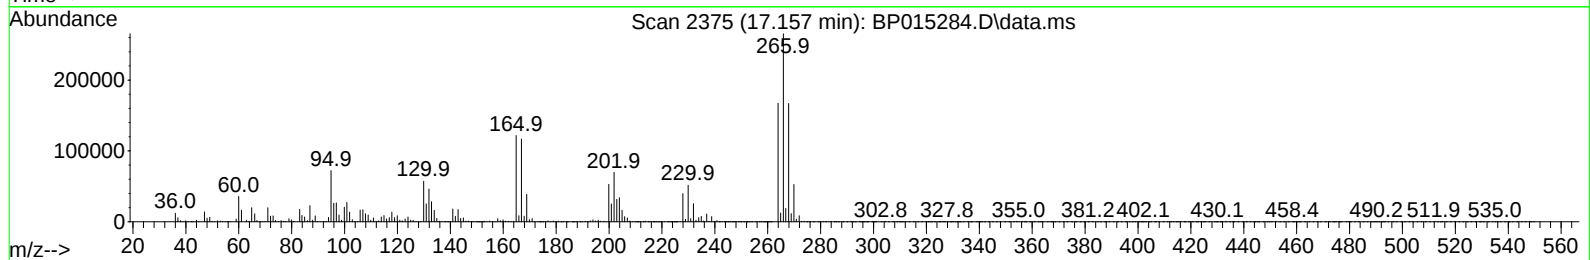


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052523\
Data File : BP015284.D
Acq On : 25 May 2023 09:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 15:16:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 01:41:43 2023
Response via : Initial Calibration

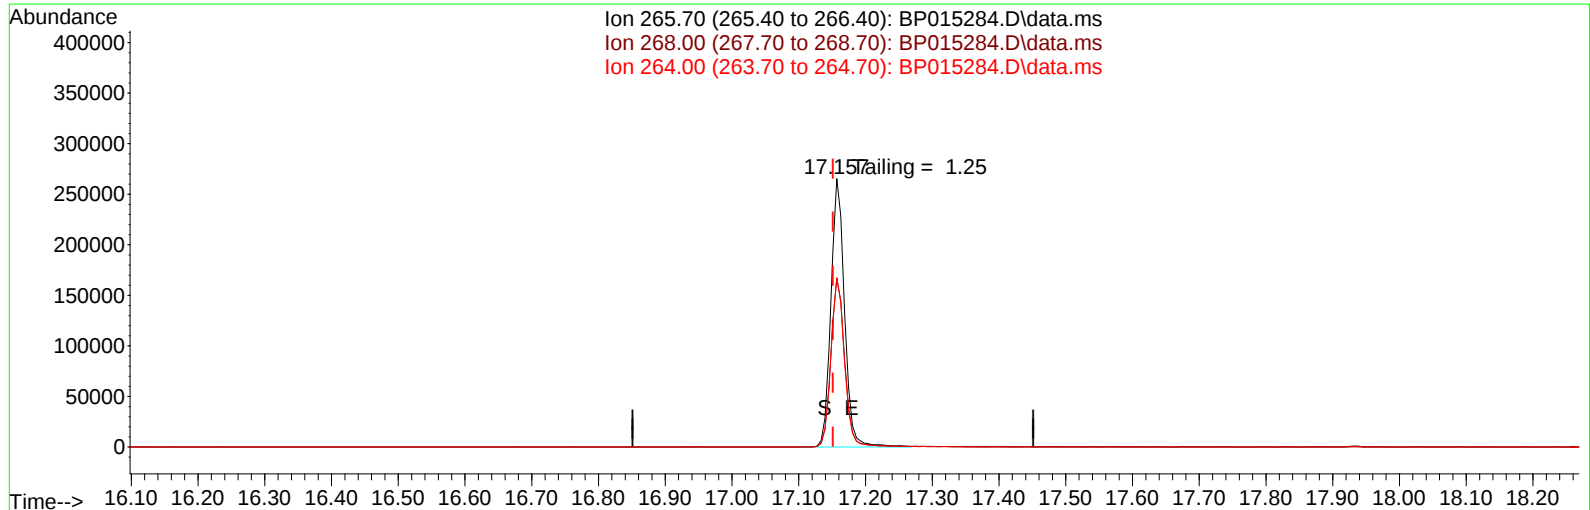

TIC: BP015284.D\data.ms

(70) Pentachlorophenol (C)




17.157min (+ 0.006) 122236.90 ng

response 378050

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	62.92
264.00	63.00	63.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052523\
Data File : BP015284.D
Acq On : 25 May 2023 09:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 15:16:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 01:41:43 2023
Response via : Initial Calibration

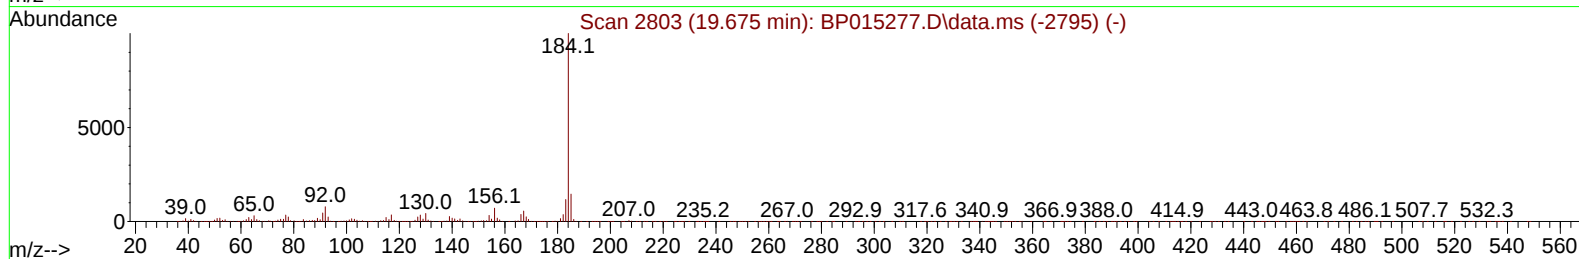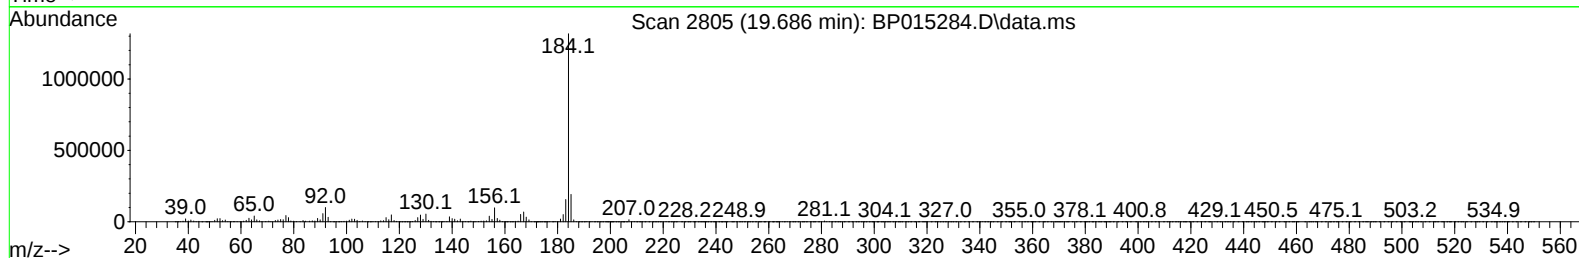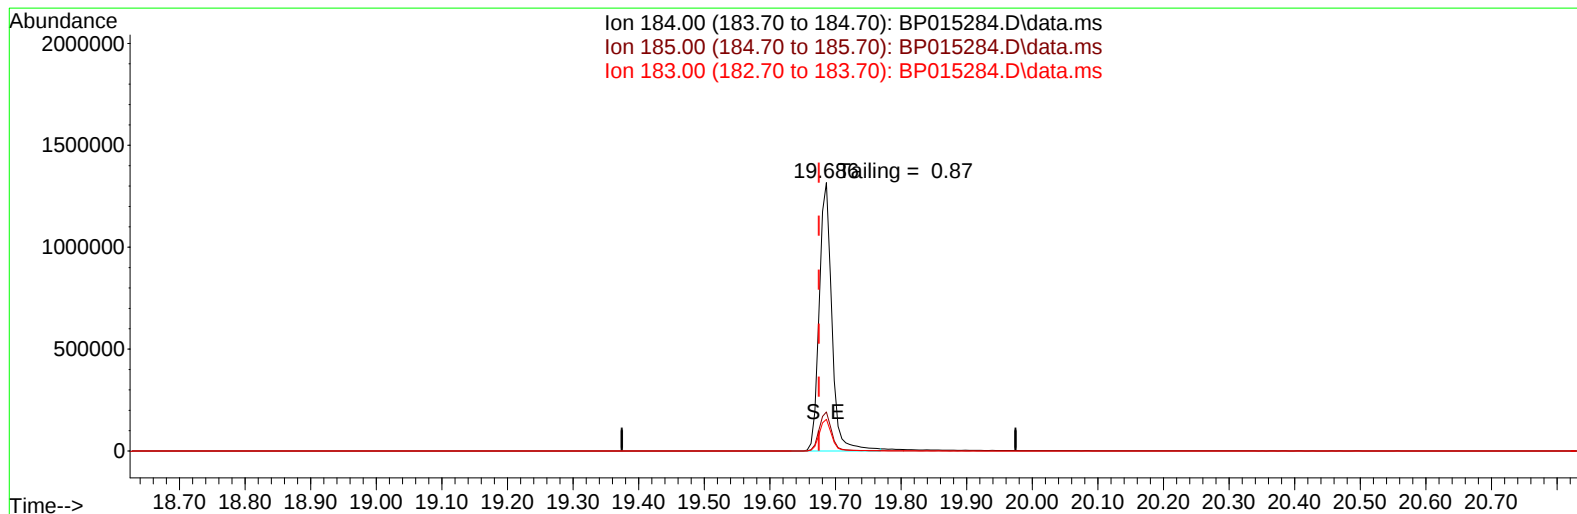

TIC: BP015284.D\data.ms

(77) Benzidine**19.686min (+ 0.012) 33876.48 ng****response 1783678**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.57
183.00	11.70	11.84
0.00	0.00	0.00