
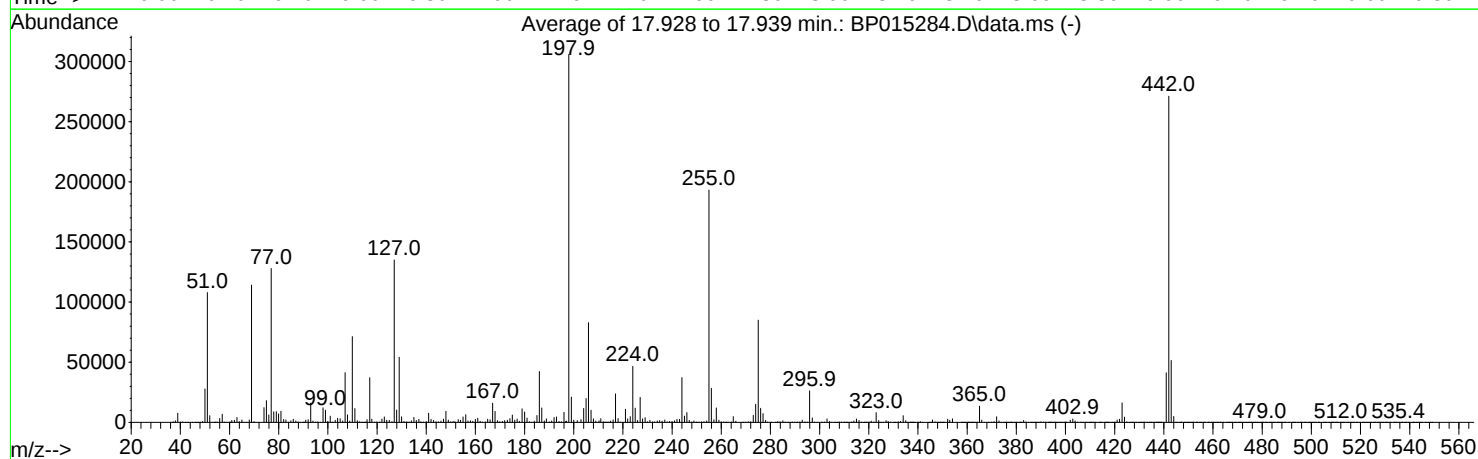


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052523\
 Data File : BP015284.D
 Acq On : 25 May 2023 09:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 25 01:41:43 2023

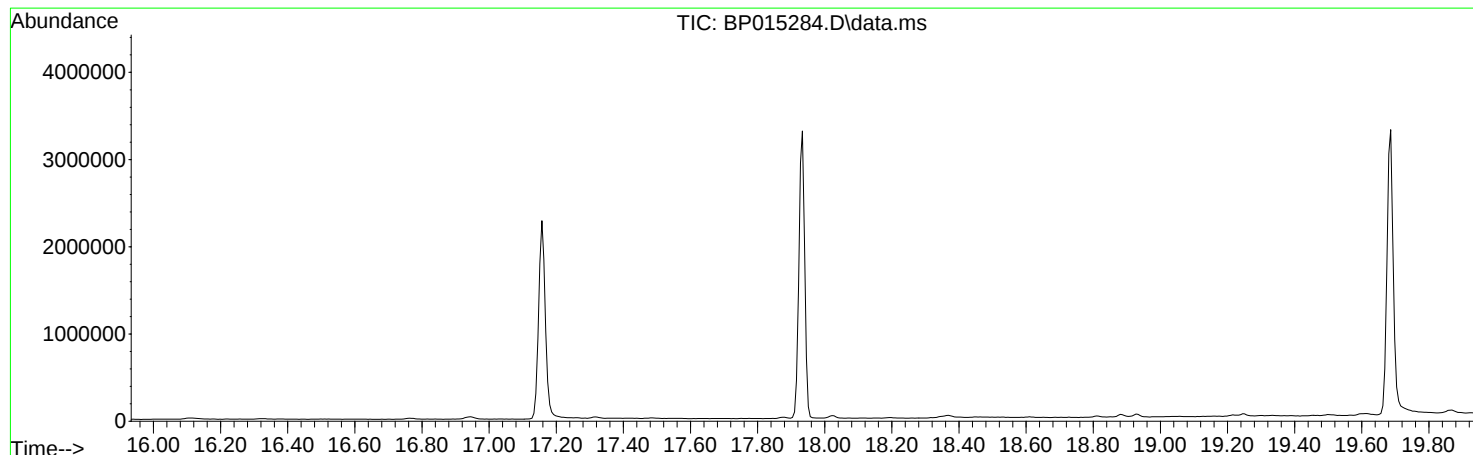

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	107936	PASS
68	69	0.00	2	1.7	1962	PASS
69	198	0.00	100	37.3	114165	PASS
70	69	0.00	2	0.6	665	PASS
127	198	10	80	44.2	135061	PASS
197	198	0.00	2	0.3	1019	PASS
198	198	100	100	100.0	305837	PASS
199	198	5	9	6.9	21085	PASS
275	198	10	60	27.8	85051	PASS
365	198	1	100	4.4	13453	PASS
441	198	0.01	100	13.5	41213	PASS
442	442	100	100	100.0	271061	PASS
443	442	15	24	19.0	51439	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
5/25/2023	BNA_P	<u>BP015284.D</u>
Compound Name	Response	Retention Time
DDT	963931	20.88
DDD	15423	20.451
DDE	501	19.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15924	979855	1.63

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052523\
Data File : BP015284.D
Acq On : 25 May 2023 09:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 25 15:16:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 01:41:43 2023
Response via : Initial Calibration

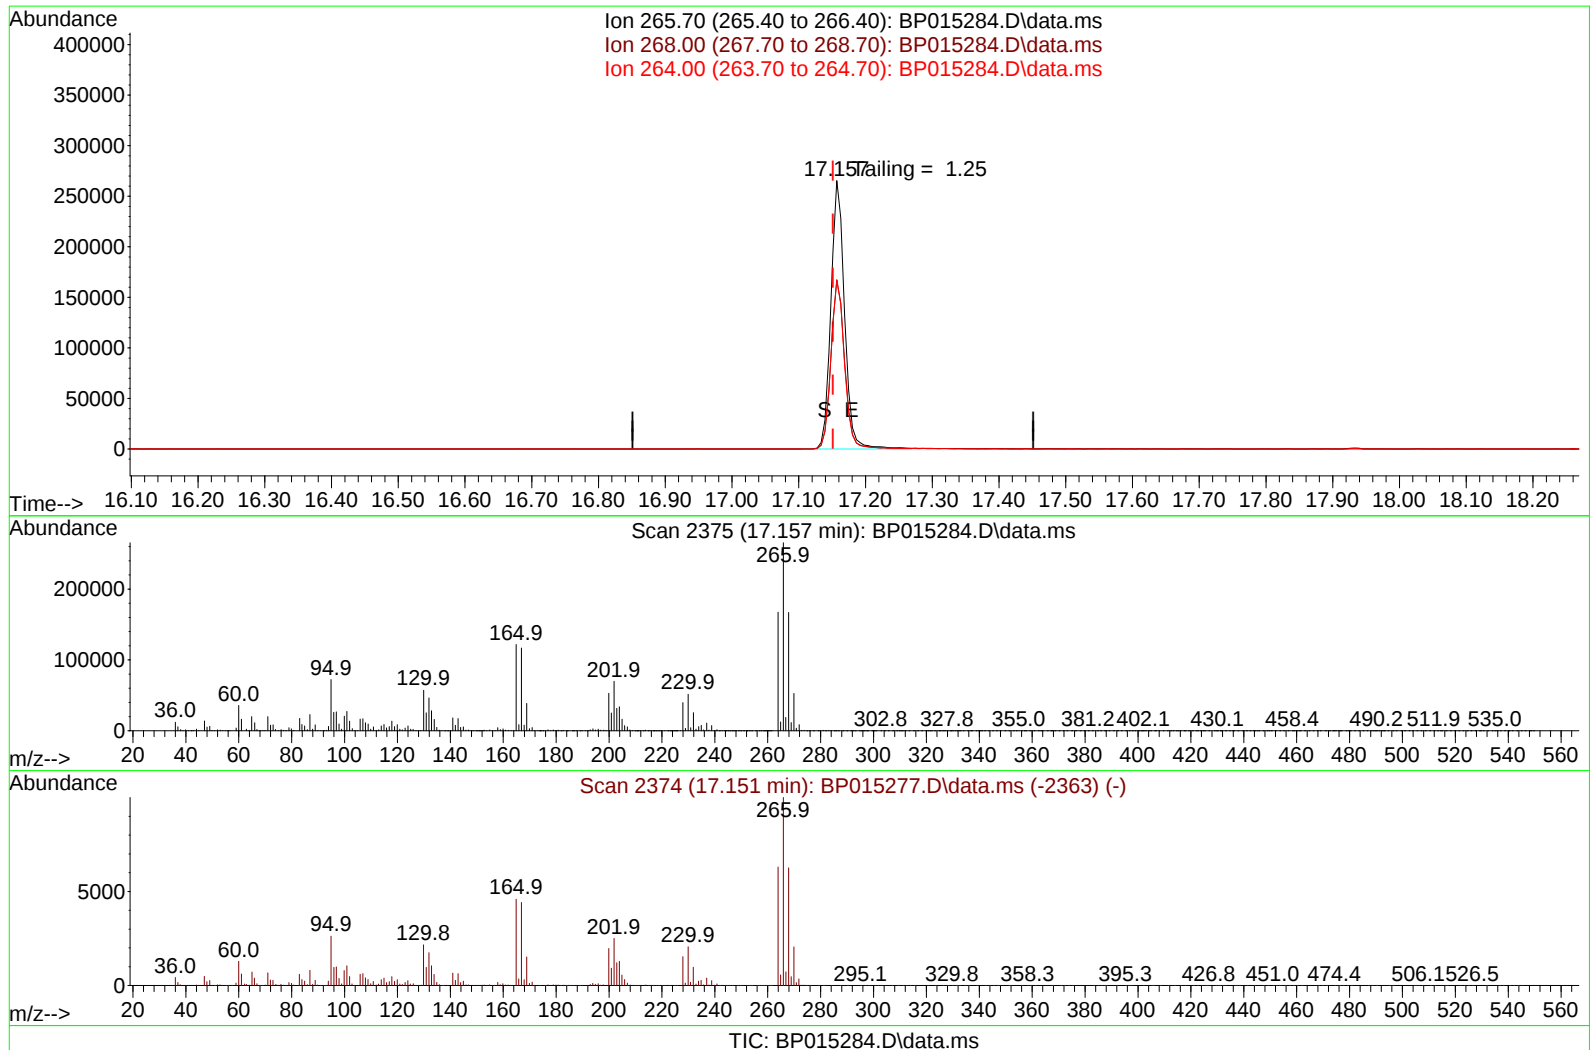

TIC: BP015284.D\data.ms

(70) Pentachlorophenol (C)

17.157min (+ 0.006) 122236.90 ng




response 378050

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	62.92
264.00	63.00	63.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052523\
Data File : BP015284.D
Acq On : 25 May 2023 09:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 25 15:16:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 01:41:43 2023
Response via : Initial Calibration

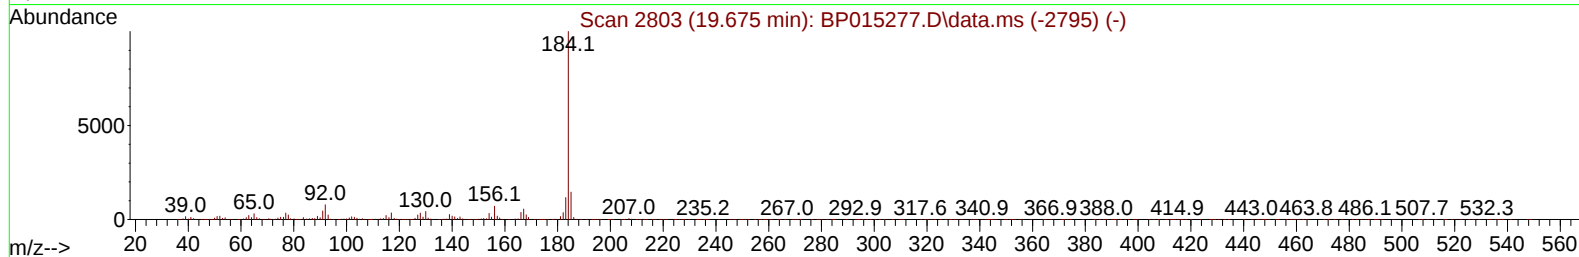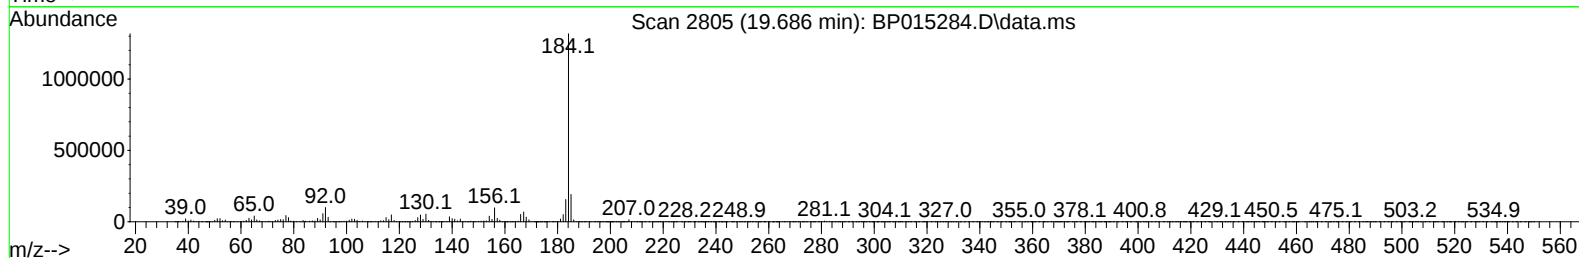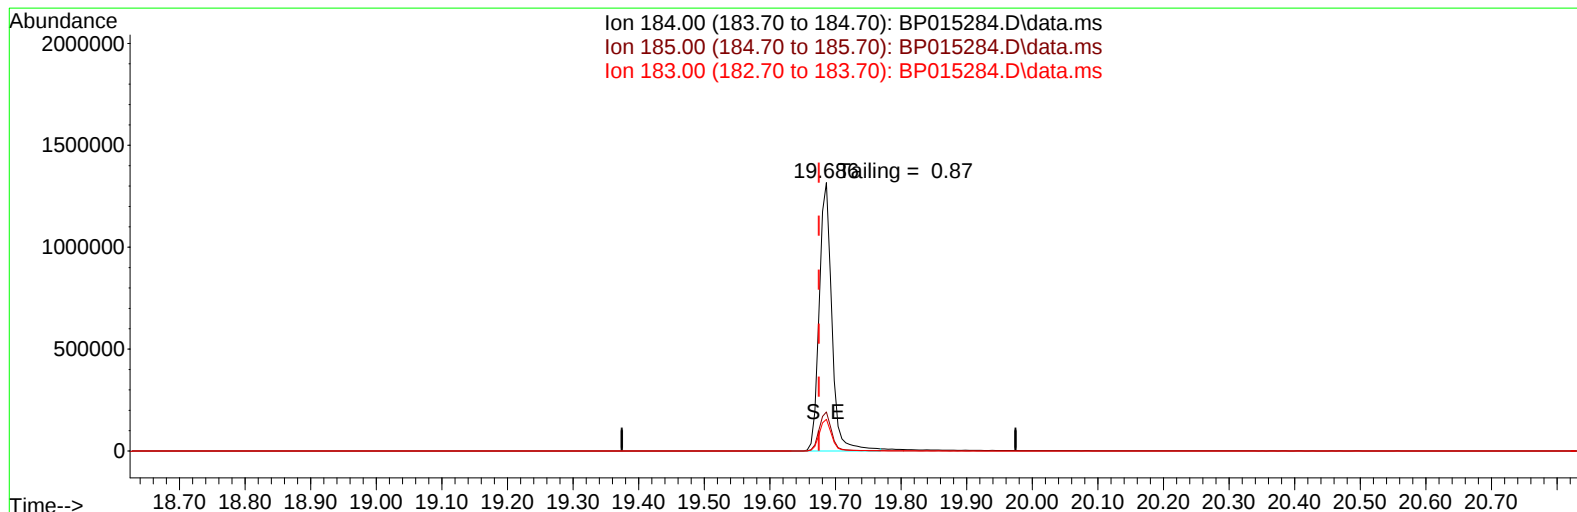

TIC: BP015284.D\data.ms

(77) Benzidine

19.686min (+ 0.012) 33876.48 ng

response 1783678

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.57
183.00	11.70	11.84
0.00	0.00	0.00