
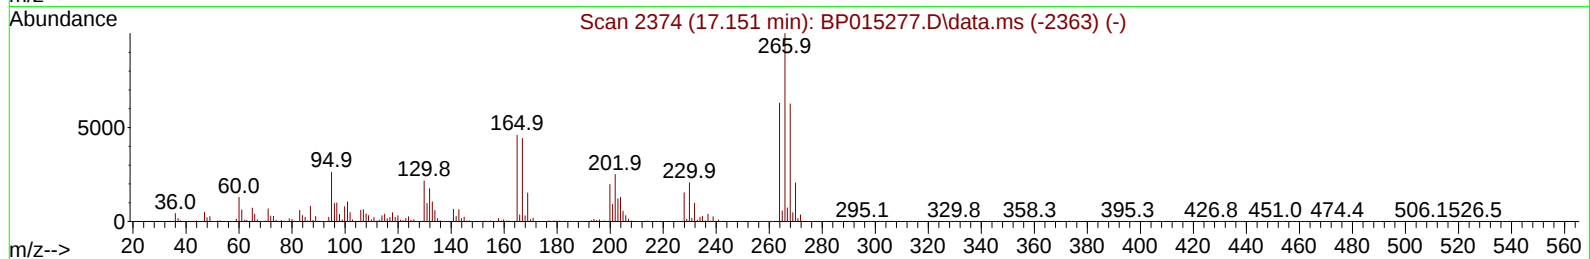
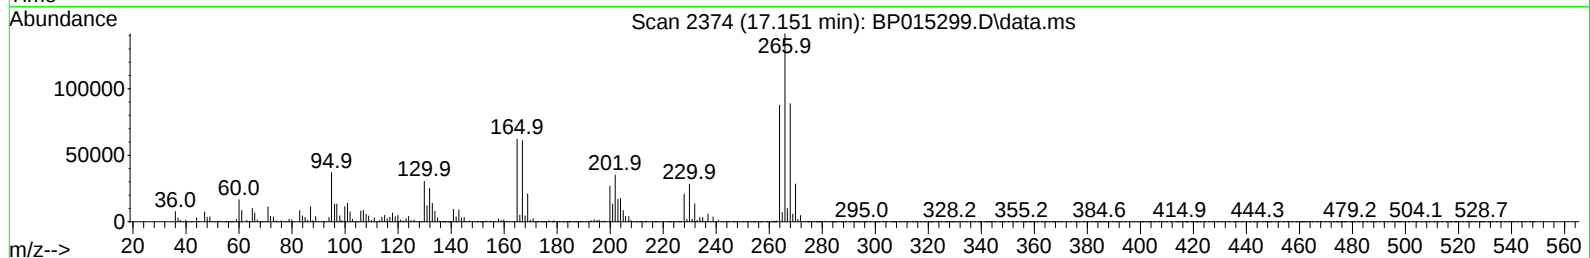


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052623\
Data File : BP015299.D
Acq On : 26 May 2023 07:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 16:54:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 01:41:43 2023
Response via : Initial Calibration

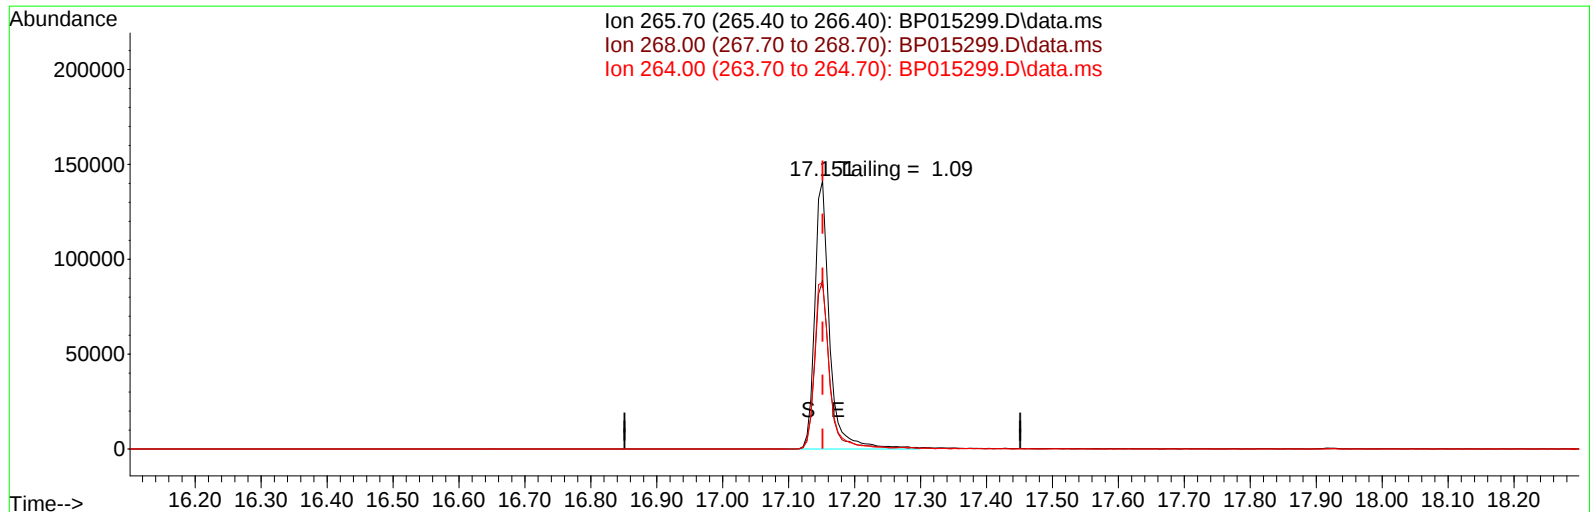

TIC: BP015299.D\data.ms

(70) Pentachlorophenol (C)




17.151min (+ 0.000) 459029.29 ng

response 221004

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	62.79
264.00	63.00	61.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052623\
 Data File : BP015299.D
 Acq On : 26 May 2023 07:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 16:54:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 25 01:41:43 2023
 Response via : Initial Calibration

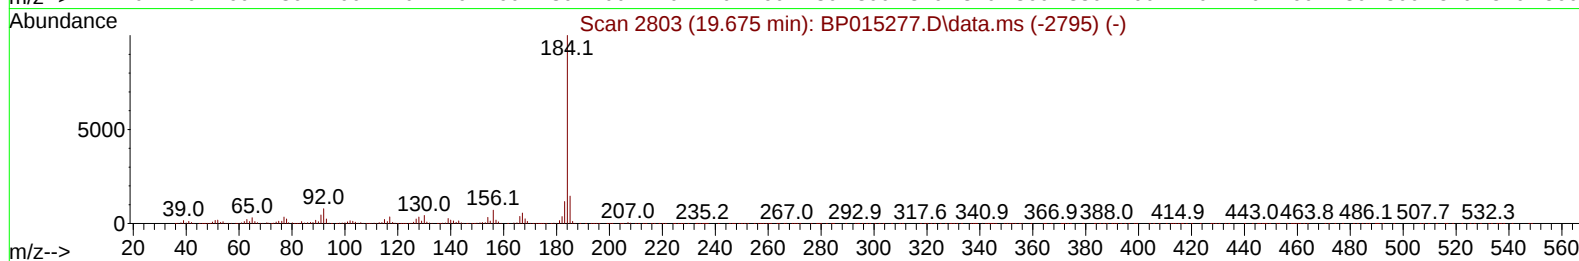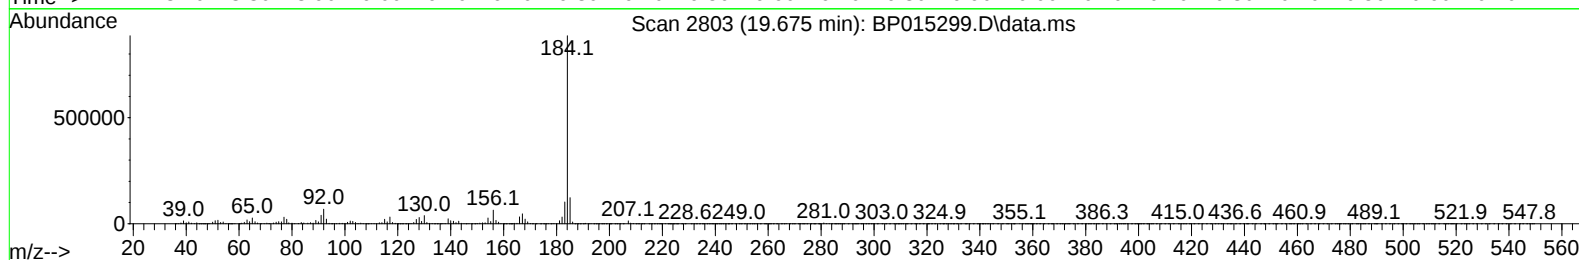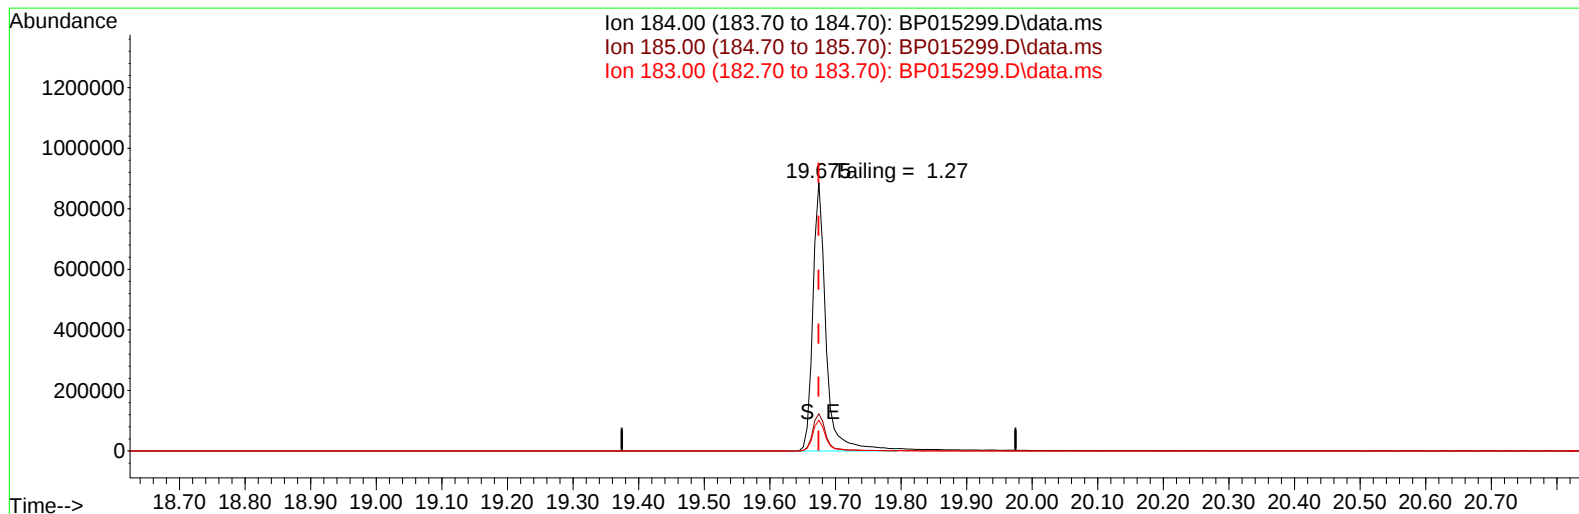

TIC: BP015299.D\data.ms

(77) Benzidine**19.675min (+ 0.000) 236942.12 ng****response 1245681**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.91
183.00	11.70	11.54
0.00	0.00	0.00