
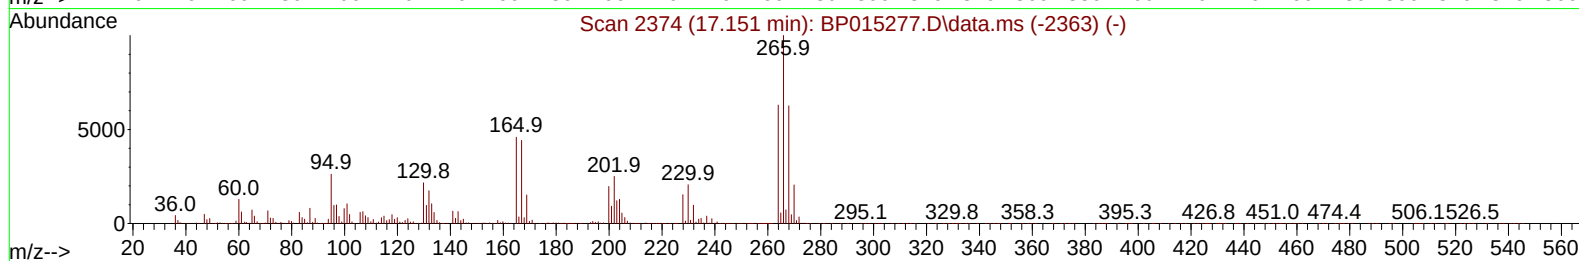
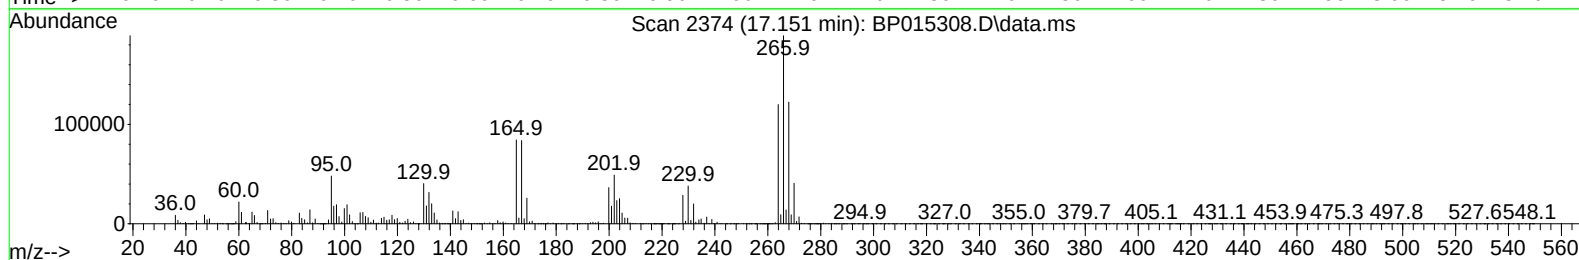


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052623\
 Data File : BP015308.D
 Acq On : 26 May 2023 14:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 15:57:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 25 01:41:43 2023
 Response via : Initial Calibration

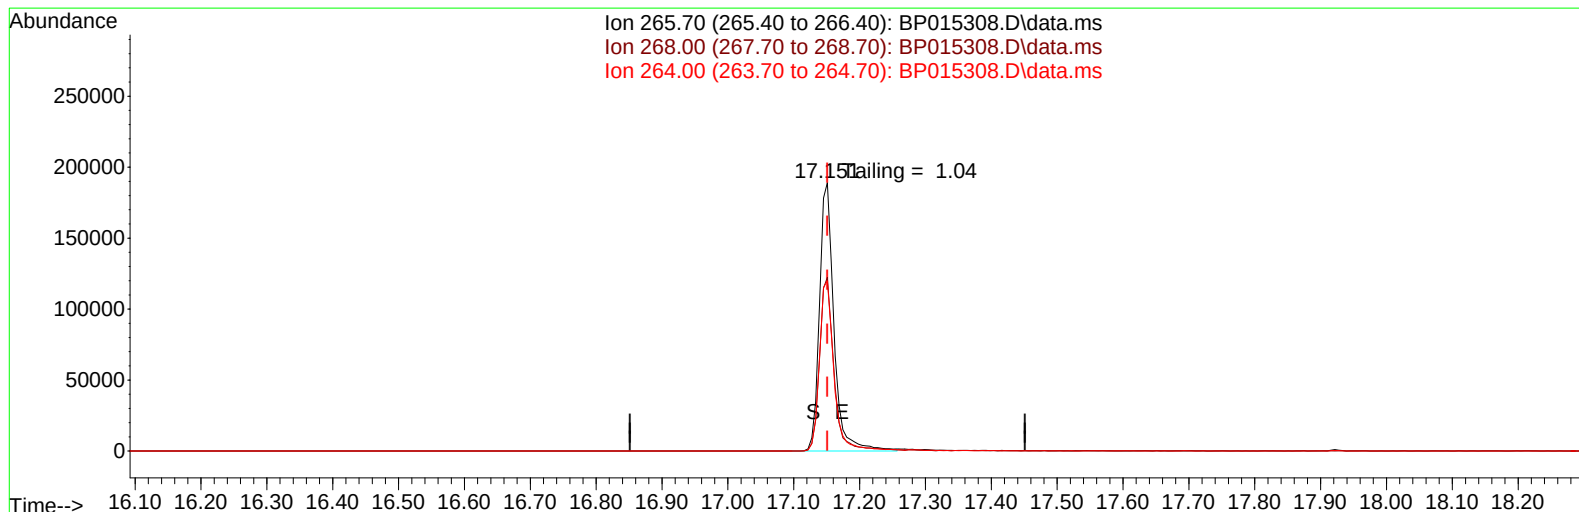

TIC: BP015308.D\data.ms

(70) Pentachlorophenol (C)




17.151min (-0.000) 157785.78 ng

response 290994

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	64.73
264.00	63.00	63.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052623\
 Data File : BP015308.D
 Acq On : 26 May 2023 14:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 15:57:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 25 01:41:43 2023
 Response via : Initial Calibration

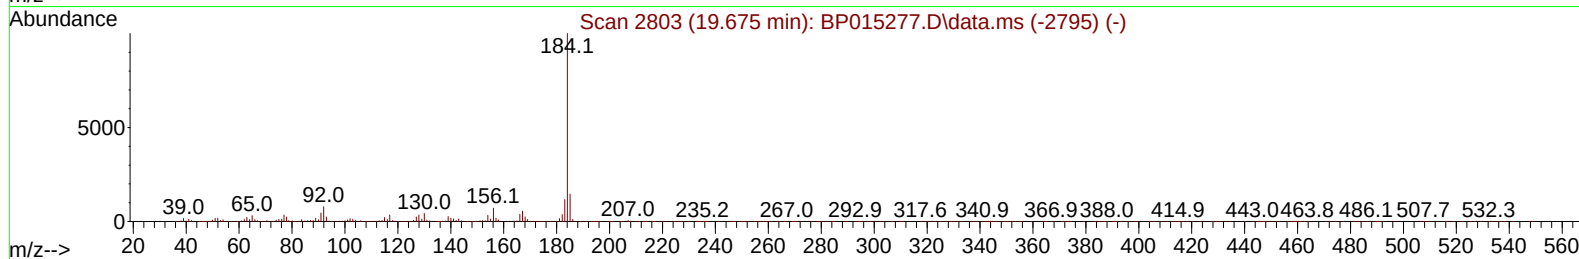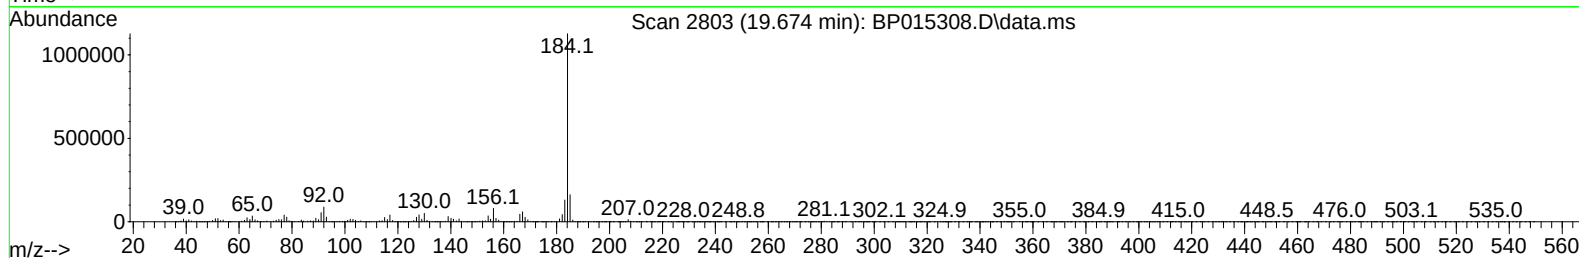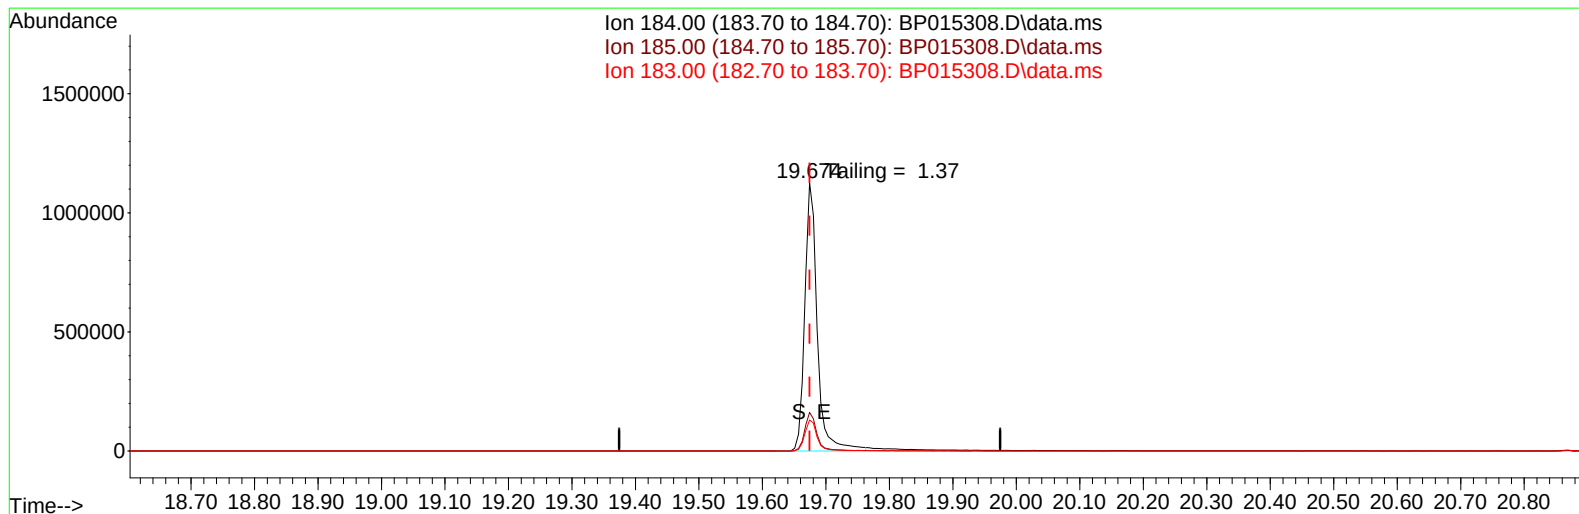

TIC: BP015308.D\data.ms

(77) Benzidine**19.674min (-0.000) 169751.74 ng****response 1594026**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.37
183.00	11.70	11.56
0.00	0.00	0.00