

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052623\
 Data File : BP015311.D
 Acq On : 26 May 2023 16:17
 Operator : CG/JU
 Sample : 02908-09
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TWP02

Quant Time: May 26 18:10:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 25 01:41:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.105	152	127464	20.000	ng	0.00
21) Naphthalene-d8	10.934	136	488646	20.000	ng	0.00
39) Acenaphthene-d10	14.745	164	287206	20.000	ng	0.00
64) Phenanthrene-d10	17.498	188	653771	20.000	ng	0.00
76) Chrysene-d12	21.580	240	717896	20.000	ng	0.00
86) Perylene-d12	24.133	264	851500	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.634	112	595804	77.455	ng	0.00
7) Phenol-d6	7.258	99	480319	47.647	ng	0.00
23) Nitrobenzene-d5	9.281	82	933894	93.316	ng	-0.01
42) 2,4,6-Tribromophenol	16.239	330	547111	140.179	ng	0.00
45) 2-Fluorobiphenyl	13.375	172	1879052	87.837	ng	0.00
79) Terphenyl-d14	20.039	244	3265357	85.556	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052623\
Data File : BP015311.D
Acq On : 26 May 2023 16:17
Operator : CG/JU
Sample : 02908-09
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TWP02

Quant Time: May 26 18:10:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 01:41:43 2023
Response via : Initial Calibration




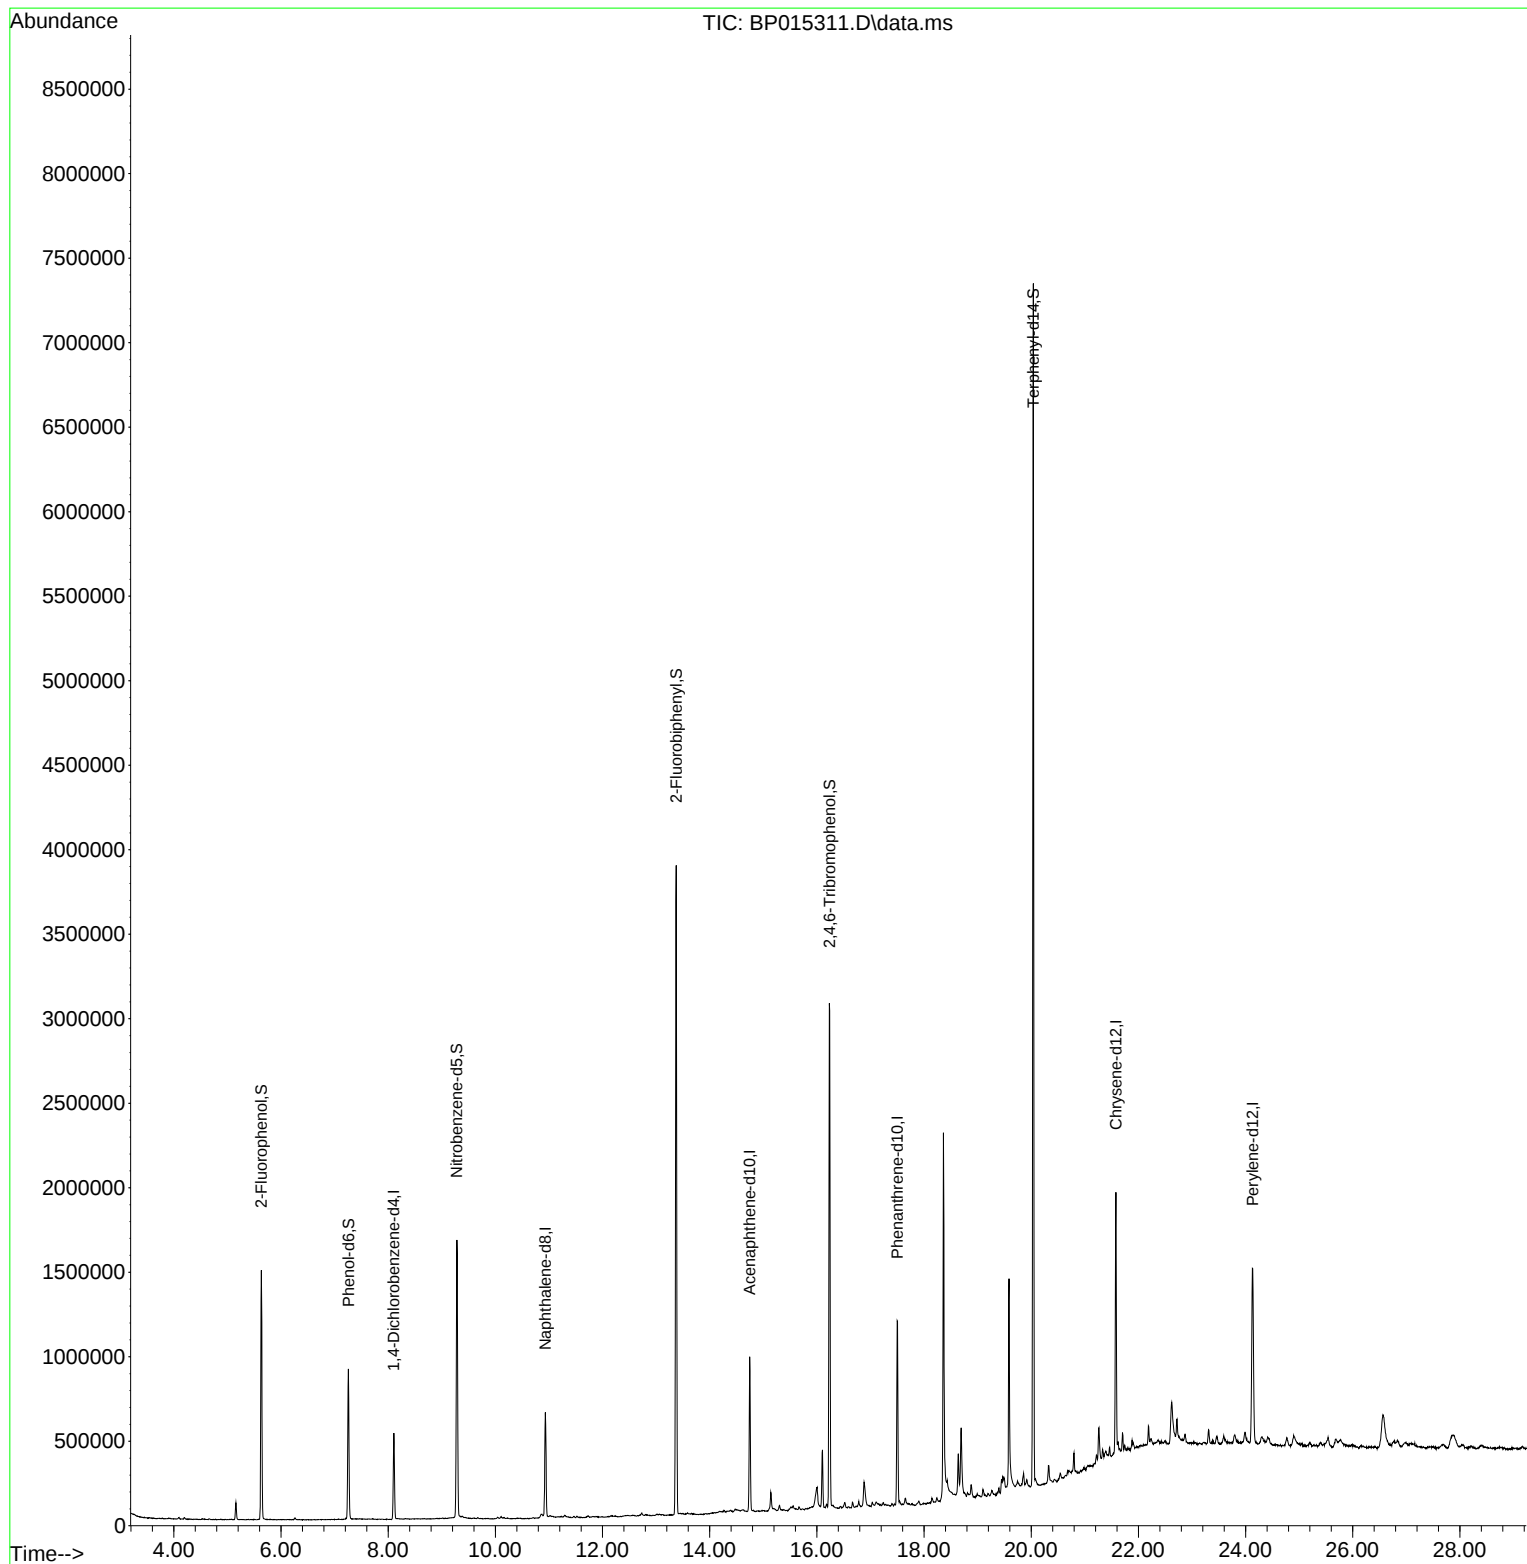


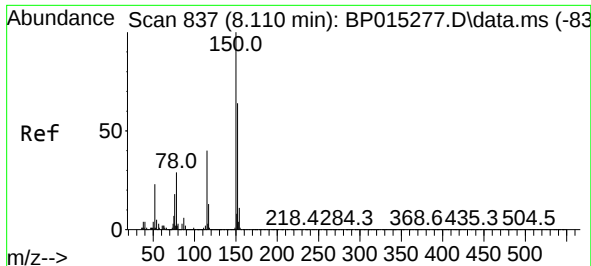

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.105 min Scan# 81
 Delta R.T. -0.005 min
 Lab File: BP015311.D
 Acq: 26 May 2023 16:17




Instrument :
 BNA_P
 ClientSampleId :
 TWP02


Tgt Ion:152 Resp: 127464
 Ion Ratio Lower Upper
 152 100
 150 151.6 124.2 186.2
 115 61.1 49.1 73.7

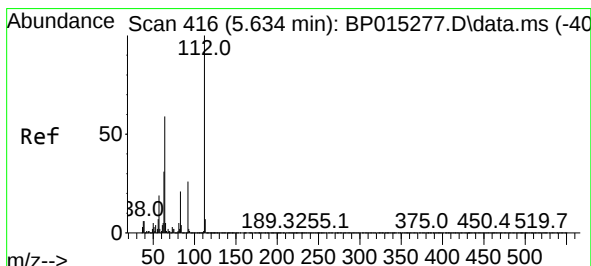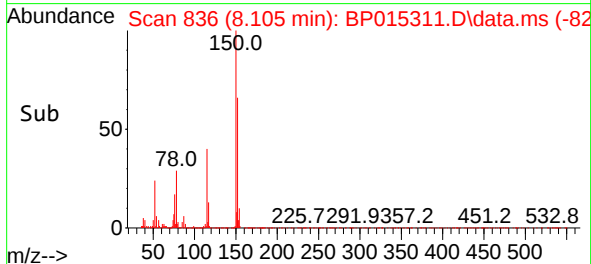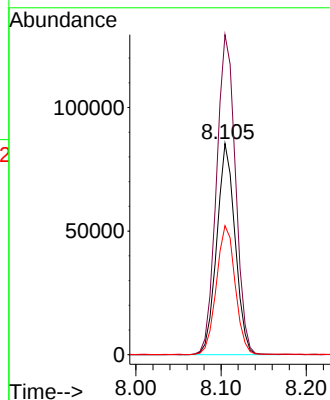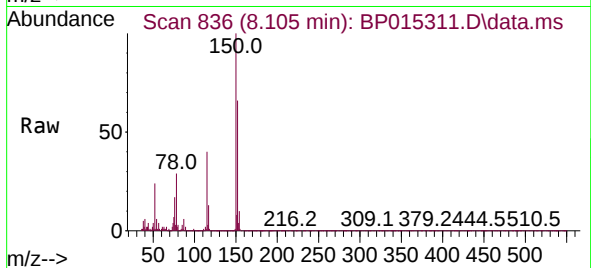

#5
 2-Fluorophenol
 Concen: 77.455 ng
 RT: 5.634 min Scan# 416
 Delta R.T. 0.000 min
 Lab File: BP015311.D
 Acq: 26 May 2023 16:17

Tgt Ion:112 Resp: 595804
 Ion Ratio Lower Upper
 112 100
 64 59.0 47.2 70.8
 63 32.4 24.6 37.0


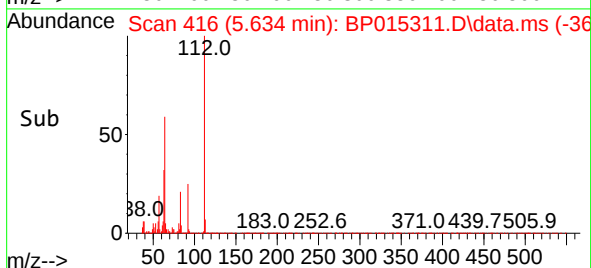
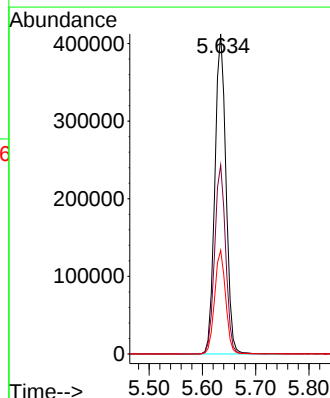
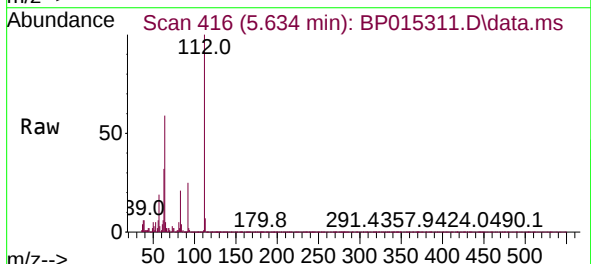


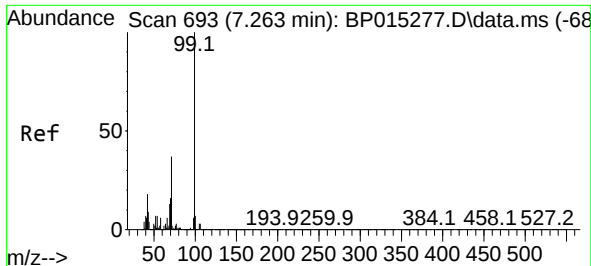

#7
Phenol-d6
Concen: 47.647 ng
RT: 7.258 min Scan# 64
Delta R.T. -0.006 min
Lab File: BP015311.D
Acq: 26 May 2023 16:17




Instrument :
BNA_P
ClientSampleId :
TWP02


Tgt Ion: 99 Resp: 480319
Ion Ratio Lower Upper
99 100
42 19.2 14.6 22.0
71 35.8 29.4 44.2

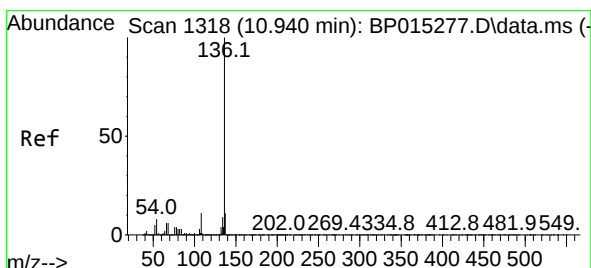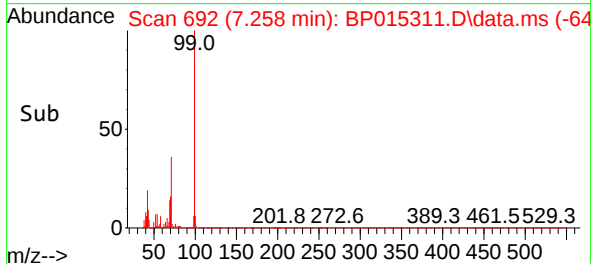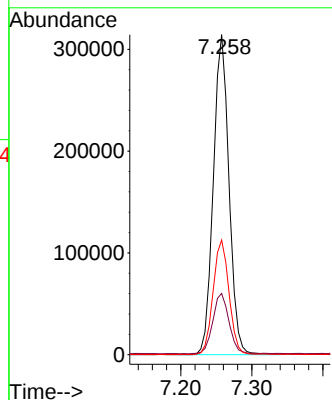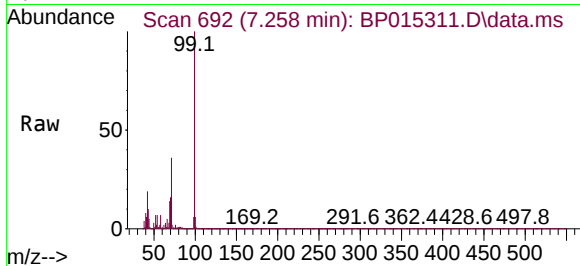

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.934 min Scan# 1317
Delta R.T. -0.006 min
Lab File: BP015311.D
Acq: 26 May 2023 16:17

Tgt Ion: 136 Resp: 488646
Ion Ratio Lower Upper
136 100
137 10.8 8.9 13.3
54 7.9 6.3 9.5
68 6.6 5.1 7.7


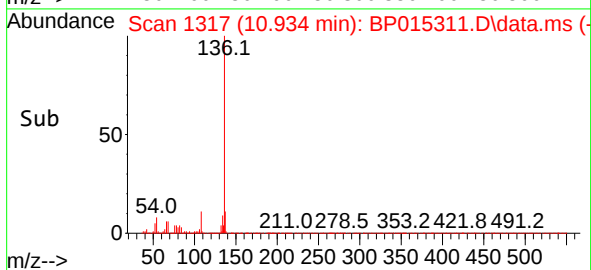
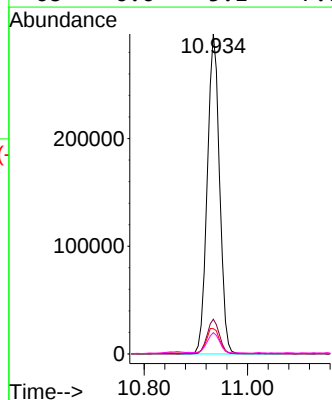
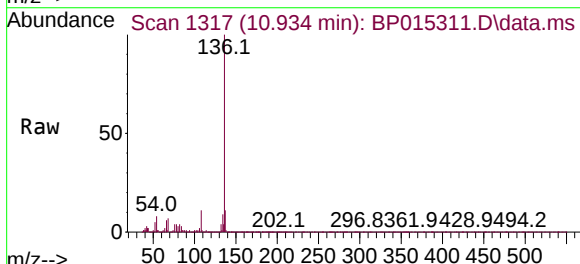


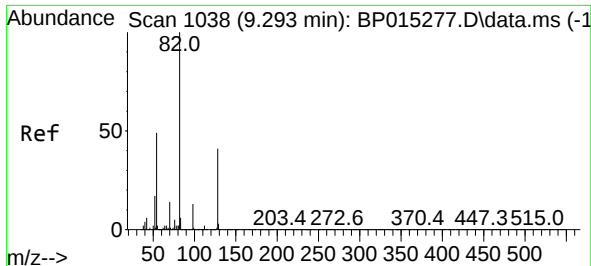

#23
Nitrobenzene-d5
Concen: 93.316 ng
RT: 9.281 min Scan# 1036
Delta R.T. -0.012 min
Lab File: BP015311.D
Acq: 26 May 2023 16:17




Instrument :
BNA_P
ClientSampleId :
TWP02


Tgt Ion: 82 Resp: 933894
Ion Ratio Lower Upper
82 100
128 40.1 33.0 49.4
54 50.5 39.2 58.8

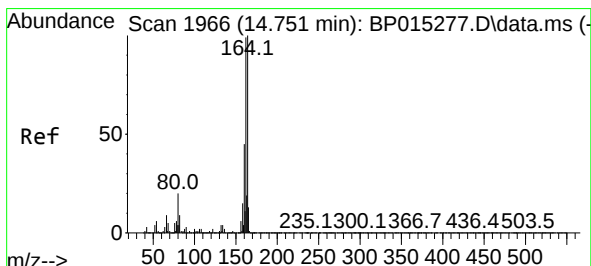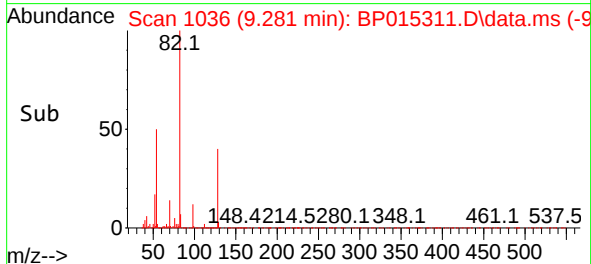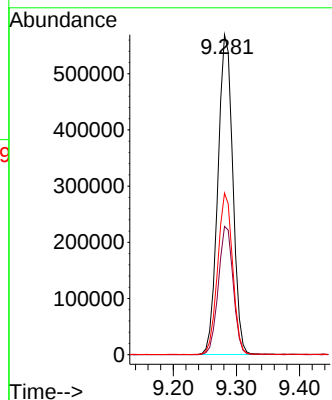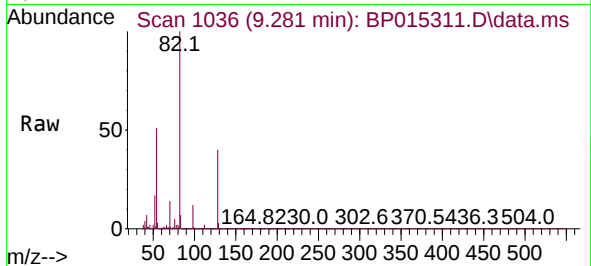

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.745 min Scan# 1965
Delta R.T. -0.006 min
Lab File: BP015311.D
Acq: 26 May 2023 16:17

Tgt Ion: 164 Resp: 287206
Ion Ratio Lower Upper
164 100
162 100.1 79.4 119.2
160 43.8 35.6 53.4

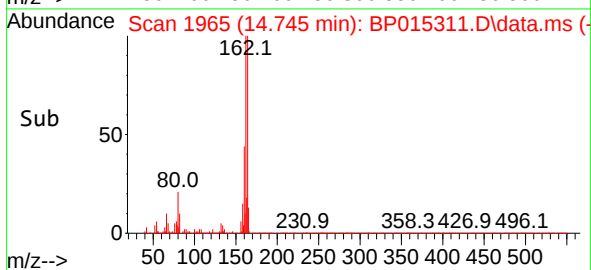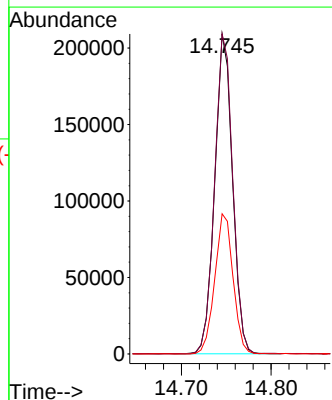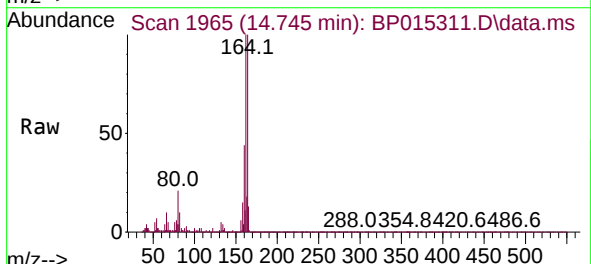

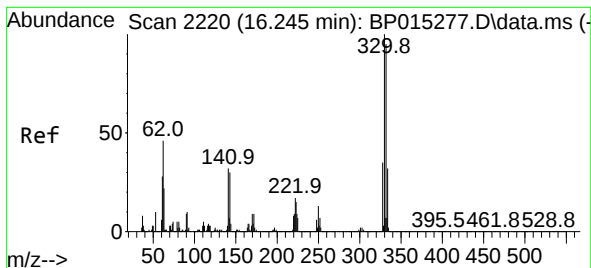

#42

2,4,6-Tribromophenol

Concen: 140.179 ng

RT: 16.239 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP015311.D

Acq: 26 May 2023 16:17

Instrument :

BNA_P

ClientSampleId :

TWP02





Tgt Ion:330 Resp: 547111

Ion Ratio Lower Upper

330 100

332 96.4 76.3 114.5

141 35.9 27.8 41.8

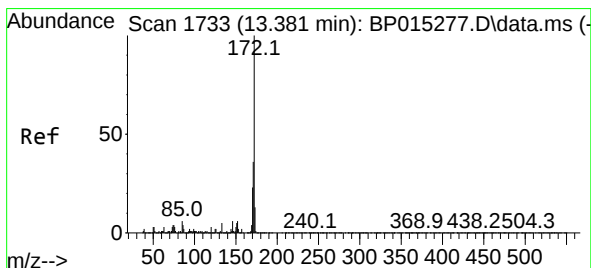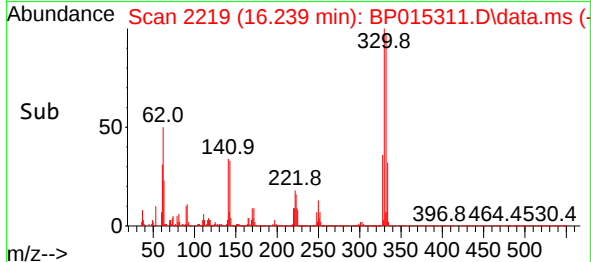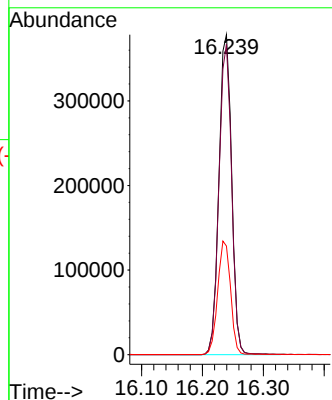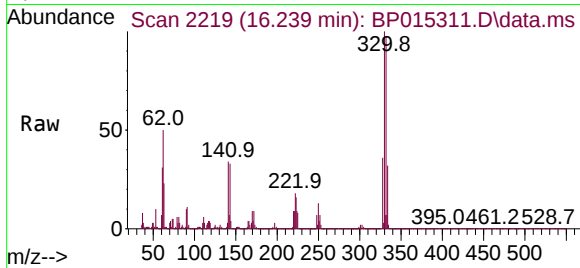

#45

2-Fluorobiphenyl

Concen: 87.837 ng

RT: 13.375 min Scan# 1732

Delta R.T. -0.006 min

Lab File: BP015311.D

Acq: 26 May 2023 16:17




Tgt Ion:172 Resp: 1879052


Ion Ratio Lower Upper

172 100

171 34.9 28.4 42.6

170 23.4 18.7 28.1

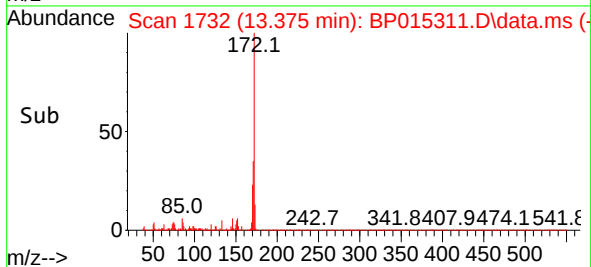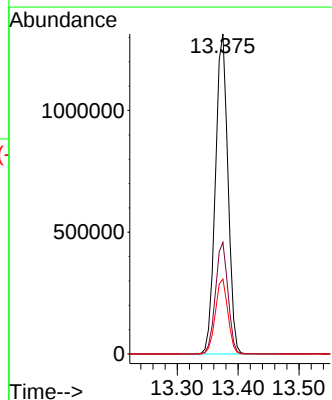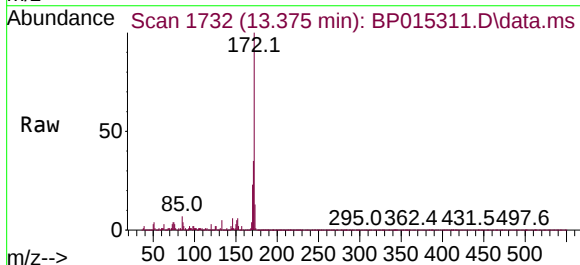

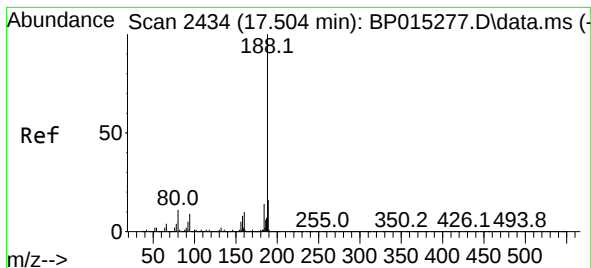

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.498 min Scan# 2434

Delta R.T. -0.006 min

Lab File: BP015311.D

Acq: 26 May 2023 16:17

Instrument :

BNA_P

ClientSampleId :

TWP02





Tgt Ion:188 Resp: 653771

Ion Ratio Lower Upper

188 100

94 9.9 7.4 11.0

80 11.4 8.6 13.0

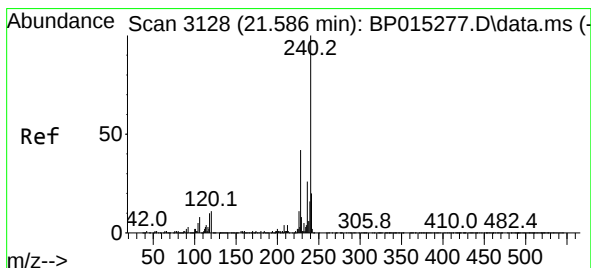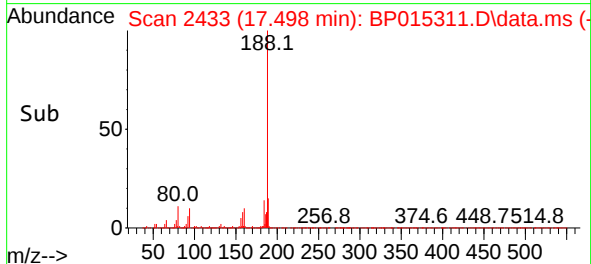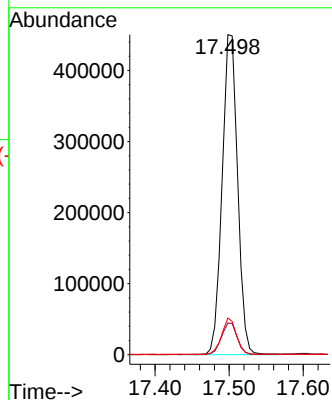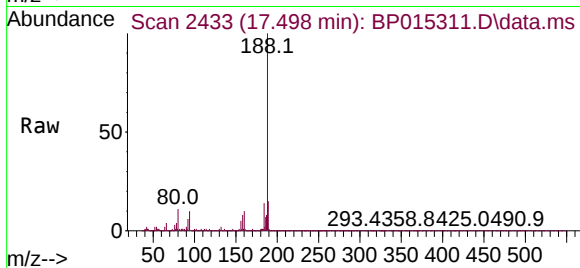

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.580 min Scan# 3127

Delta R.T. -0.006 min

Lab File: BP015311.D

Acq: 26 May 2023 16:17




Tgt Ion:240 Resp: 717896


Ion Ratio Lower Upper

240 100

120 11.3 8.8 13.2

236 26.1 20.5 30.7


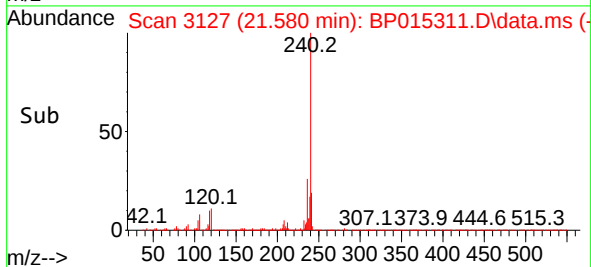
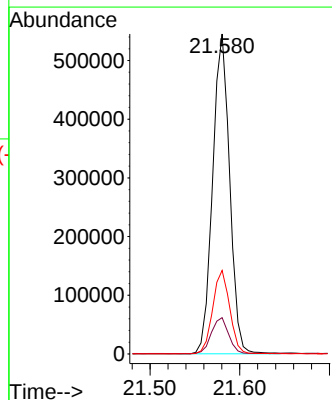
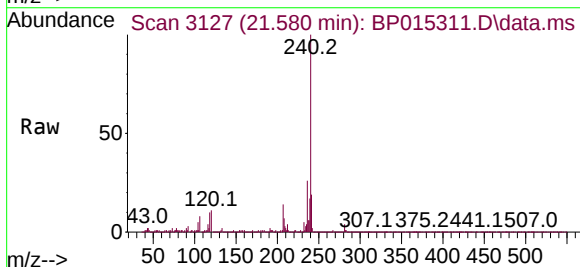


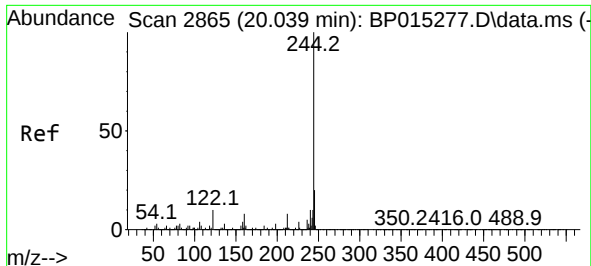

#79
 Terphenyl-d14
 Concen: 85.556 ng
 RT: 20.039 min Scan# 2865
 Delta R.T. 0.000 min
 Lab File: BP015311.D
 Acq: 26 May 2023 16:17

Instrument :
 BNA_P
 ClientSampleId :
 TWP02

Tgt Ion:244 Resp: 3265357
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.0 9.0
 122 10.1 8.2 12.4

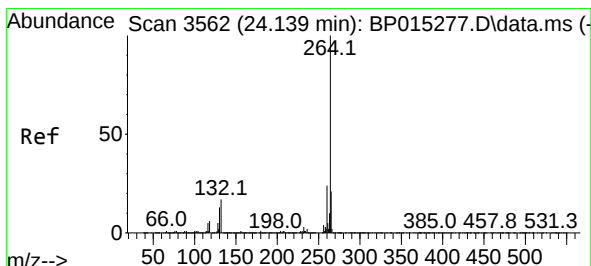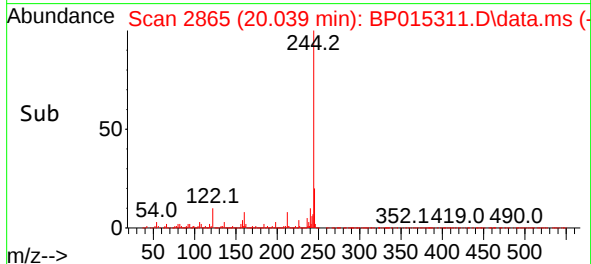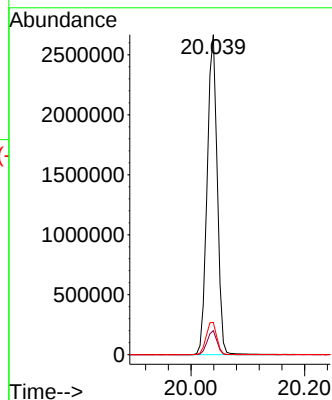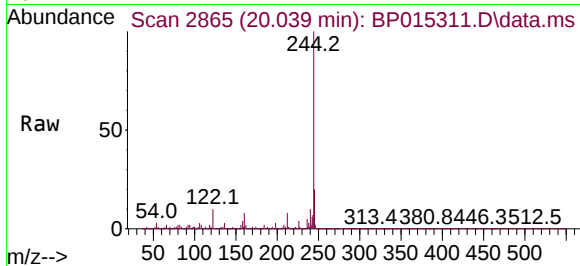

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.133 min Scan# 3561
 Delta R.T. -0.006 min
 Lab File: BP015311.D
 Acq: 26 May 2023 16:17

Tgt Ion:264 Resp: 851500
 Ion Ratio Lower Upper
 264 100
 260 24.1 19.0 28.6
 265 21.4 17.5 26.3

