
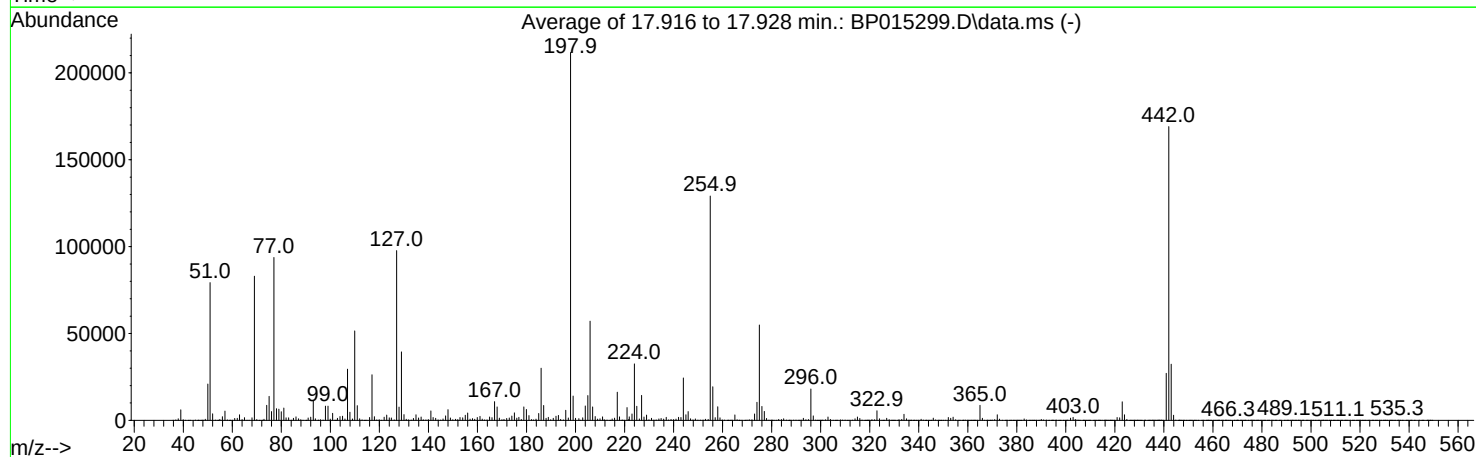


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052623\
Data File : BP015299.D
Acq On : 26 May 2023 07:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 25 01:41:43 2023

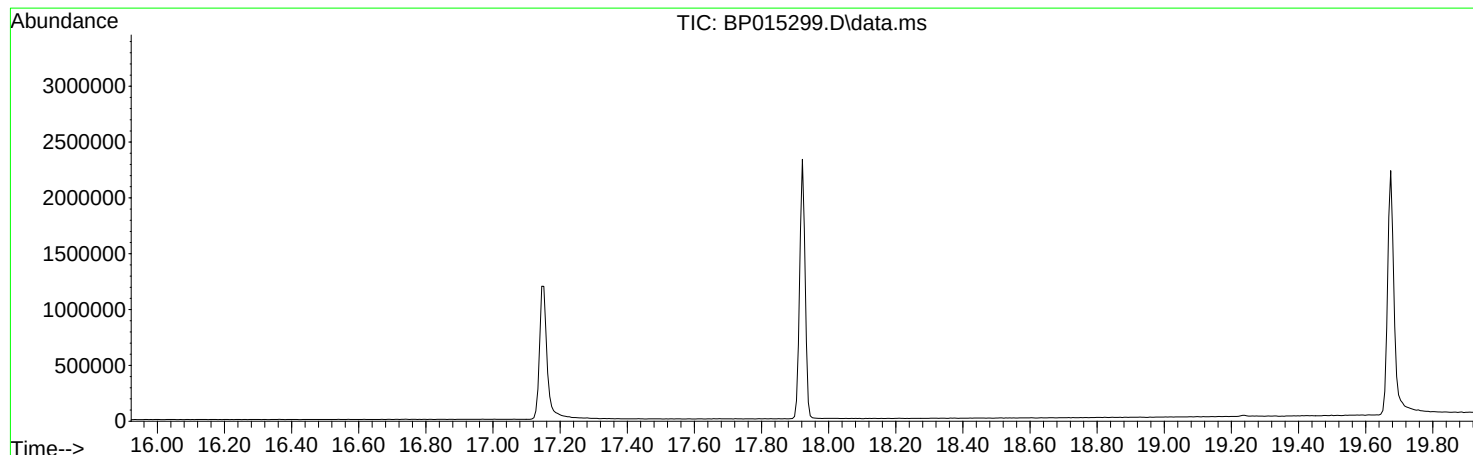

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	79276	PASS
68	69	0.00	2	1.7	1445	PASS
69	198	0.00	100	39.2	83011	PASS
70	69	0.00	2	0.5	451	PASS
127	198	10	80	46.1	97680	PASS
197	198	0.00	2	0.7	1408	PASS
198	198	100	100	100.0	211733	PASS
199	198	5	9	6.6	14042	PASS
275	198	10	60	25.9	54896	PASS
365	198	1	100	4.1	8616	PASS
441	198	0.01	100	12.8	27047	PASS
442	442	100	100	100.0	169072	PASS
443	442	15	24	19.1	32331	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/26/2023	BNA_P	<u>BP015299.D</u>
Compound Name	Response	Retention Time
DDT	685247	20.869
DDD	9380	20.492
DDE	424	19.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9804	695051	1.41

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052623\
Data File : BP015299.D
Acq On : 26 May 2023 07:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 26 16:54:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 01:41:43 2023
Response via : Initial Calibration

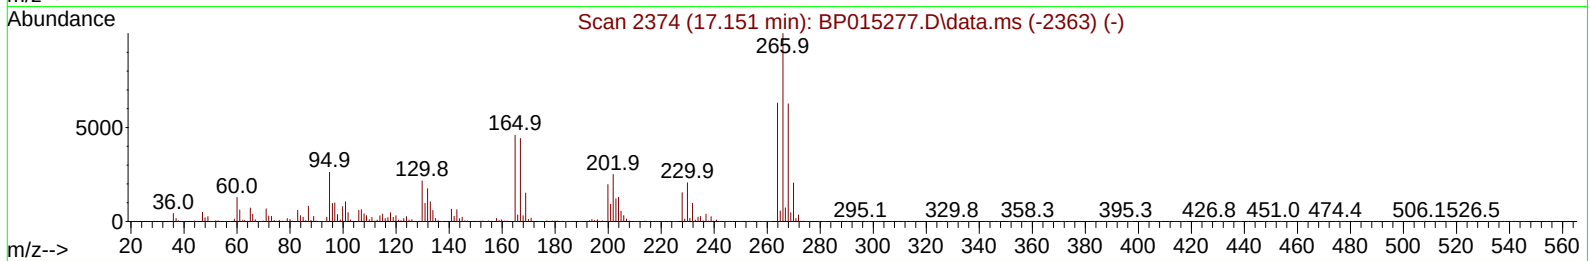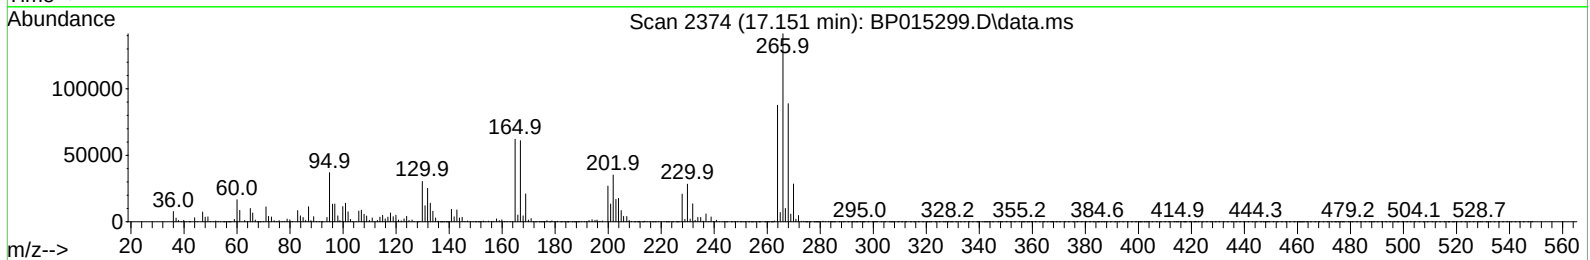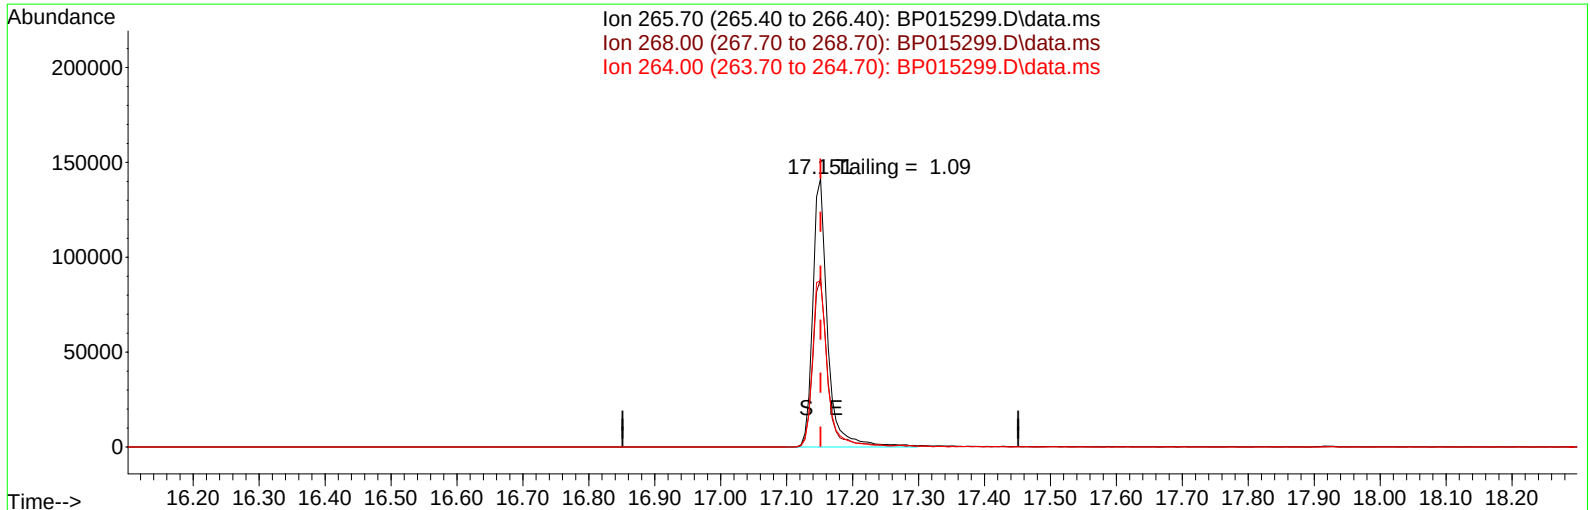

TIC: BP015299.D\data.ms

(70) Pentachlorophenol (C)

17.151min (+ 0.000) 459029.29 ng




response 221004

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	62.79
264.00	63.00	61.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052623\
 Data File : BP015299.D
 Acq On : 26 May 2023 07:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 26 16:54:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 25 01:41:43 2023
 Response via : Initial Calibration

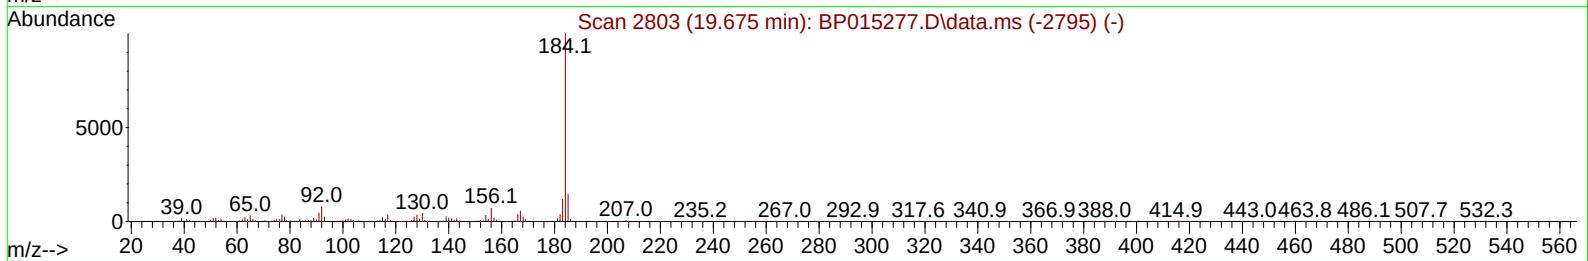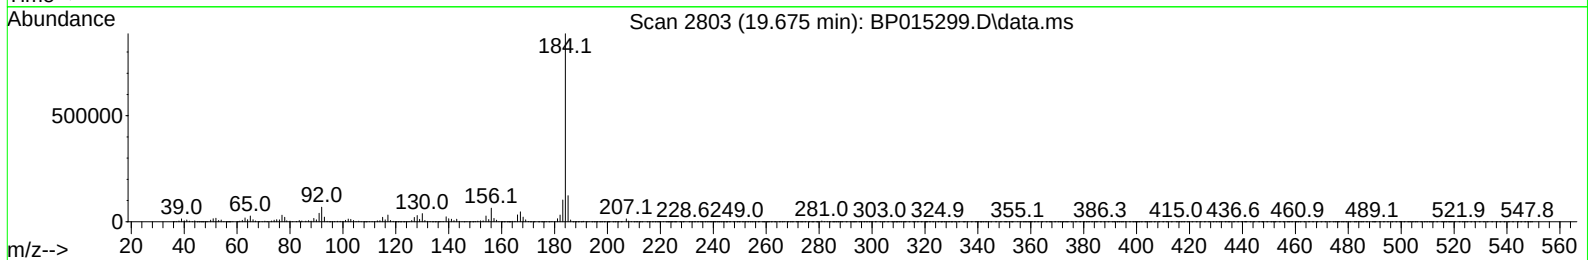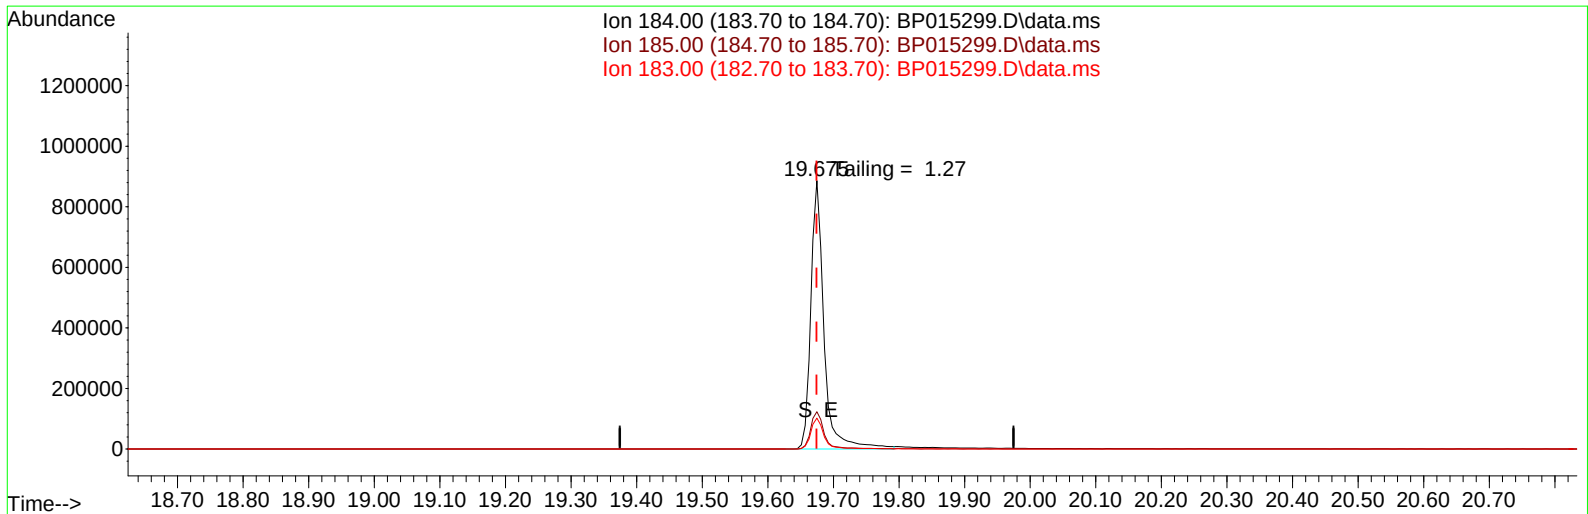

TIC: BP015299.D\data.ms

(77) Benzidine

19.675min (+ 0.000) 236942.12 ng

response 1245681

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.91
183.00	11.70	11.54
0.00	0.00	0.00