
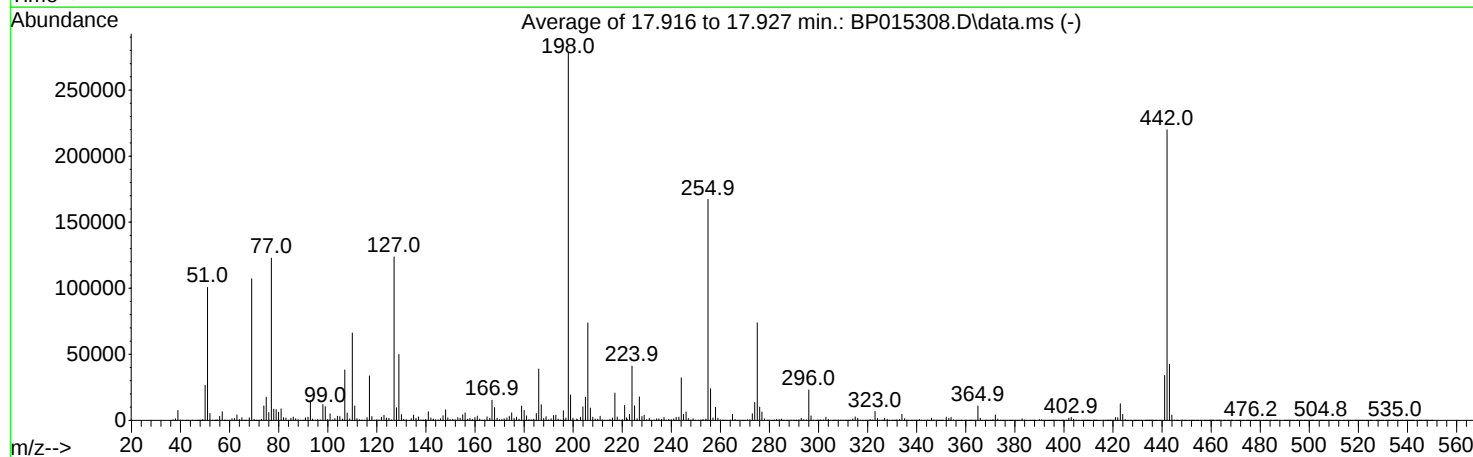


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052623\
Data File : BP015308.D
Acq On : 26 May 2023 14:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 25 01:41:43 2023

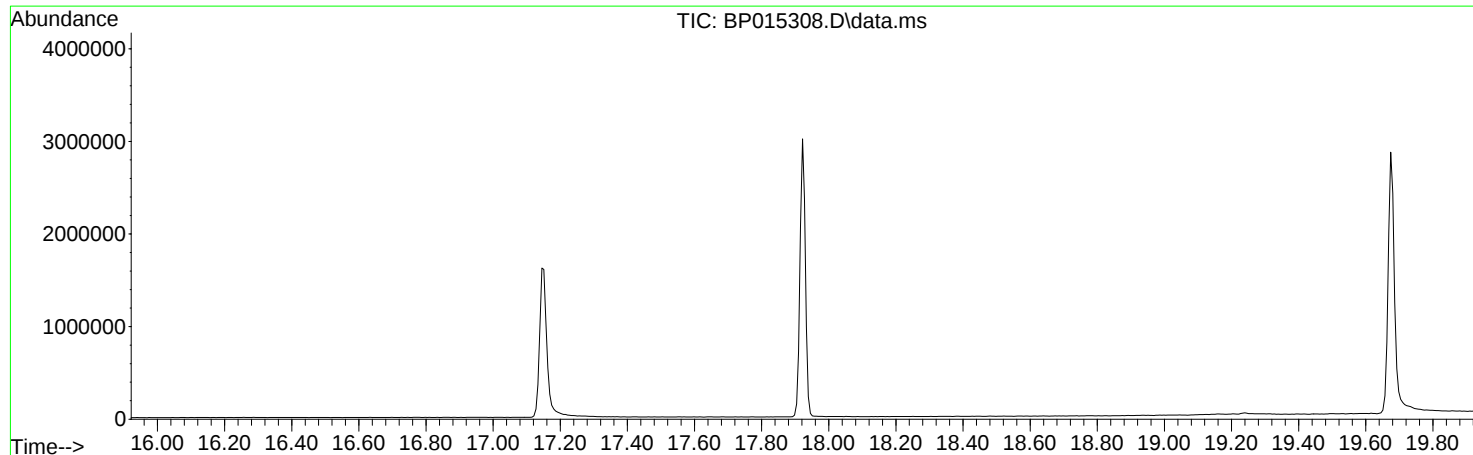

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2496

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	36.1	100640	PASS
68	69	0.00	2	1.9	1984	PASS
69	198	0.00	100	38.5	107195	PASS
70	69	0.00	2	0.6	689	PASS
127	198	10	80	44.4	123752	PASS
197	198	0.00	2	0.6	1779	PASS
198	198	100	100	100.0	278443	PASS
199	198	5	9	6.9	19264	PASS
275	198	10	60	26.5	73824	PASS
365	198	1	100	3.9	10958	PASS
441	198	0.01	100	12.2	34091	PASS
442	442	100	100	100.0	219949	PASS
443	442	15	24	19.3	42477	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/26/2023	BNA_P	<u>BP015308.D</u>
Compound Name	Response	Retention Time
DDT	847648	20.868
DDD	13497	20.439
DDE	509	19.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14006	861654	1.63

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052623\
 Data File : BP015308.D
 Acq On : 26 May 2023 14:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 26 15:57:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 25 01:41:43 2023
 Response via : Initial Calibration

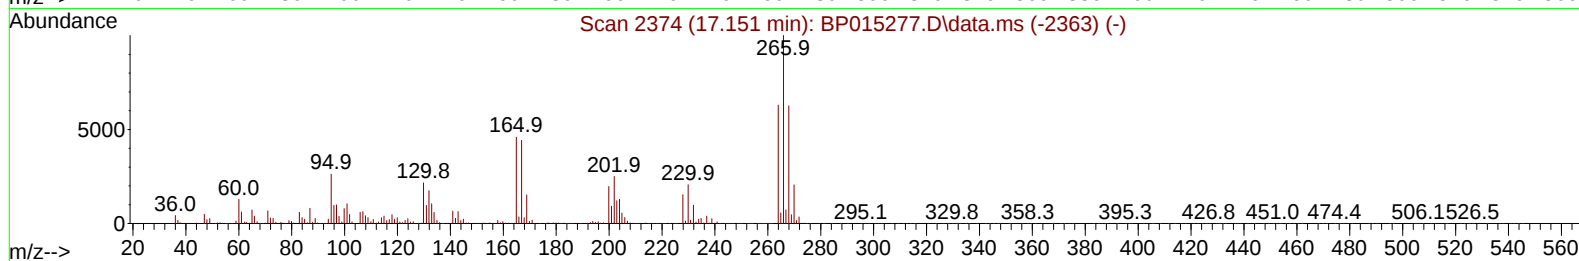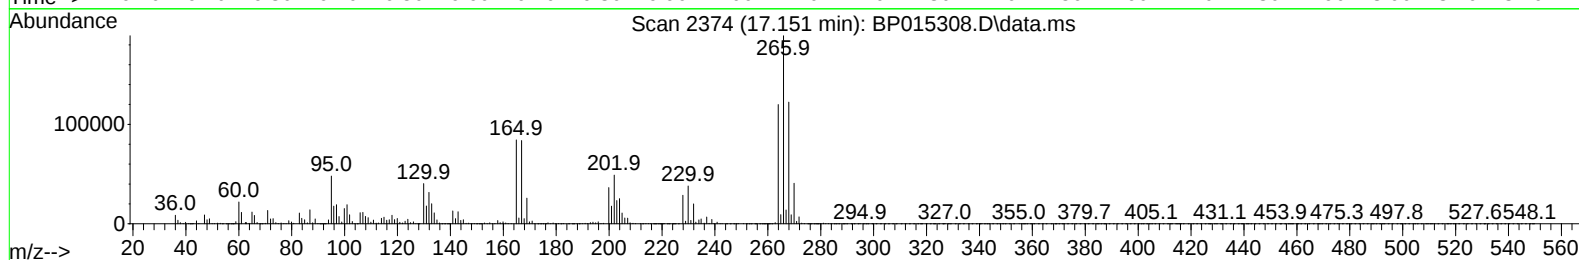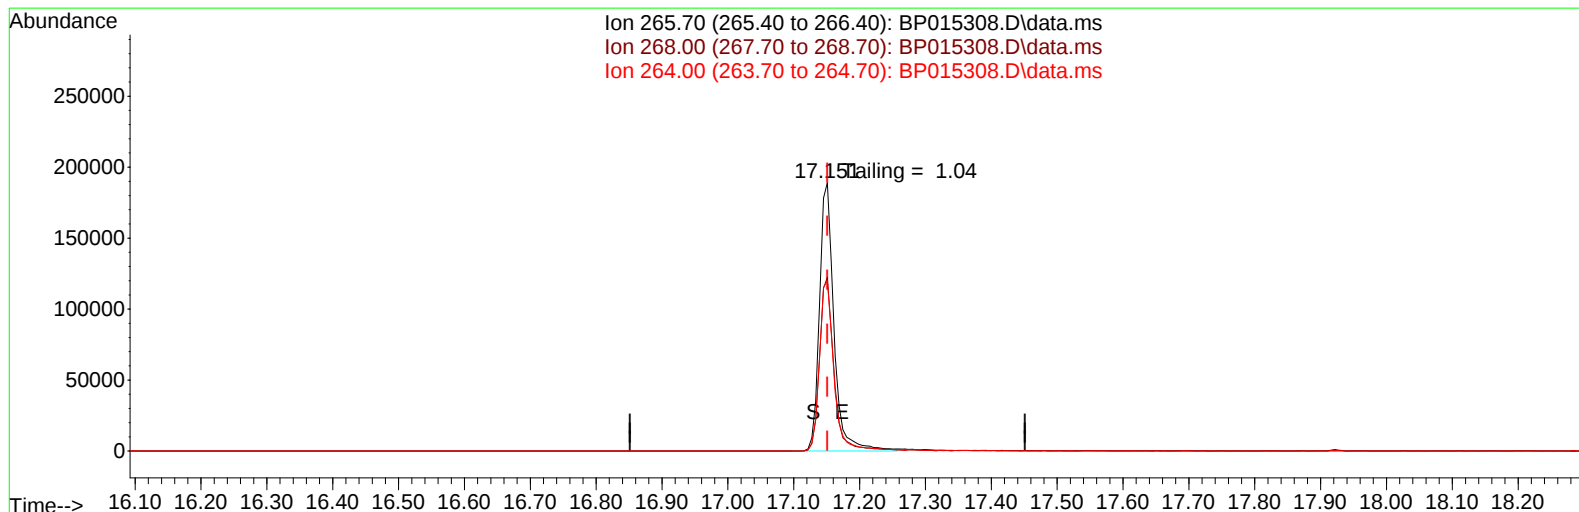

TIC: BP015308.D\data.ms

(70) Pentachlorophenol (C)

17.151min (-0.000) 157785.78 ng




response 290994

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	64.73
264.00	63.00	63.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052623\
Data File : BP015308.D
Acq On : 26 May 2023 14:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 26 15:57:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 01:41:43 2023
Response via : Initial Calibration

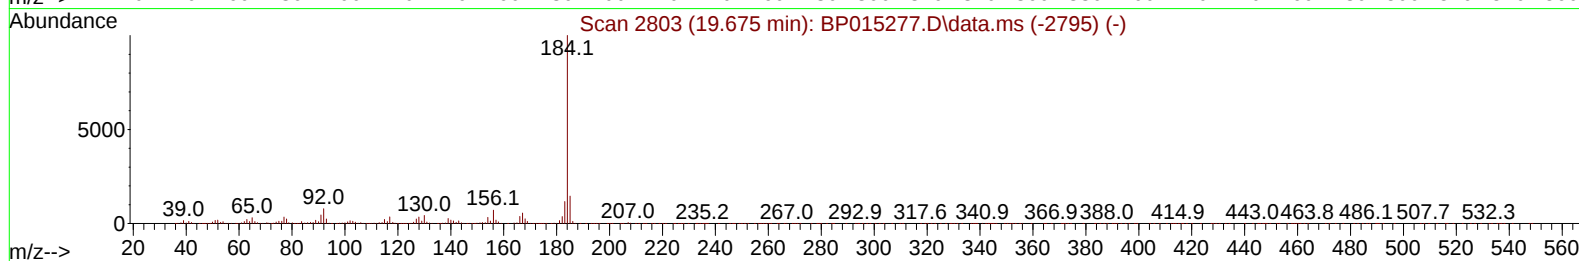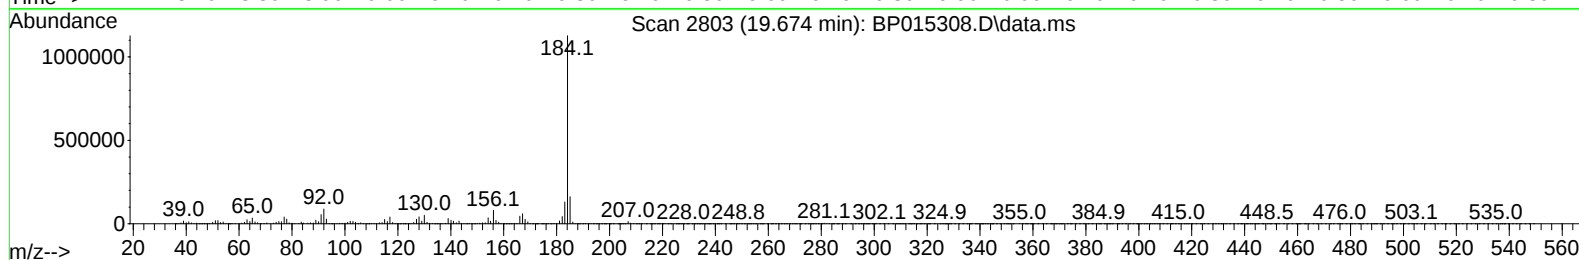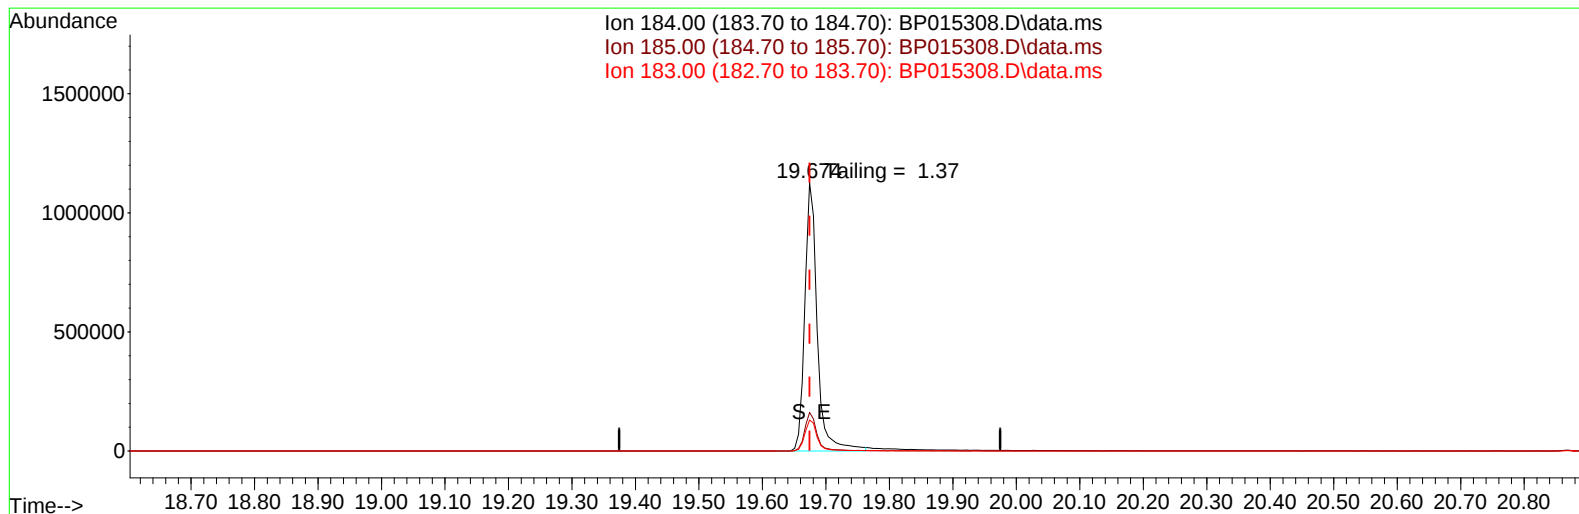

TIC: BP015308.D\data.ms

(77) Benzidine

19.674min (-0.000) 169751.74 ng

response 1594026

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.37
183.00	11.70	11.56
0.00	0.00	0.00