

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052722\
 Data File : BP010573.D
 Acq On : 27 May 2022 09:17
 Operator : CG/JU
 Sample : PB145094BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK094

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010573.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	39	42	48	rBV	34544	46704	1.17%	0.118%
2	3.752	110	113	137	rBV	457284	862225	21.51%	2.178%
3	4.075	165	168	172	rVB4	9759	13856	0.35%	0.035%
4	4.546	246	248	254	rVB5	3184	4294	0.11%	0.011%
5	7.052	667	674	686	rBV	572361	990703	24.72%	2.503%
6	7.211	695	701	716	rVB	477592	809201	20.19%	2.044%
7	7.417	727	736	748	rBV	599215	1021580	25.49%	2.581%
8	7.881	807	815	829	rBV	544927	889044	22.18%	2.246%
9	8.593	929	936	953	rBV	738853	1287010	32.11%	3.251%
10	8.922	990	992	999	rVB7	2221	4102	0.10%	0.010%
11	9.040	1005	1012	1025	rBV	638862	1115876	27.84%	2.819%
12	9.763	1126	1135	1149	rBV	518832	910643	22.72%	2.300%
13	10.305	1220	1227	1244	rBV	655788	1257926	31.39%	3.178%
14	10.681	1283	1291	1306	rBV	762908	1316651	32.85%	3.326%
15	10.822	1308	1315	1328	rBV	515933	1073394	26.78%	2.712%
16	12.293	1560	1565	1572	rBV3	11292	23116	0.58%	0.058%
17	13.928	1833	1843	1856	rBV	1462537	2206662	55.06%	5.574%
18	14.034	1859	1861	1866	rVB5	4863	6697	0.17%	0.017%
19	14.204	1883	1890	1907	rBV	1535027	2432270	60.69%	6.144%
20	14.516	1935	1943	1955	rBV	1221536	1867735	46.61%	4.718%
21	14.722	1969	1978	2000	rBV	326785	864971	21.58%	2.185%
22	15.157	2048	2052	2055	rBV6	2800	4194	0.10%	0.011%
23	15.510	2105	2112	2127	rBV	2104927	3086594	77.02%	7.797%
24	15.634	2127	2133	2149	rVV	603186	970553	24.22%	2.452%
25	15.751	2149	2153	2159	rVB	27666	45019	1.12%	0.114%
26	16.198	2223	2229	2233	rBV9	2743	6717	0.17%	0.017%
27	16.298	2241	2246	2251	rVB7	8308	11003	0.27%	0.028%
28	16.945	2353	2356	2361	rVB6	4568	6121	0.15%	0.015%
29	17.069	2372	2377	2381	rBV7	3148	5462	0.14%	0.014%
30	17.269	2403	2411	2421	rBV	1571177	2286980	57.07%	5.777%
31	17.369	2421	2428	2443	rVV	2380163	3465839	86.48%	8.755%
32	17.945	2520	2526	2529	rBV7	2514	5030	0.13%	0.013%
33	18.175	2559	2565	2570	rBV10	10349	26658	0.67%	0.067%
34	19.181	2732	2736	2744	rVB4	28822	38749	0.97%	0.098%
35	19.245	2744	2747	2757	rBV2	22748	42867	1.07%	0.108%
36	19.604	2801	2808	2820	rBV	2939723	4007562	100.00%	10.124%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052722\
Data File : BP010573.D
Acq On : 27 May 2022 09:17
Operator : CG/JU
Sample : PB145094BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK094

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Title : SVOA CALIBRATION

37	21.351	3100	3105	3120	rBV	1408957	2153657	53.74%	5.440%
38	23.616	3483	3490	3505	rBV2	1294694	2753403	68.71%	6.956%
39	23.774	3510	3517	3530	rVB2	741664	1664660	41.54%	4.205%




Sum of corrected areas: 39585728

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052722\
Data File : BP010573.D
Acq On : 27 May 2022 09:17
Operator : CG/JU
Sample : PB145094BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK094

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

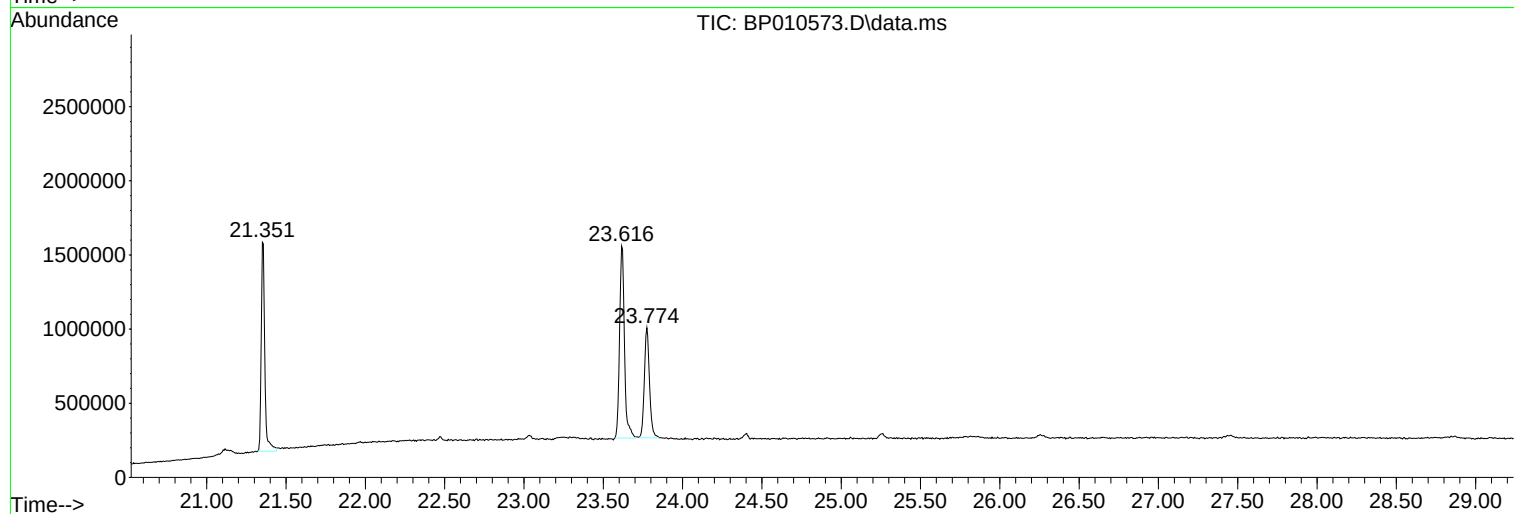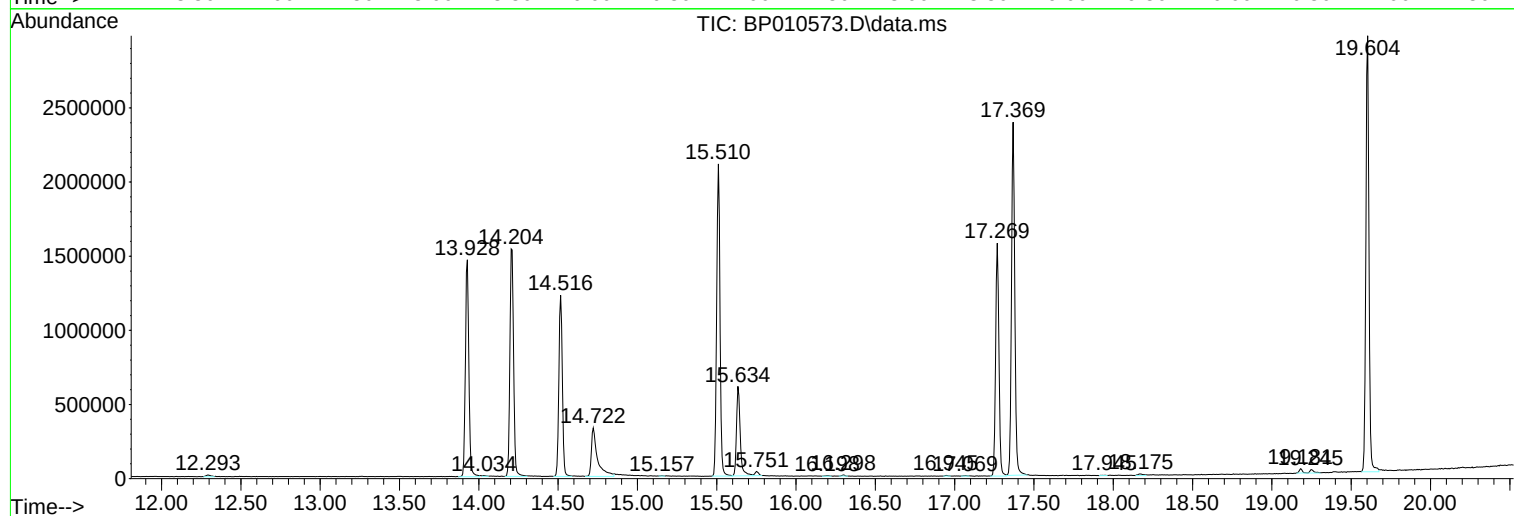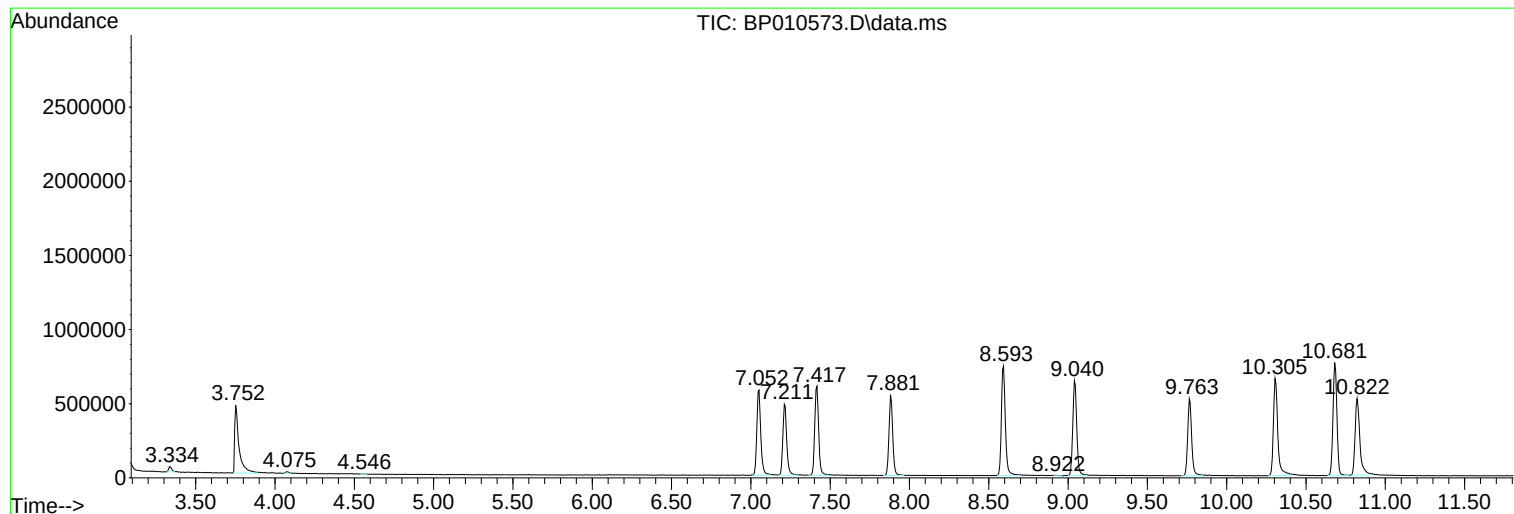

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052722\
Data File : BP010573.D
Acq On : 27 May 2022 09:17
Operator : CG/JU
Sample : PB145094BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK094

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052722\
Data File : BP010573.D
Acq On : 27 May 2022 09:17
Operator : CG/JU
Sample : PB145094BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK094

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------