

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052722\
 Data File : BP010578.D
 Acq On : 27 May 2022 13:31
 Operator : CG/JU
 Sample : PB145142BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK142

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010578.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	39	42	49	rVB	28000	39958	1.06%	0.110%
2	3.752	109	113	131	rBV	377929	724079	19.22%	1.990%
3	4.075	165	168	171	rVB2	7551	8821	0.23%	0.024%
4	7.046	666	673	689	rBV	505634	857662	22.76%	2.357%
5	7.211	694	701	716	rVV	423716	694042	18.42%	1.907%
6	7.411	726	735	752	rBV	515851	871635	23.13%	2.395%
7	7.881	807	815	830	rBV	449830	759334	20.15%	2.087%
8	8.587	928	935	950	rBV	647041	1119092	29.70%	3.075%
9	9.040	1004	1012	1025	rVV	546862	982520	26.08%	2.700%
10	9.763	1128	1135	1148	rBV	443574	786415	20.87%	2.161%
11	10.305	1219	1227	1254	rBV	568300	1131482	30.03%	3.109%
12	10.681	1283	1291	1307	rVB	650804	1145538	30.40%	3.148%
13	10.816	1307	1314	1336	rBV	462623	981849	26.06%	2.698%
14	12.293	1559	1565	1576	rVV5	10408	24238	0.64%	0.067%
15	13.922	1834	1842	1855	rBV	1296338	1959347	52.00%	5.384%
16	14.204	1882	1890	1903	rBV	1410311	2141446	56.84%	5.884%
17	14.510	1934	1942	1961	rBV	1105457	1646332	43.70%	4.524%
18	14.716	1970	1977	2007	rBV	299883	862808	22.90%	2.371%
19	15.334	2080	2082	2085	rVB4	2973	3812	0.10%	0.010%
20	15.504	2103	2111	2124	rBV	1892861	2783940	73.89%	7.650%
21	15.628	2125	2132	2148	rVV	566761	908178	24.10%	2.496%
22	15.745	2148	2152	2158	rVB	23880	38679	1.03%	0.106%
23	16.287	2240	2244	2249	rBV4	9068	14719	0.39%	0.040%
24	16.939	2349	2355	2358	rBV7	4834	9581	0.25%	0.026%
25	17.057	2370	2375	2376	rBV4	3377	5112	0.14%	0.014%
26	17.263	2402	2410	2419	rBV	1482806	2073435	55.03%	5.697%
27	17.363	2420	2427	2444	rVB	2152848	3159037	83.84%	8.680%
28	18.163	2558	2563	2569	rBV10	10227	23020	0.61%	0.063%
29	19.175	2731	2735	2741	rBV3	26895	37955	1.01%	0.104%
30	19.245	2743	2747	2751	rVB	22766	30223	0.80%	0.083%
31	19.386	2768	2771	2772	rBV3	5583	5995	0.16%	0.016%
32	19.598	2801	2807	2822	rBV	2697169	3767776	100.00%	10.353%
33	21.345	3099	3104	3117	rBV	1403420	2116461	56.17%	5.816%
34	23.610	3482	3489	3506	rVB2	1364517	2925731	77.65%	8.039%
35	23.768	3509	3516	3532	rVB2	786048	1752241	46.51%	4.815%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052722\
Data File : BP010578.D
Acq On : 27 May 2022 13:31
Operator : CG/JU
Sample : PB145142BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK142

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Title : SVOA CALIBRATION




Sum of corrected areas: 36392493

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052722\
Data File : BP010578.D
Acq On : 27 May 2022 13:31
Operator : CG/JU
Sample : PB145142BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK142

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

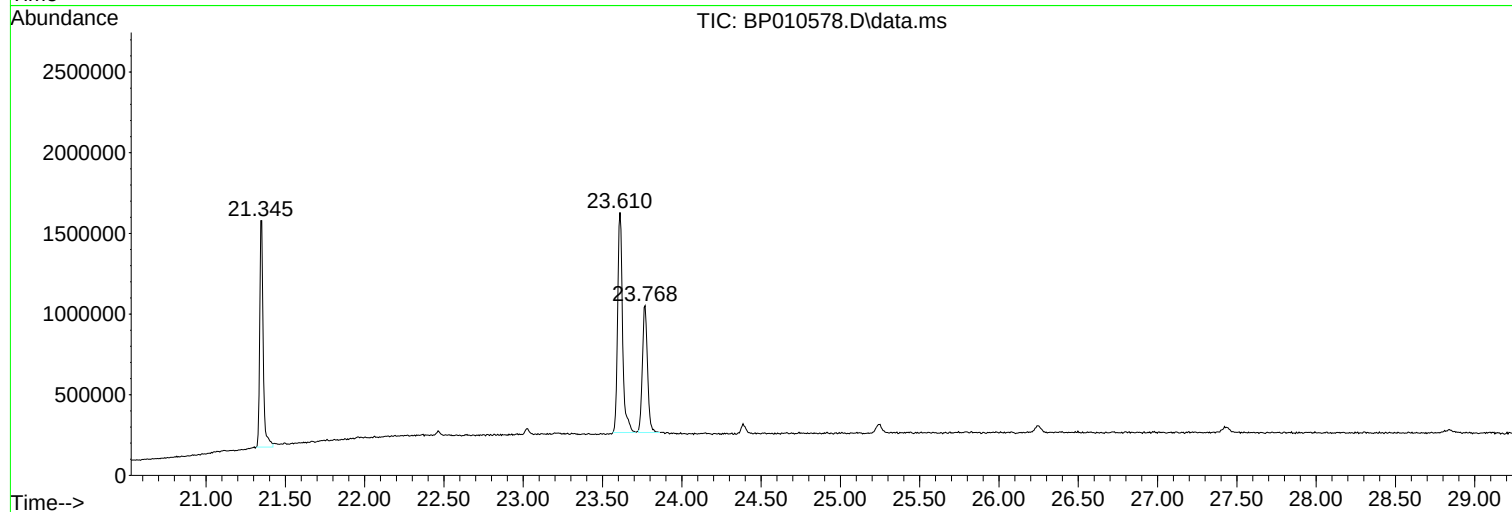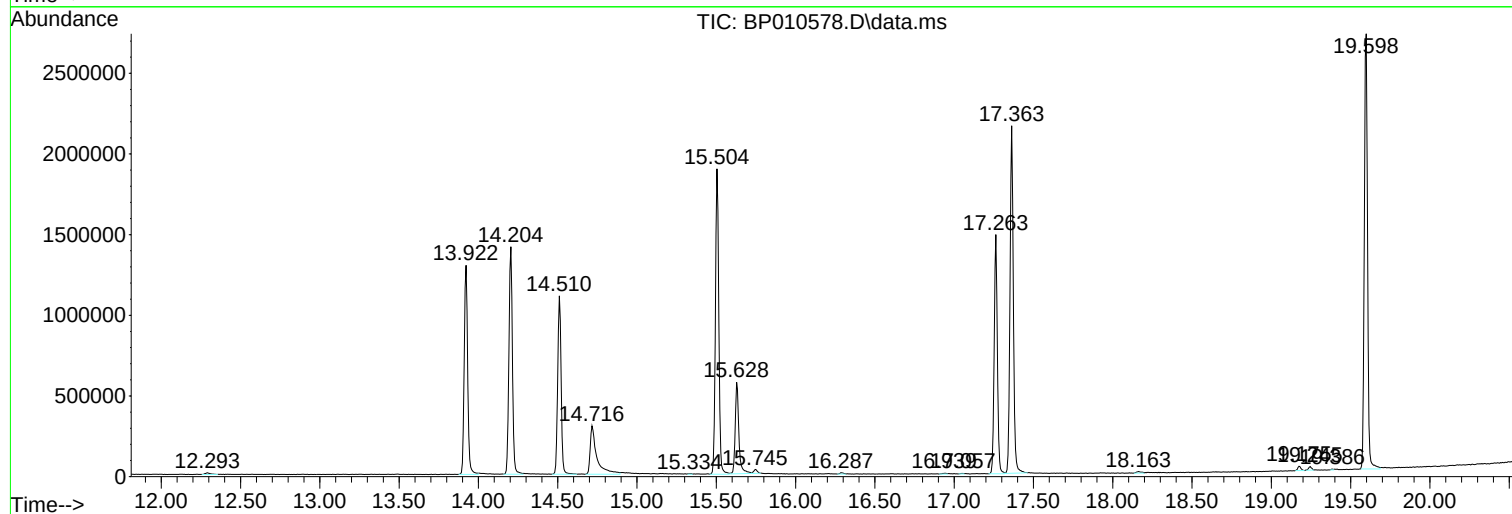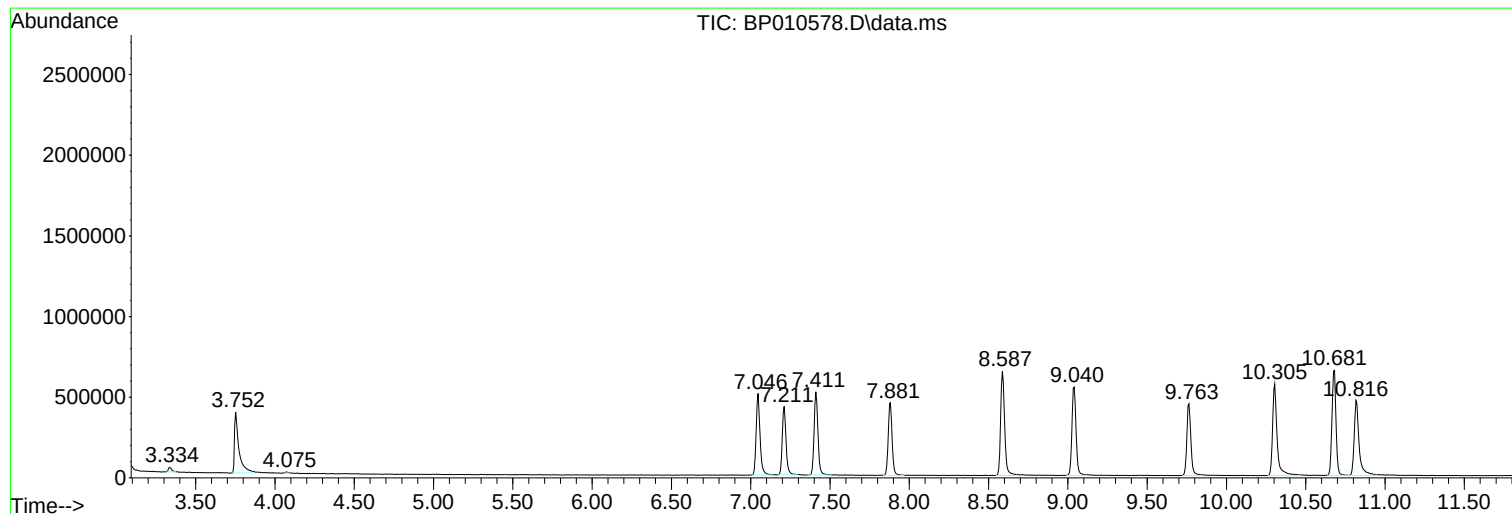

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052722\
Data File : BP010578.D
Acq On : 27 May 2022 13:31
Operator : CG/JU
Sample : PB145142BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK142

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052722\
Data File : BP010578.D
Acq On : 27 May 2022 13:31
Operator : CG/JU
Sample : PB145142BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK142

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------