
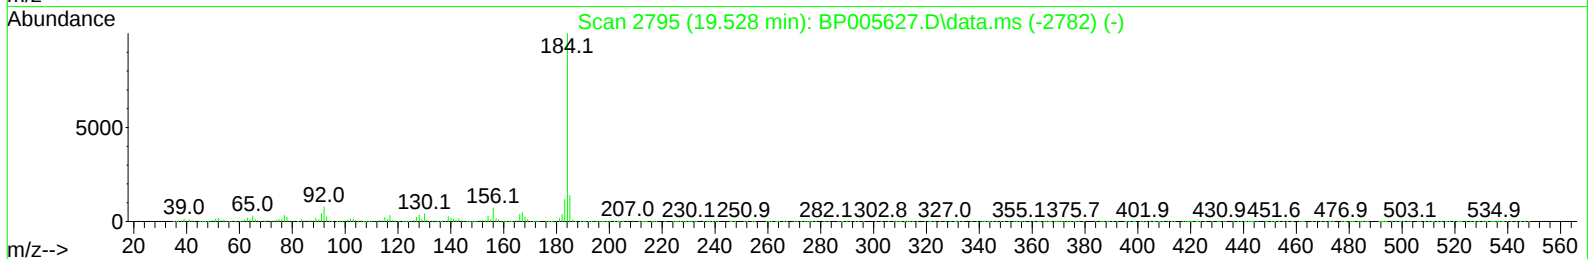
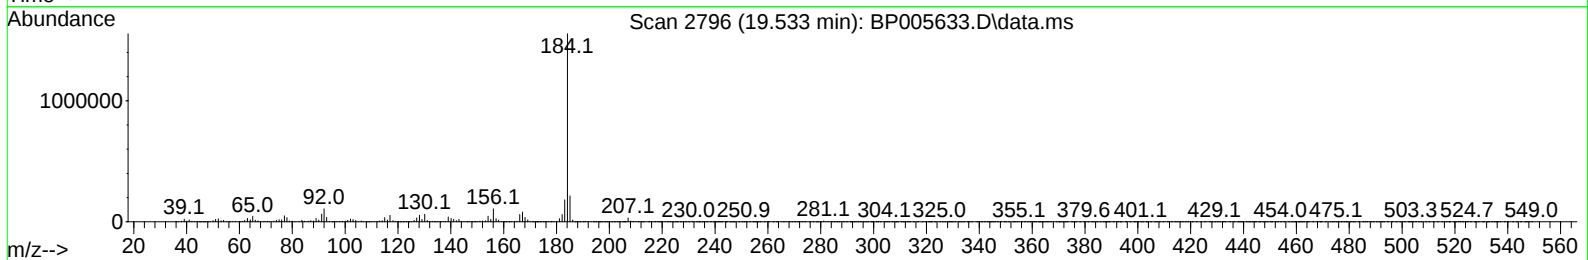


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052821\
 Data File : BP005633.D
 Acq On : 28 May 2021 11:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 11:45:03 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 27 16:11:11 2021
 Response via : Initial Calibration

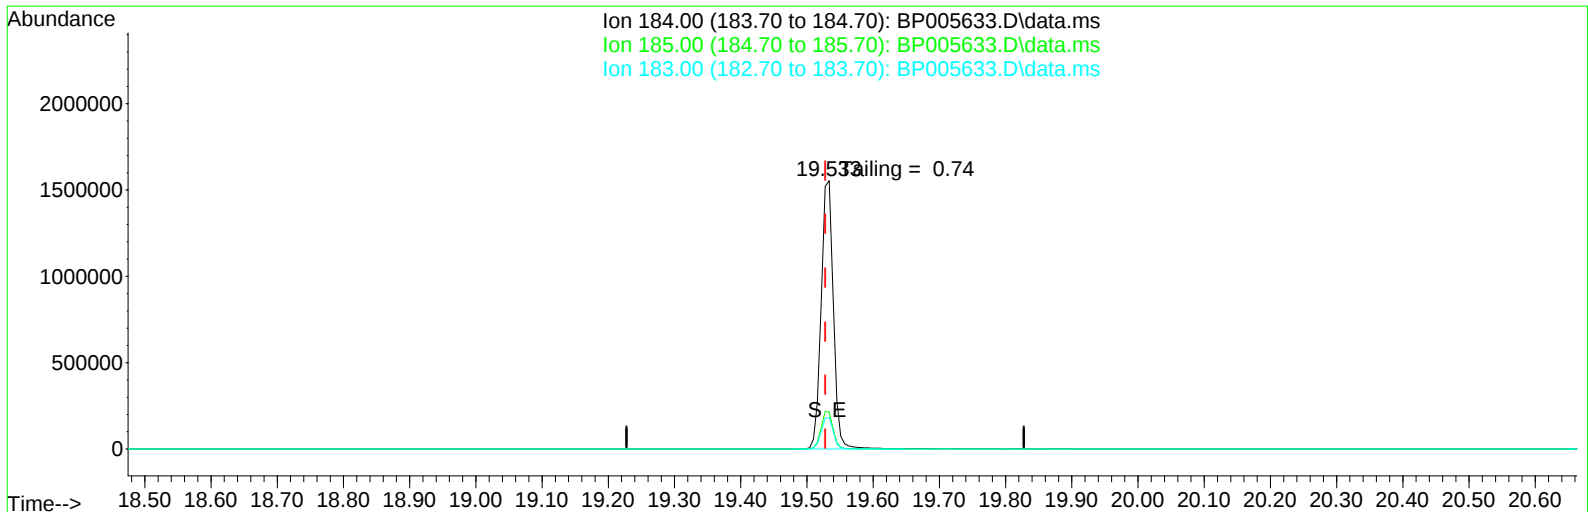

TIC: BP005633.D\data.ms

(77) Benzidine




19.533min (+ 0.006) 5355.65 ng

response 1992414

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.79
183.00	12.30	11.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052821\
Data File : BP005633.D
Acq On : 28 May 2021 11:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 11:45:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 16:11:11 2021
Response via : Initial Calibration

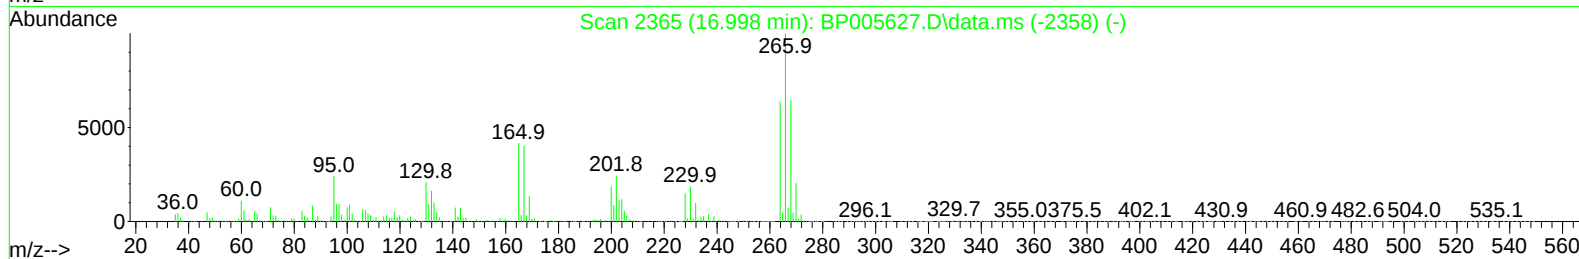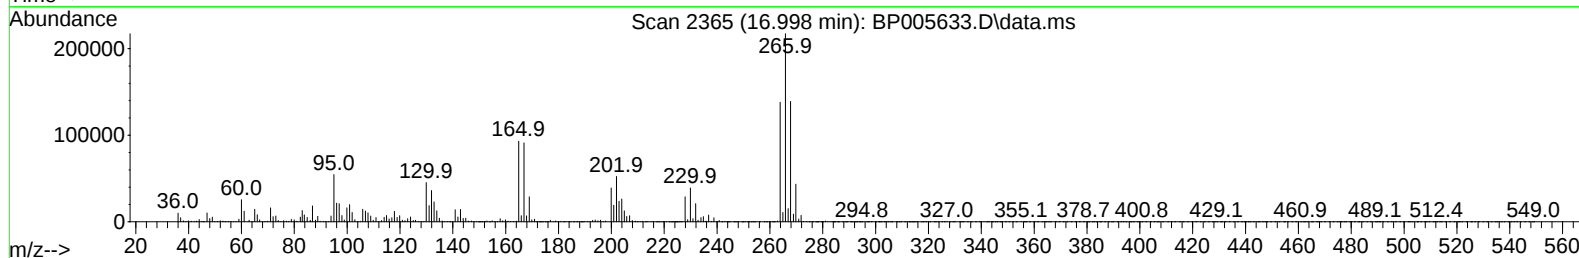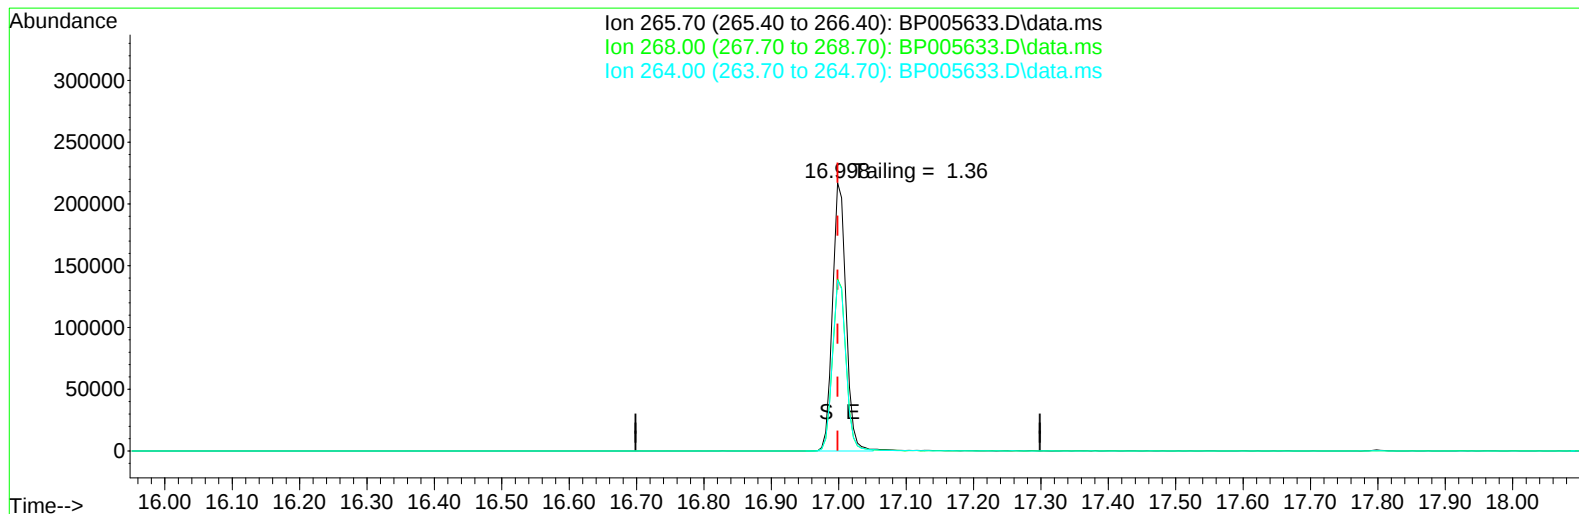

TIC: BP005633.D\data.ms

(70) Pentachlorophenol (C)

16.998min (-0.000) 830347.47 ng

response 304652

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	64.04
264.00	67.10	63.56
0.00	0.00	0.00