
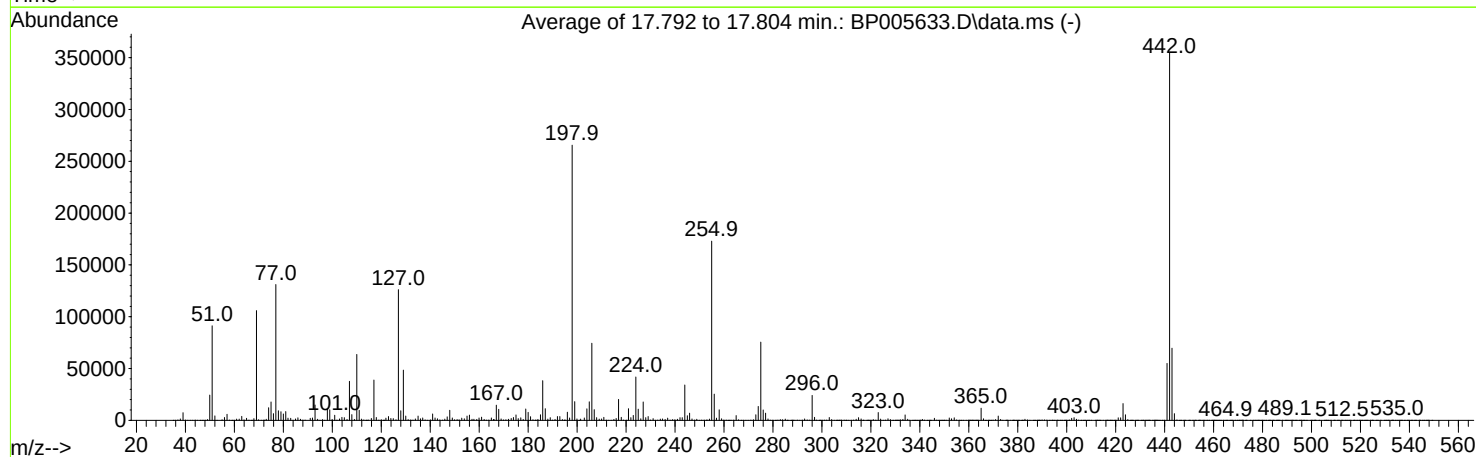


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052821\
 Data File : BP005633.D
 Acq On : 28 May 2021 11:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 27 16:11:11 2021

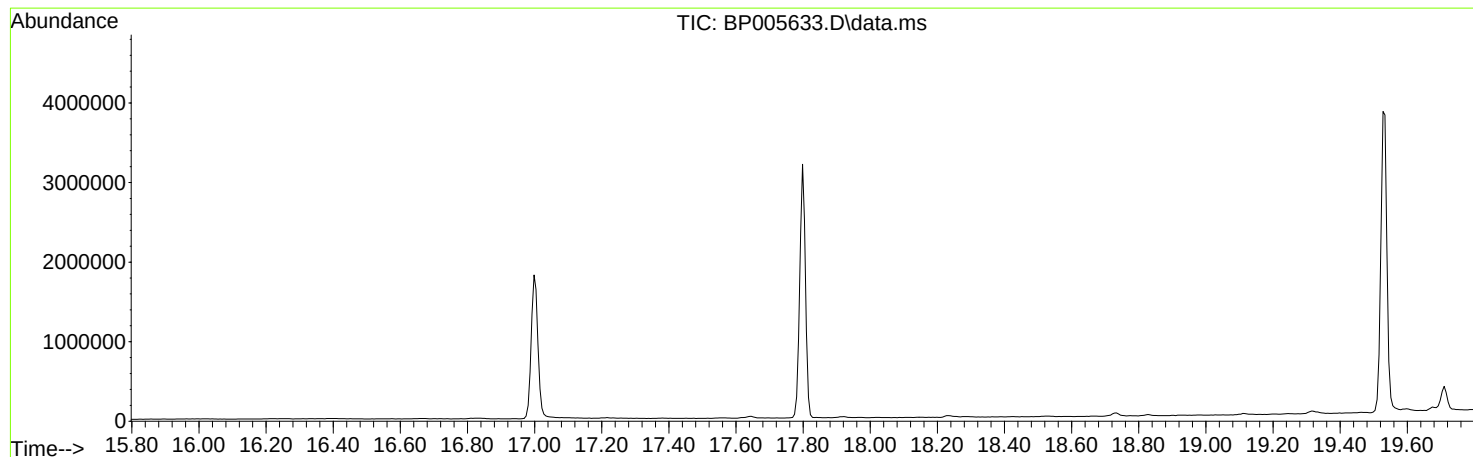

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	91306	PASS
68	69	0.00	2	1.7	1753	PASS
69	198	0.00	100	39.9	105956	PASS
70	69	0.00	2	0.6	619	PASS
127	198	10	80	47.5	126156	PASS
197	198	0.00	2	0.9	2390	PASS
198	198	100	100	100.0	265481	PASS
199	198	5	9	6.8	18136	PASS
275	198	10	60	28.4	75467	PASS
365	198	1	100	4.4	11678	PASS
441	198	0.01	100	20.7	54942	PASS
442	442	100	100	100.0	354944	PASS
443	442	15	24	19.6	69691	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/28/2021	BNA_P	<u>BP005633.D</u>
Compound Name	Response	Retention Time
DDT	953283	20.73
DDD	3508	20.3
DDE	1312	20.3
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4820	958103	0.50

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052821\
 Data File : BP005633.D
 Acq On : 28 May 2021 11:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 28 11:45:03 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 27 16:11:11 2021
 Response via : Initial Calibration

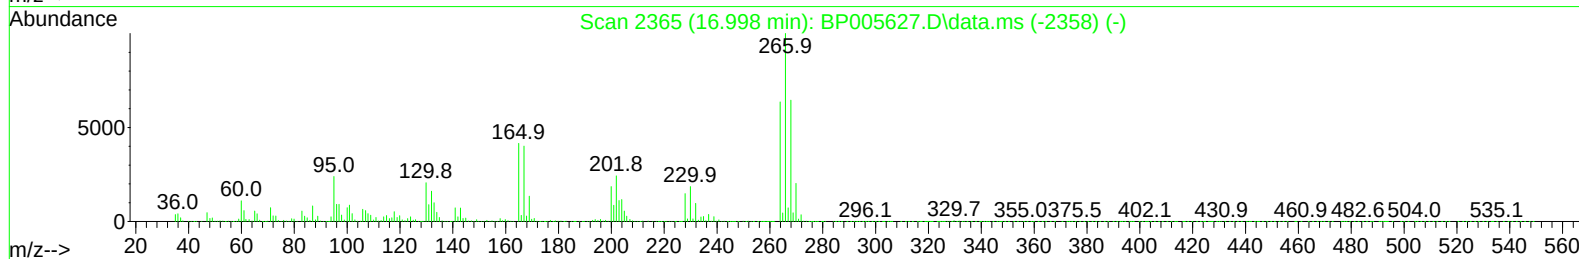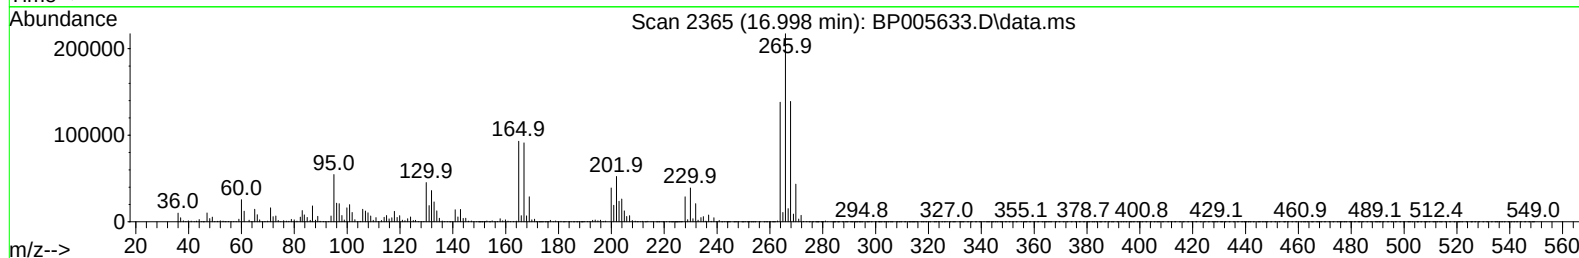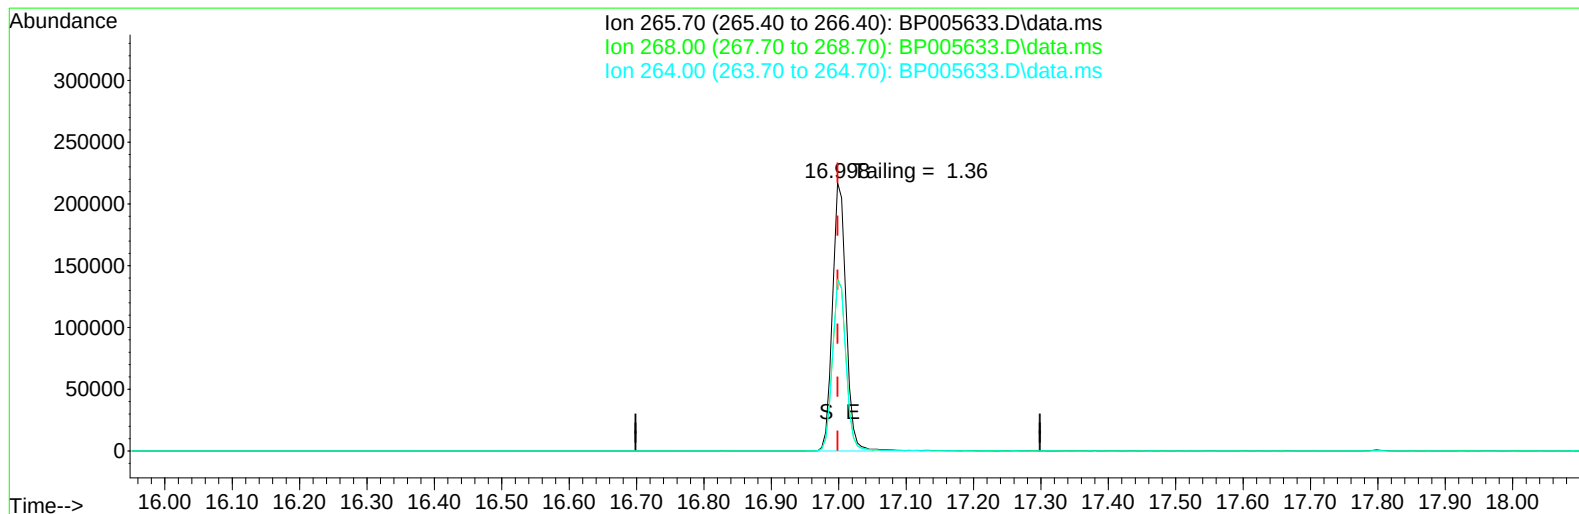

TIC: BP005633.D\data.ms

(70) Pentachlorophenol (C)

16.998min (-0.000) 830347.47 ng




response 304652

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	64.04
264.00	67.10	63.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052821\
 Data File : BP005633.D
 Acq On : 28 May 2021 11:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 28 11:45:03 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 27 16:11:11 2021
 Response via : Initial Calibration

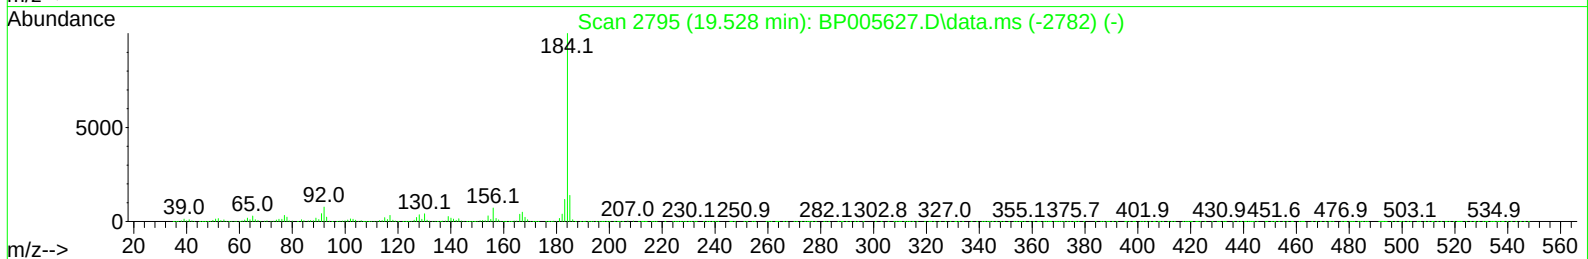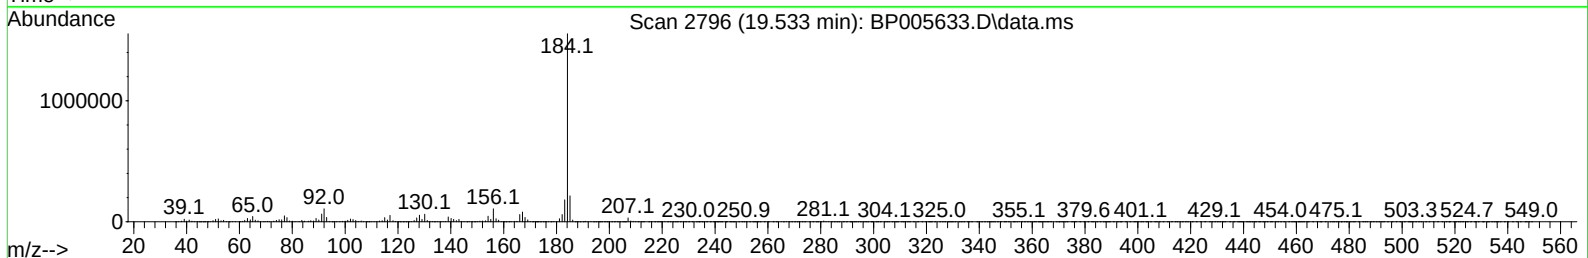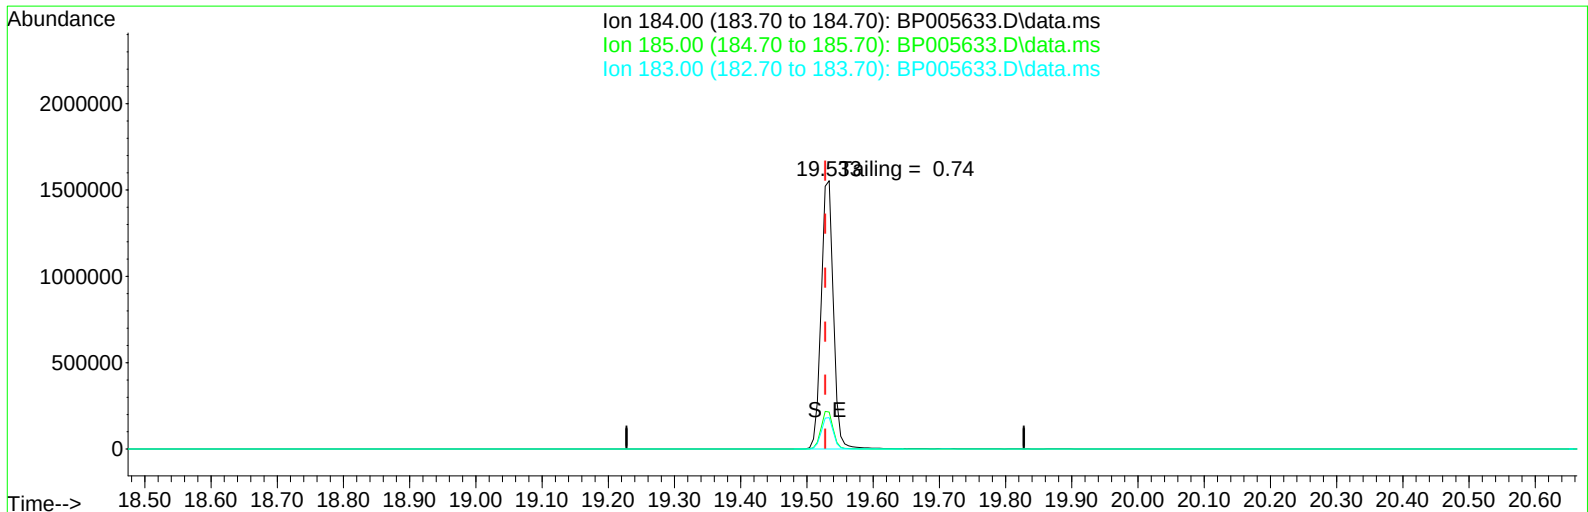

TIC: BP005633.D\data.ms

(77) Benzidine

19.533min (+ 0.006) 5355.65 ng

response 1992414

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.79
183.00	12.30	11.68
0.00	0.00	0.00