
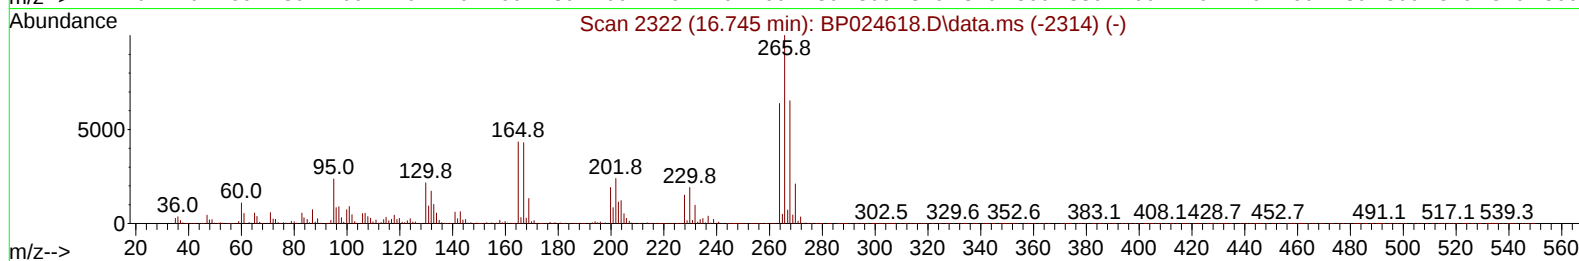
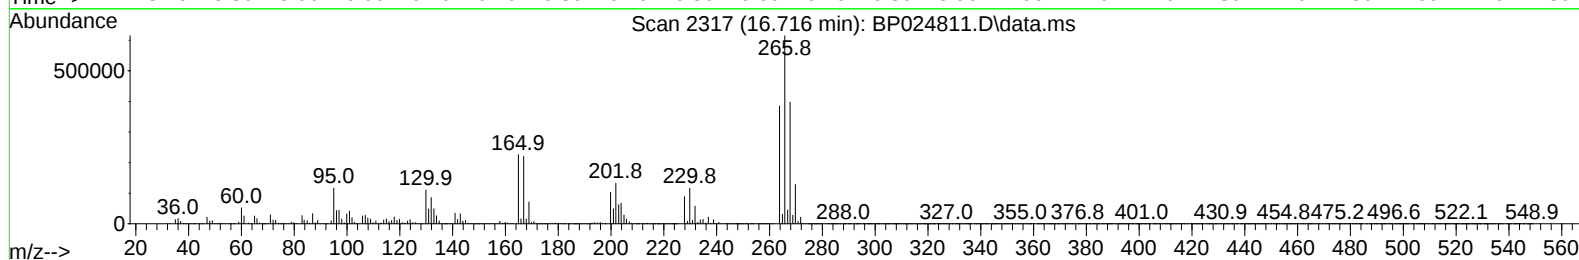


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052825\
Data File : BP024811.D
Acq On : 28 May 2025 11:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 14:29:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 28 14:16:13 2025
Response via : Initial Calibration

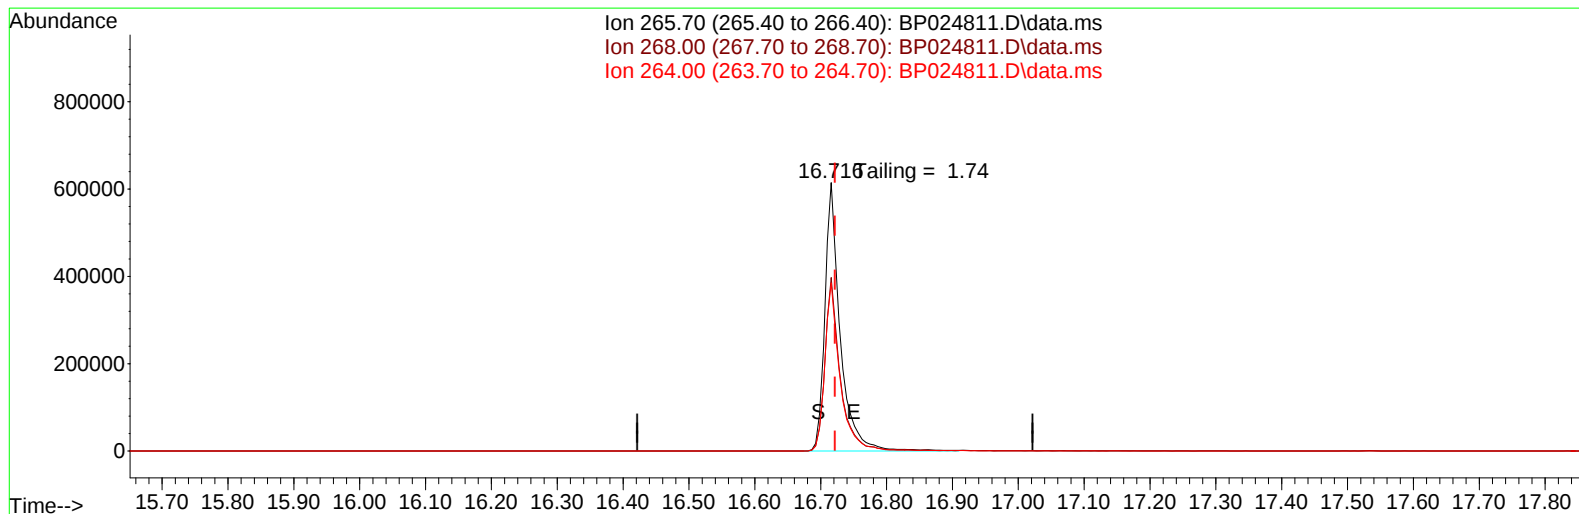

TIC: BP024811.D\data.ms

(70) Pentachlorophenol (C)




16.716min (-0.006) 59299.44 ng

response 989356

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.65
264.00	63.90	62.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052825\
Data File : BP024811.D
Acq On : 28 May 2025 11:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 14:29:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 28 14:16:13 2025
Response via : Initial Calibration

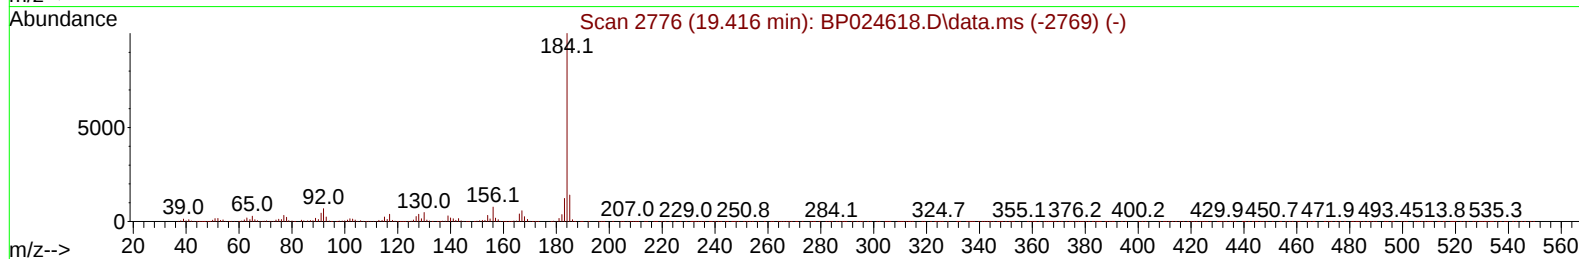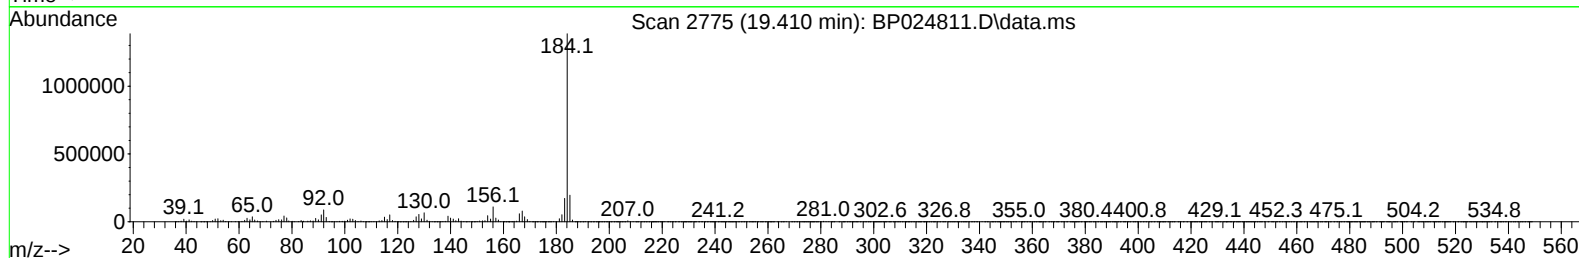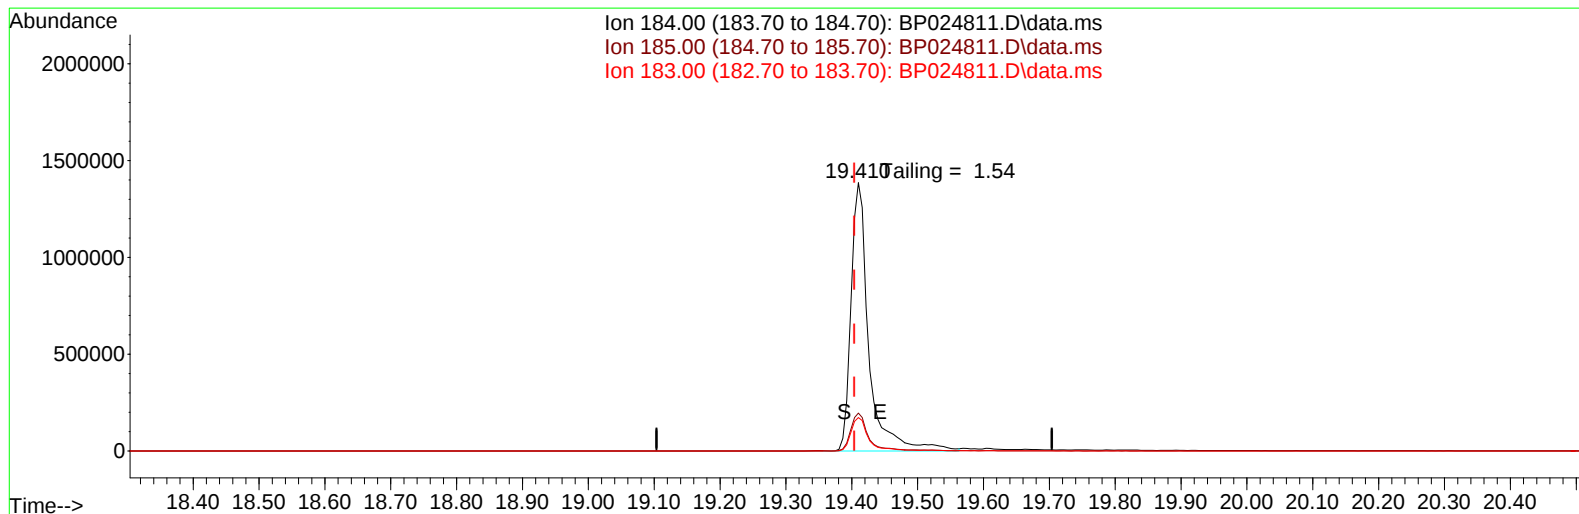

TIC: BP024811.D\data.ms

(77) Benzidine**19.410min (+ 0.006) 5826.15 ng****response 2541907**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.12
183.00	12.30	12.46
0.00	0.00	0.00