
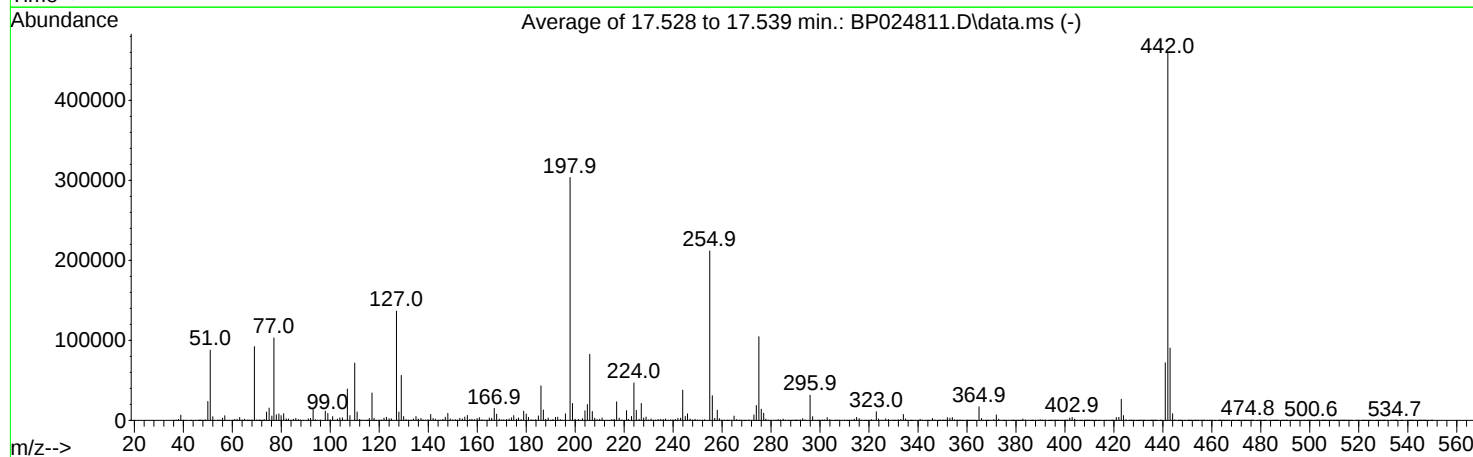


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052825\
Data File : BP024811.D
Acq On : 28 May 2025 11:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 28 14:16:13 2025

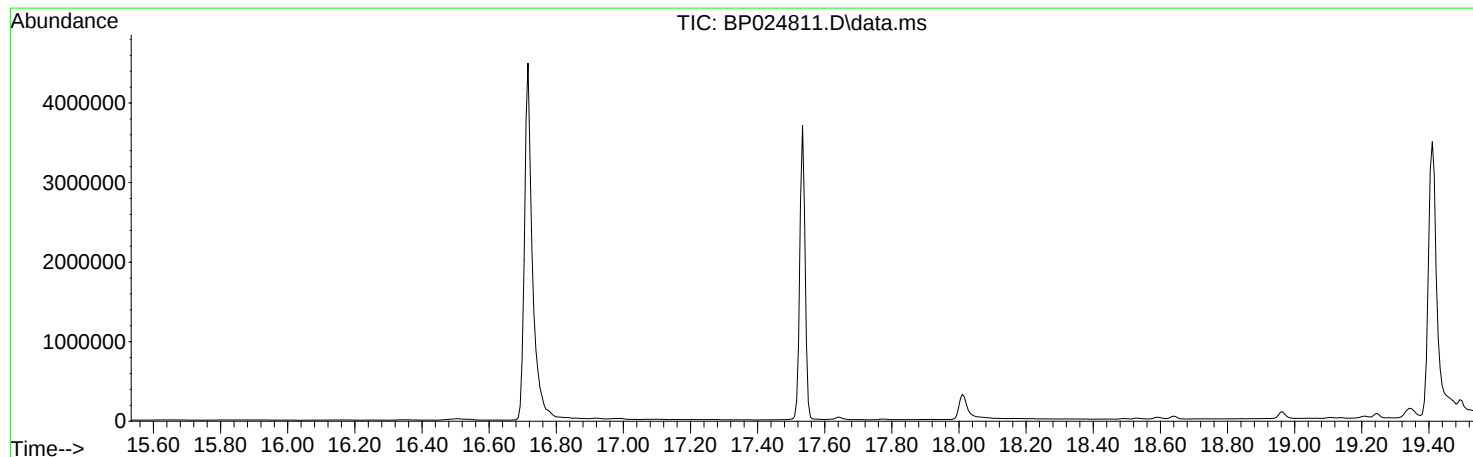




AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	87856	PASS
68	69	0.00	2	0.7	619	PASS
69	198	0.00	100	30.4	92148	PASS
70	69	0.00	2	0.6	562	PASS
127	198	10	80	45.0	136491	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	303569	PASS
199	198	5	9	7.0	21179	PASS
275	198	10	60	34.4	104506	PASS
365	198	1	100	5.6	17036	PASS
441	198	0.01	100	23.7	72085	PASS
442	442	100	100	100.0	459731	PASS
443	442	15	24	19.7	90469	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052825\
Data File : BP024811.D
Acq On : 28 May 2025 11:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 28 14:29:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 28 14:16:13 2025
Response via : Initial Calibration

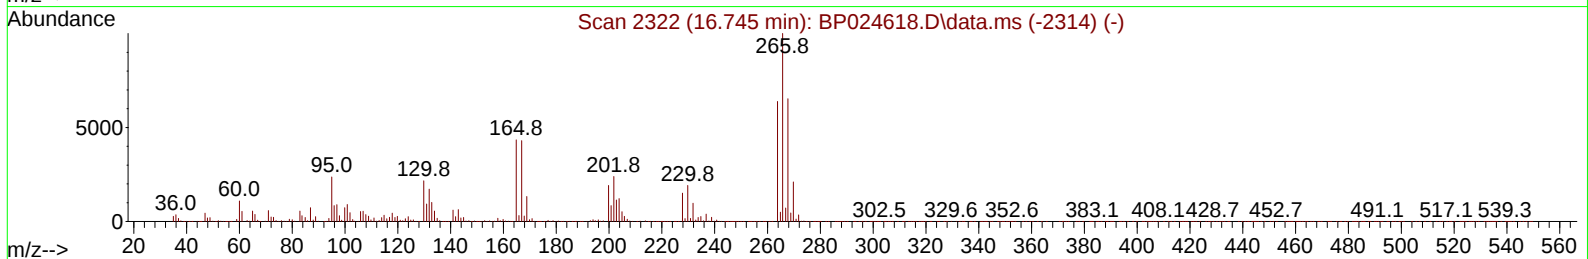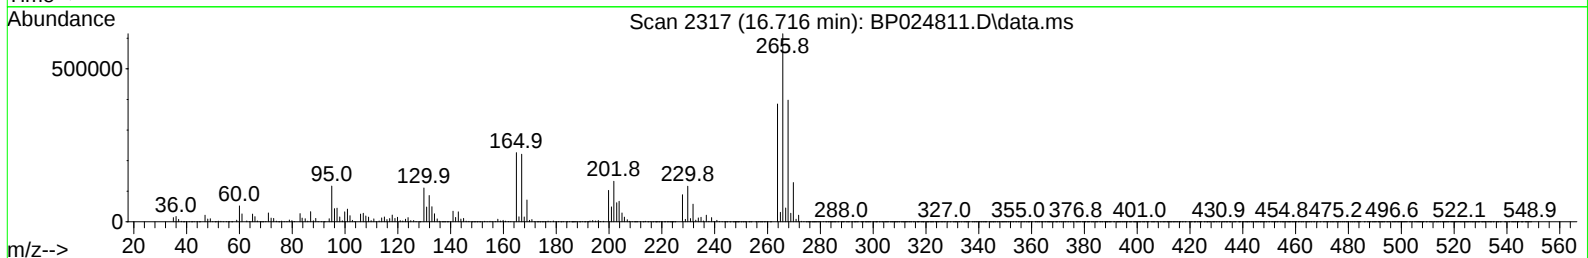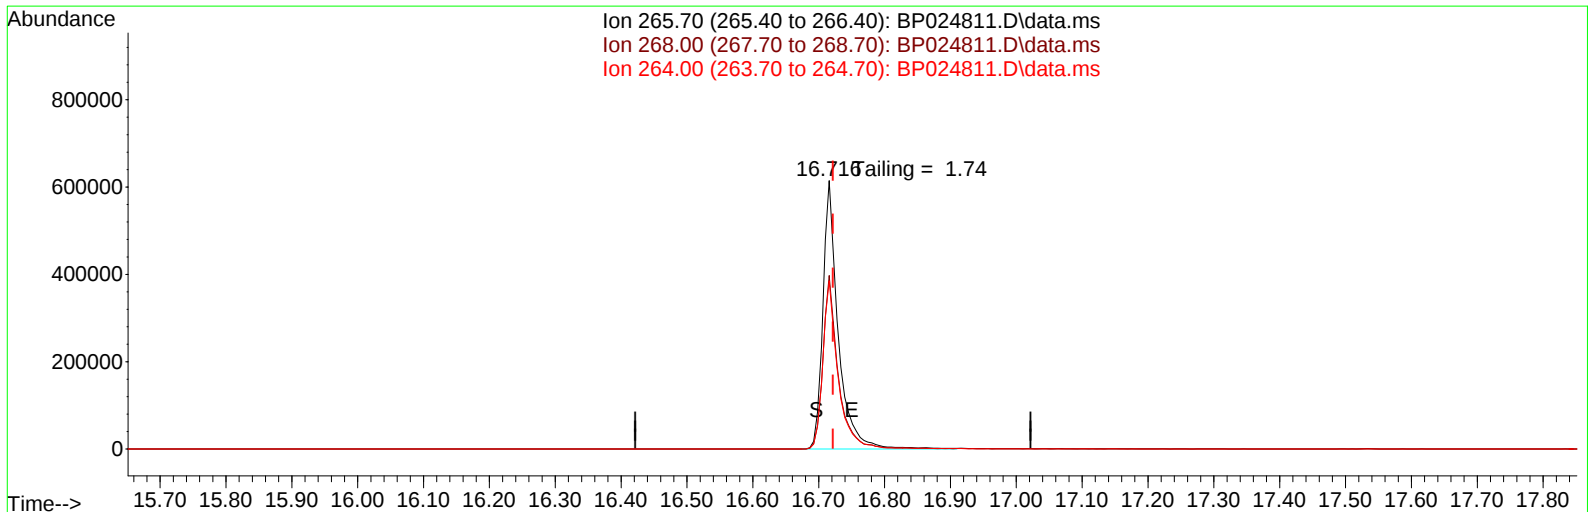

TIC: BP024811.D\data.ms

(70) Pentachlorophenol (C)

16.716min (-0.006) 59299.44 ng




response 989356

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.65
264.00	63.90	62.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052825\
Data File : BP024811.D
Acq On : 28 May 2025 11:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 28 14:29:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 28 14:16:13 2025
Response via : Initial Calibration

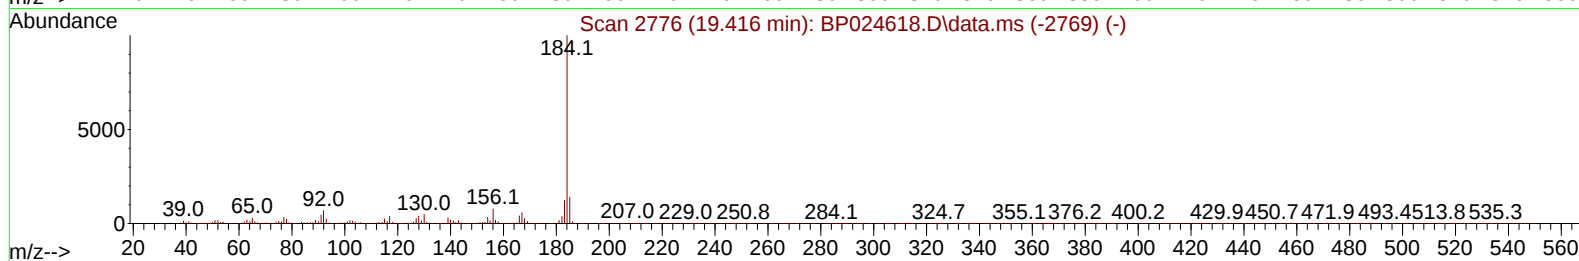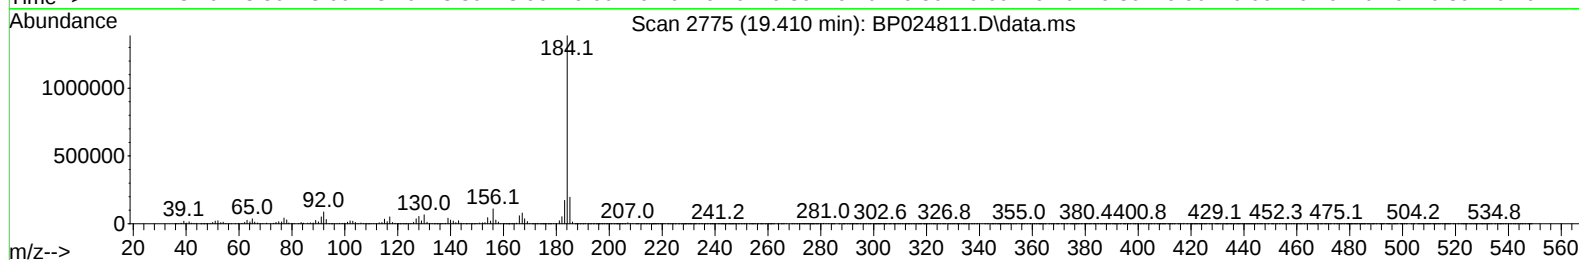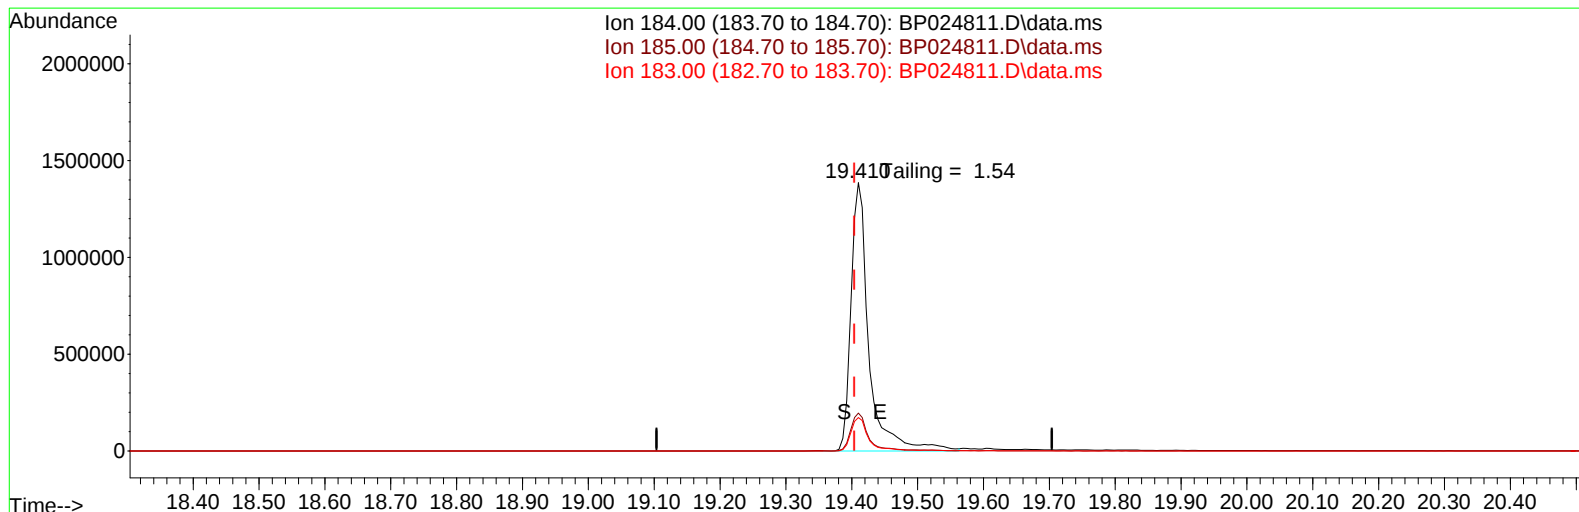

TIC: BP024811.D\data.ms

(77) Benzidine

19.410min (+ 0.006) 5826.15 ng

response 2541907

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.12
183.00	12.30	12.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/28/2025	BNA_P	<u>BP024811.D</u>
Compound Name	Response	Retention Time
DDT	1107244	20.686
DDD	20960	20.239
DDE	3511	19.704
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24471	1131715	2.16

Instrument :
BNA_P
ClientSampleId :
DFTPP