




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060525\
Data File : BP024855.D
Acq On : 05 Jun 2025 15:20
Operator : RC/JU
Sample : PB166618TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB618

Manual IntegrationsAPPROVED

Reviewed By :Rahul Chavli 06/06/2025
Supervised By :Jagrut Upadhyay 06/06/2025

Quant Time: Jun 05 16:56:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060525.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 05 15:37:10 2025
Response via : Initial Calibration

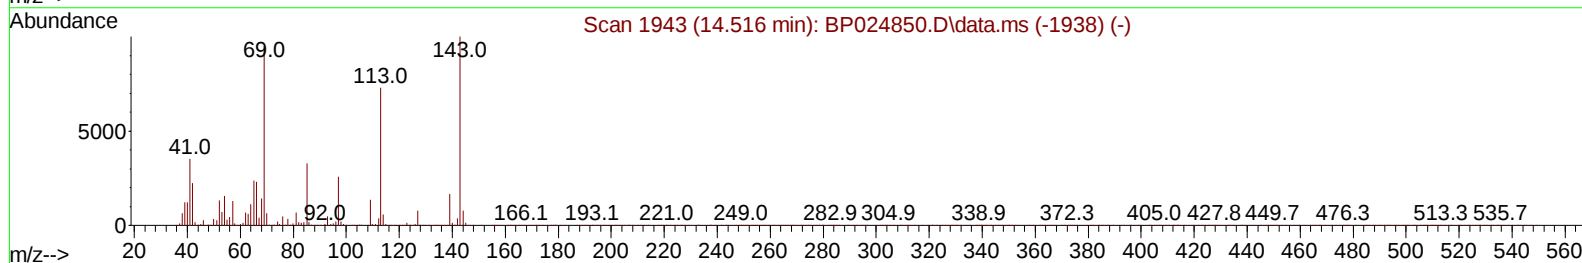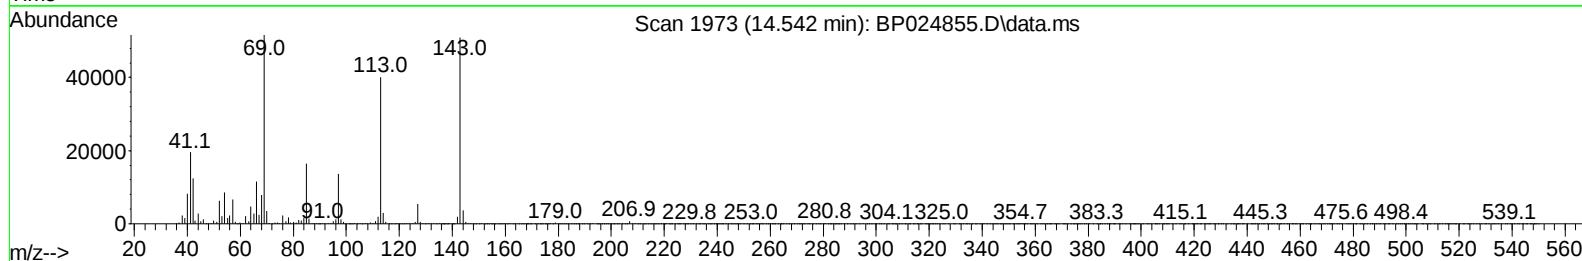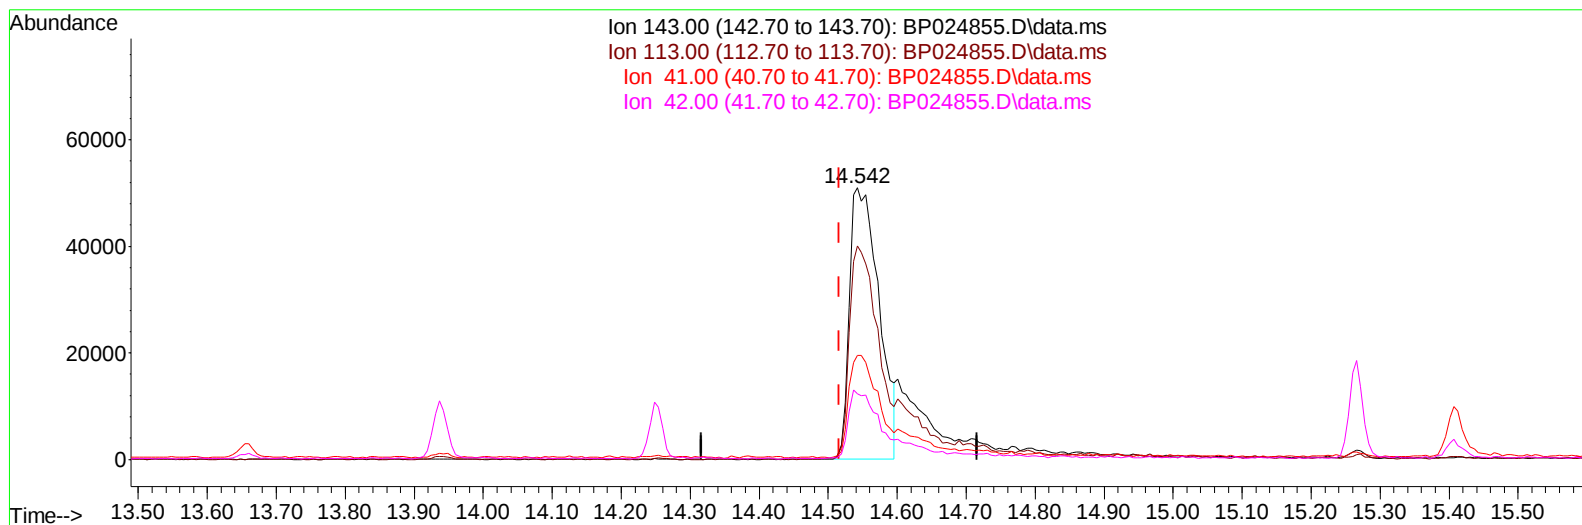

TIC: BP024855.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.542min (+ 0.026) 24.42 ng/u1

response 150974

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	73.10	78.65
41.00	36.00	38.36
42.00	22.80	24.23




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060525\
Data File : BP024855.D
Acq On : 05 Jun 2025 15:20
Operator : RC/JU
Sample : PB166618TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB618

Manual IntegrationsAPPROVED

Quant Time: Jun 05 16:56:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060525.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 05 15:37:10 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 06/06/2025
Supervised By :Jagrut Upadhyay 06/06/2025

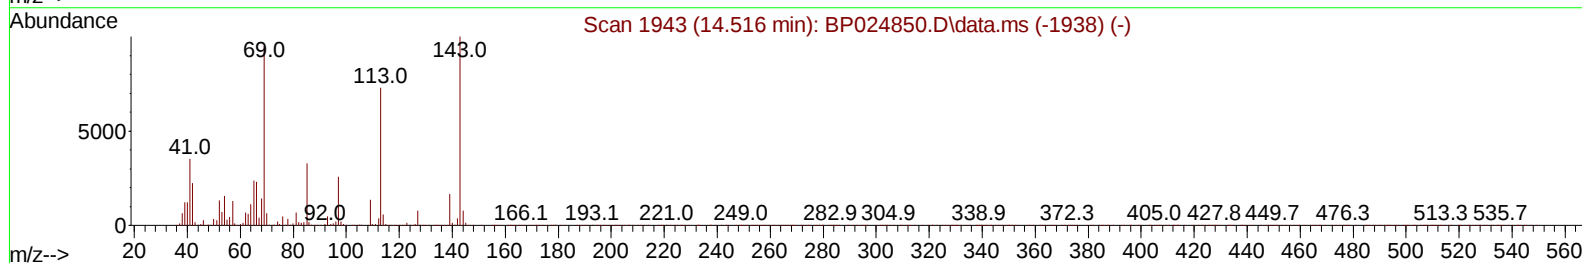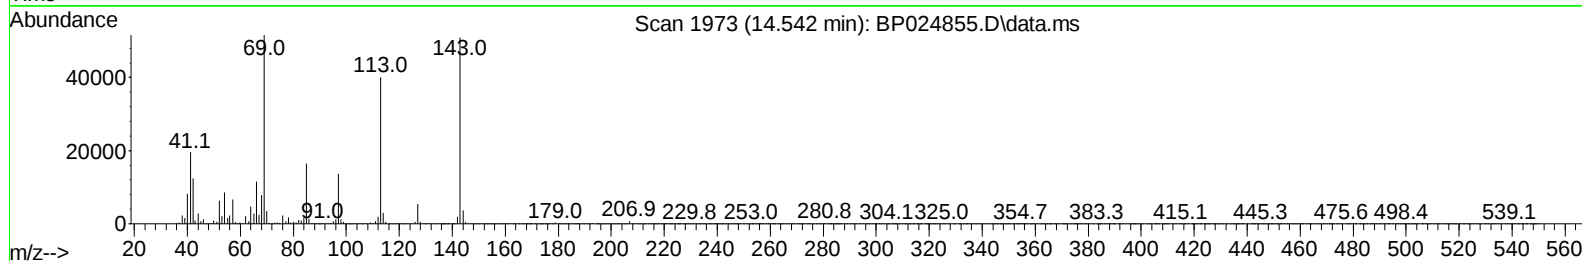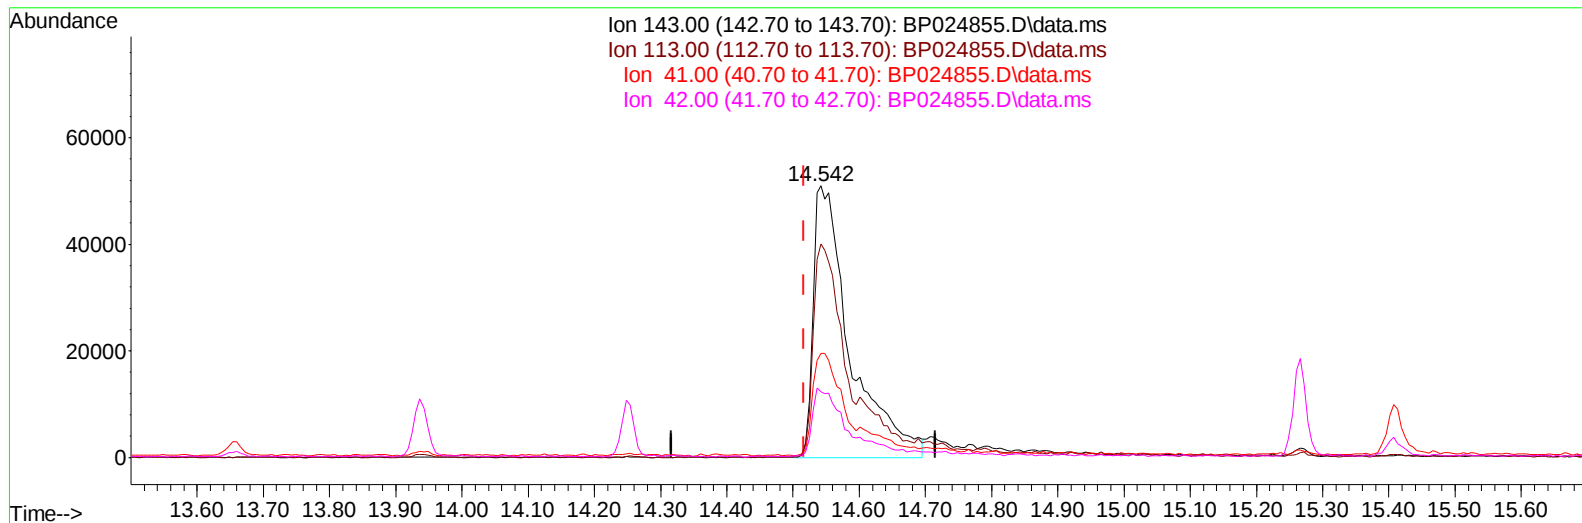

TIC: BP024855.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.542min (+ 0.026) 31.77 ng/ul m

response 196402

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	73.10	78.65
41.00	36.00	38.36
42.00	22.80	24.23

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060525\
 Data File : BP024855.D
 Acq On : 05 Jun 2025 15:20
 Operator : RC/JU
 Sample : PB166618TB
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB618

Manual IntegrationsAPPROVED

Reviewed By :Rahul Chavli 06/06/2025
 Supervised By :Jagrut Upadhyay 06/06/2025

Quant Time: Jun 05 16:58:20 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060525.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 05 15:37:10 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.613	152	204625	20.000	ng/ul	0.00
20) Naphthalene-d8	10.378	136	832640	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.248	164	549089	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.054	188	1089360	20.000	ng/ul	0.00
79) Chrysene-d12	21.483	240	1220345	20.000	ng/ul	0.00
88) Perylene-d12	24.718	264	1423198	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.137	96	33484	6.266	ng/uL	0.00
4) Pyridine-d5	3.555	84	405870	31.292	ng/ul	0.00
7) Phenol-d5	6.819	99	551734	33.500	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.955	67	309462	31.843	ng/ul	0.00
11) 2-Chlorophenol-d4	7.160	132	469950	34.696	ng/ul	0.00
15) 4-Methylphenol-d8	8.337	113	460231	33.962	ng/ul	0.00
21) Nitrobenzene-d5	8.760	128	212104	32.557	ng/ul	0.00
24) 2-Nitrophenol-d4	9.478	143	240806	33.077	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.037	165	411647	32.883	ng/ul	0.00
31) 4-Chloroaniline-d4	10.531	131	521696	28.517	ng/ul	0.00
46) Dimethylphthalate-d6	13.660	166	1403830	34.602	ng/ul	0.00
49) Acenaphthylene-d8	13.936	160	1480120	32.695	ng/ul	0.00
54) 4-Nitrophenol-d4	14.542	143	196402m	31.770	ng/ul	0.03
60) Fluorene-d10	15.266	176	1107044	33.615	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.407	200	203410	27.603	ng/ul	0.00
73) Anthracene-d10	17.160	188	1769051	33.922	ng/ul	0.00
81) Pyrene-d10	19.542	212	2092480	33.102	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.507	264	2443538	33.691	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060525\
Data File : BP024855.D
Acq On : 05 Jun 2025 15:20
Operator : RC/JU
Sample : PB166618TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB618

Manual IntegrationsAPPROVED

Quant Time: Jun 05 16:58:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060525.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 05 15:37:10 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 06/06/2025
Supervised By :Jagrut Upadhyay 06/06/2025

