




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
 Data File : BP015401.D
 Acq On : 07 Jun 2023 16:27
 Operator : MA/JU
 Sample : 02950-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW981

Manual IntegrationsAPPROVED

Quant Time: Jun 08 00:11:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 07 23:46:15 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/08/2023
 Supervised By :mohammad ahmed 06/08/2023

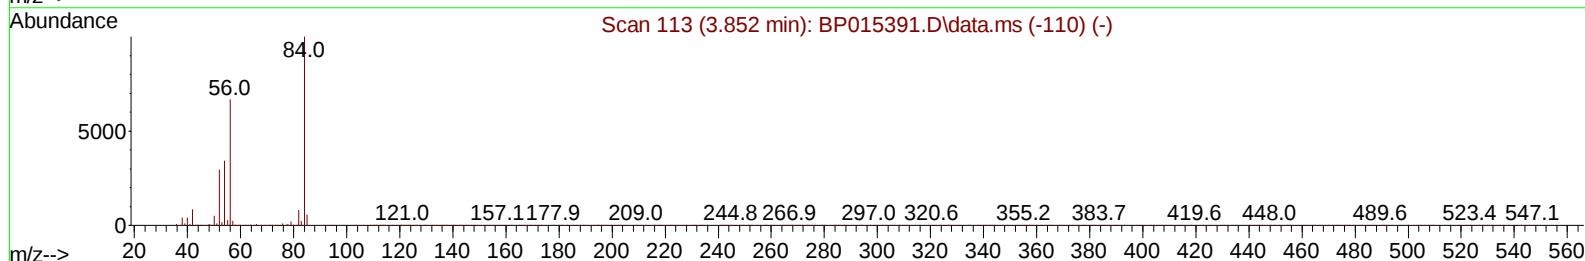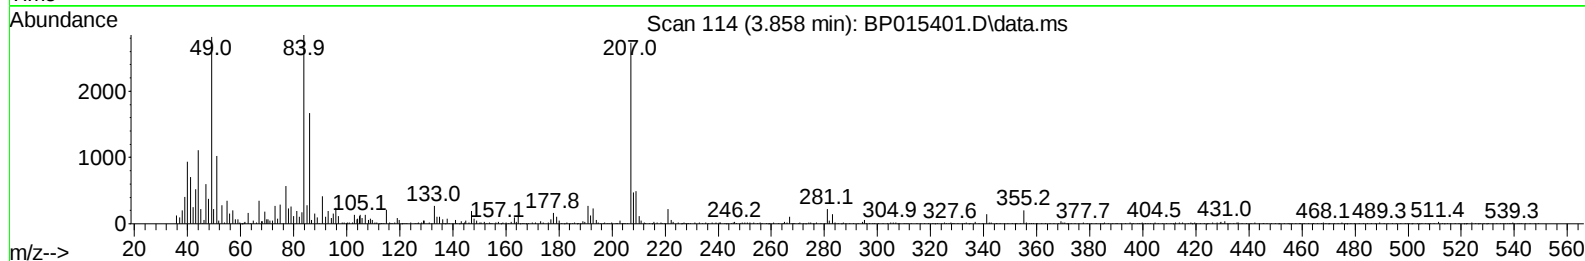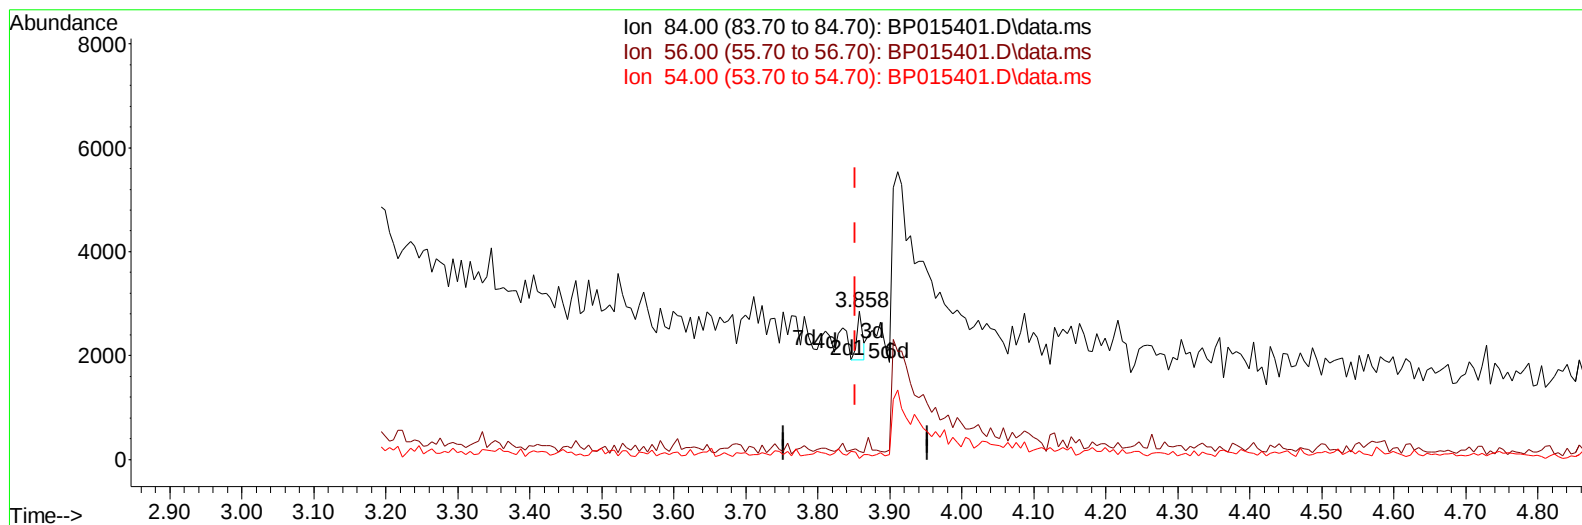

TIC: BP015401.D\data.ms

(4) Pyridine-d5 (S)

3.858min (+ 0.006) 0.04 ng/u1

response 515

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.90	5.51#
54.00	33.70	0.70#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
 Data File : BP015401.D
 Acq On : 07 Jun 2023 16:27
 Operator : MA/JU
 Sample : 02950-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW981

Manual IntegrationsAPPROVED

Quant Time: Jun 08 00:11:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 07 23:46:15 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/08/2023
 Supervised By :mohammad ahmed 06/08/2023

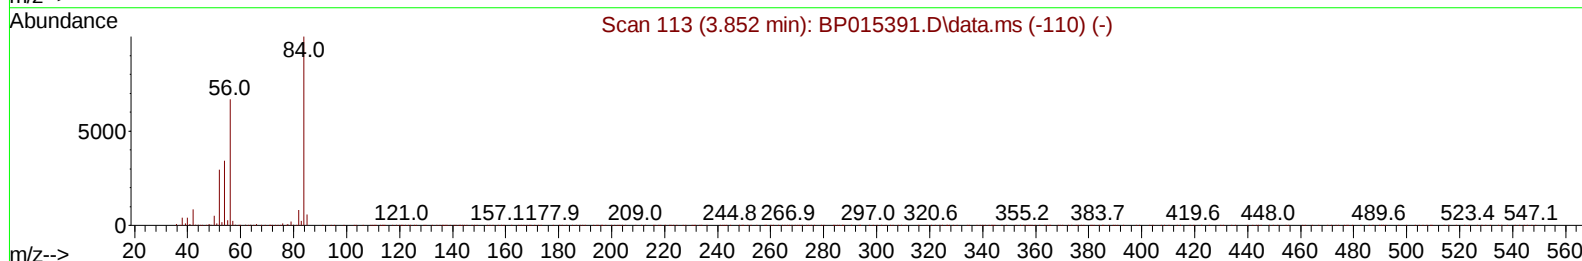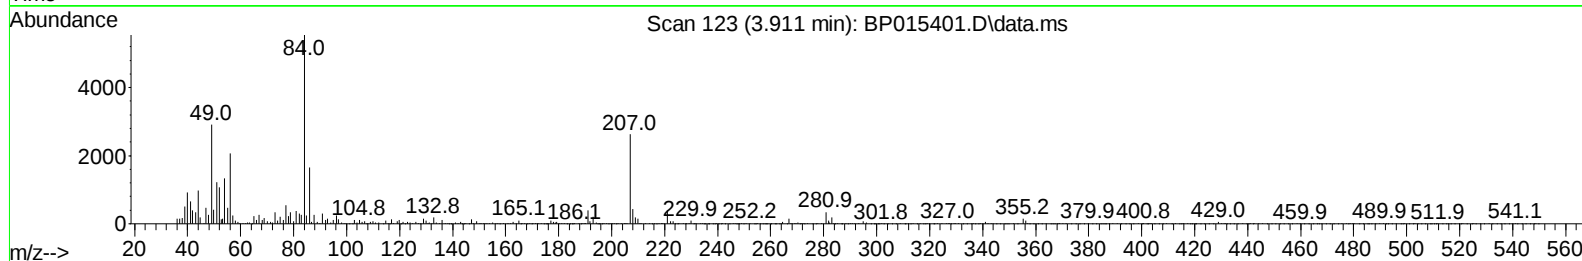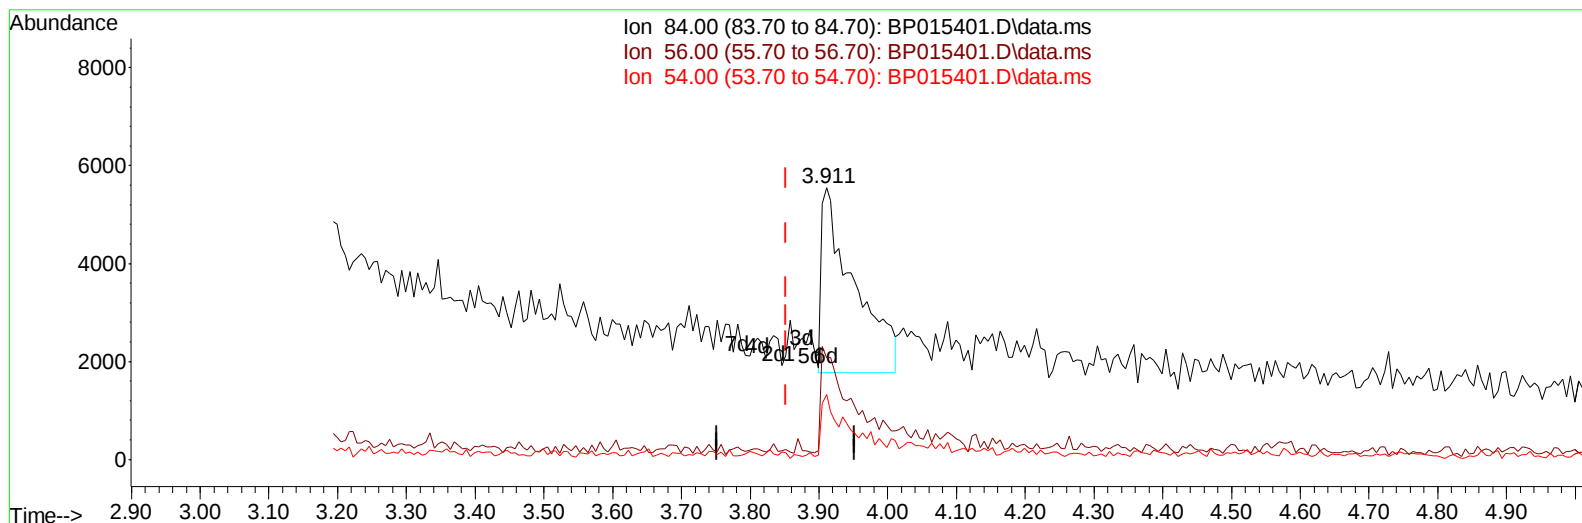

TIC: BP015401.D\data.ms

(4) Pyridine-d5 (S)

3.911min (+ 0.059) 1.04 ng/ul m

response 12427

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.90	37.41#
54.00	33.70	24.03#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
 Data File : BP015401.D
 Acq On : 07 Jun 2023 16:27
 Operator : MA/JU
 Sample : 02950-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW981

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/08/2023
 Supervised By :mohammad ahmed 06/08/2023

Quant Time: Jun 08 00:30:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 07 23:46:15 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.099	152		170922	20.000	ng/ul	0.00
20) Naphthalene-d8	10.928	136		768039	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.746	164		548224	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.498	188		1300758	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240		1270072	20.000	ng/ul	0.00
88) Perylene-d12	24.133	264		1375986	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.411	96		17721	3.839	ng/uL	0.00
4) Pyridine-d5	3.911	84		12427m	1.036	ng/ul	0.06
7) Phenol-d5	7.252	99		304966	19.367	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.422	67		206607	21.970	ng/ul	0.00
11) 2-Chlorophenol-d4	7.622	132		250168	21.913	ng/ul	0.00
15) 4-Methylphenol-d8	8.816	113		253372	19.606	ng/ul	0.00
21) Nitrobenzene-d5	9.275	128		132369	21.952	ng/ul	0.00
24) 2-Nitrophenol-d4	10.005	143		156821	22.774	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.546	165		253965	20.218	ng/ul	0.00
31) 4-Chloroaniline-d4	11.069	131		315592	17.503	ng/ul	0.00
46) Dimethylphthalate-d6	14.146	166		1091196	25.241	ng/ul	0.00
49) Acenaphthylene-d8	14.440	160		1098536	23.239	ng/ul	0.00
54) 4-Nitrophenol-d4	14.946	143		147949	19.111	ng/ul	0.00
60) Fluorene-d10	15.734	176		881653	24.185	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200		163770	19.874	ng/ul	0.00
73) Anthracene-d10	17.598	188		1562919	26.408	ng/ul	0.00
81) Pyrene-d10	19.822	212		2062289	30.338	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.969	264		2016997	29.214	ng/ul	0.00
Target Compounds							
16) Acetophenone	8.934	105		92285	4.475	ng/ul	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
Data File : BP015401.D
Acq On : 07 Jun 2023 16:27
Operator : MA/JU
Sample : 02950-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW981

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/08/2023
Supervised By :mohammad ahmed 06/08/2023

Quant Time: Jun 08 00:30:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 07 23:46:15 2023
Response via : Initial Calibration

