




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
 Data File : BP015417.D
 Acq On : 08 Jun 2023 02:30
 Operator : MA/JU
 Sample : 02950-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW994

Manual IntegrationsAPPROVED

Quant Time: Jun 09 05:14:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 07 23:46:15 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/09/2023
 Supervised By :mohammad ahmed 06/12/2023

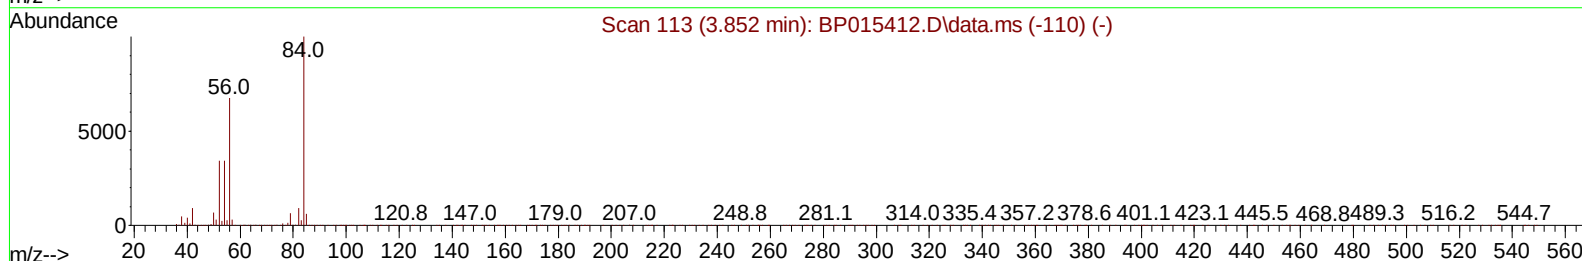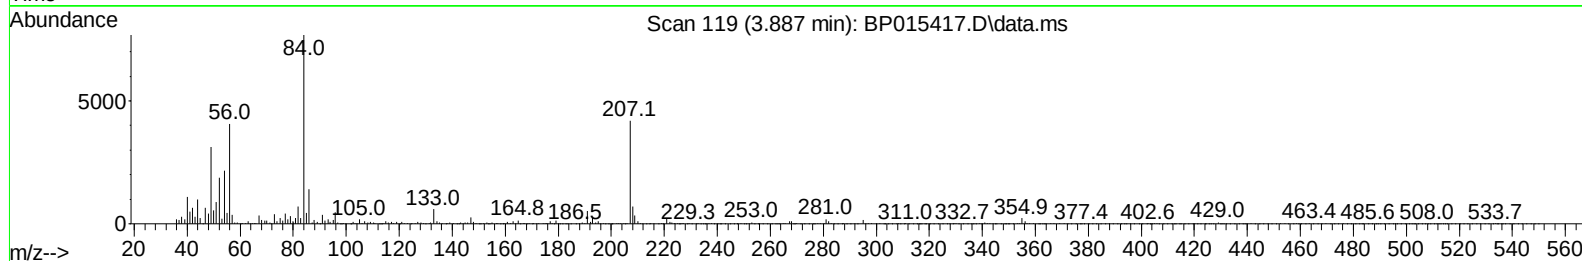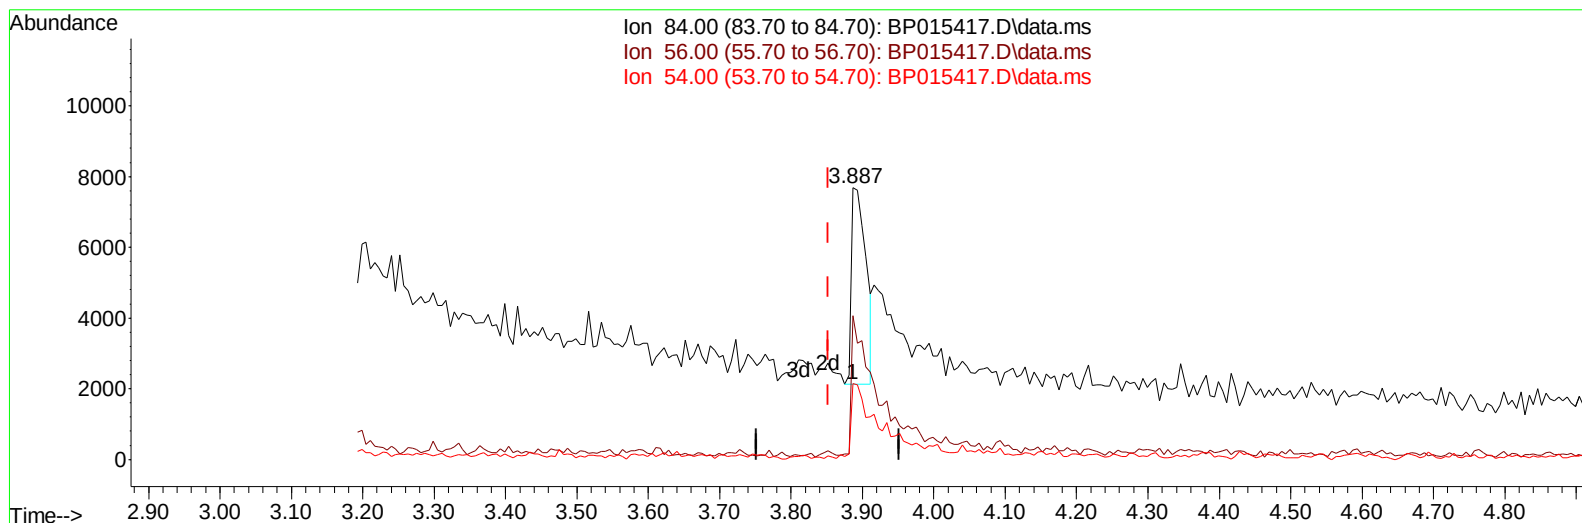

TIC: BP015417.D\data.ms

(4) Pyridine-d5 (S)

3.887min (+ 0.035) 0.73 ng/u1

response 7752

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.90	52.92
54.00	33.70	28.02
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
 Data File : BP015417.D
 Acq On : 08 Jun 2023 02:30
 Operator : MA/JU
 Sample : 02950-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW994

Manual IntegrationsAPPROVED

Quant Time: Jun 08 03:06:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 07 23:46:15 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/09/2023
 Supervised By :mohammad ahmed 06/12/2023

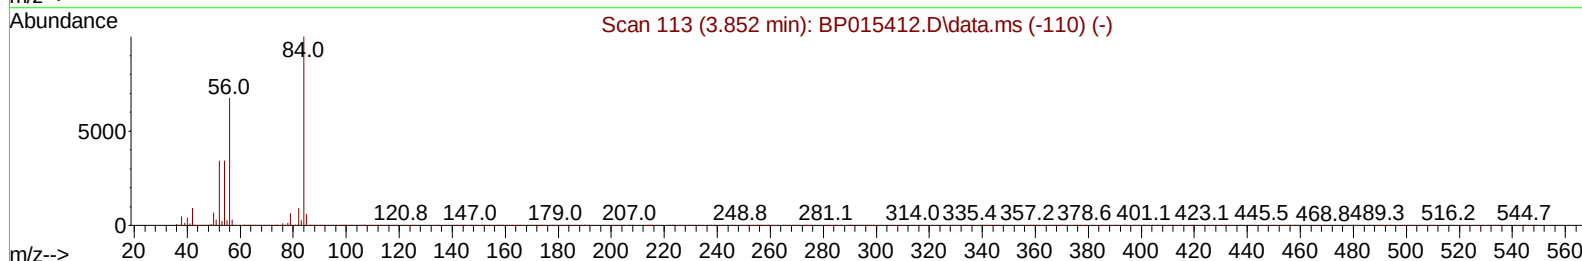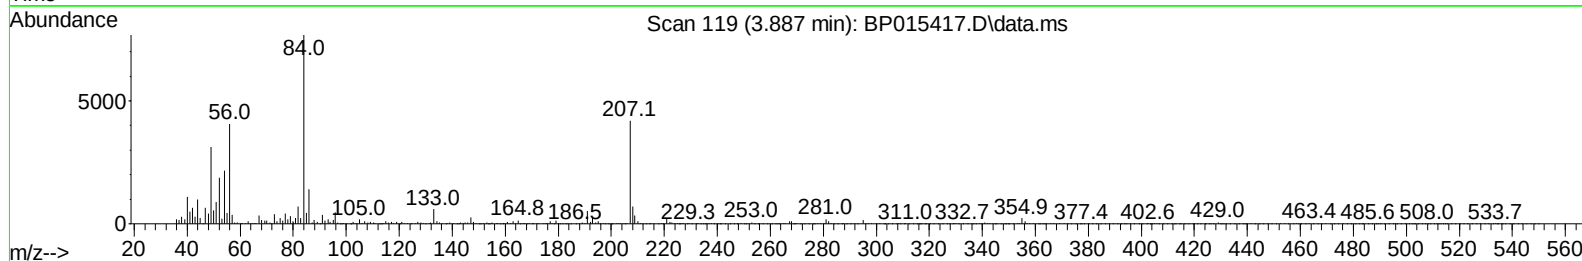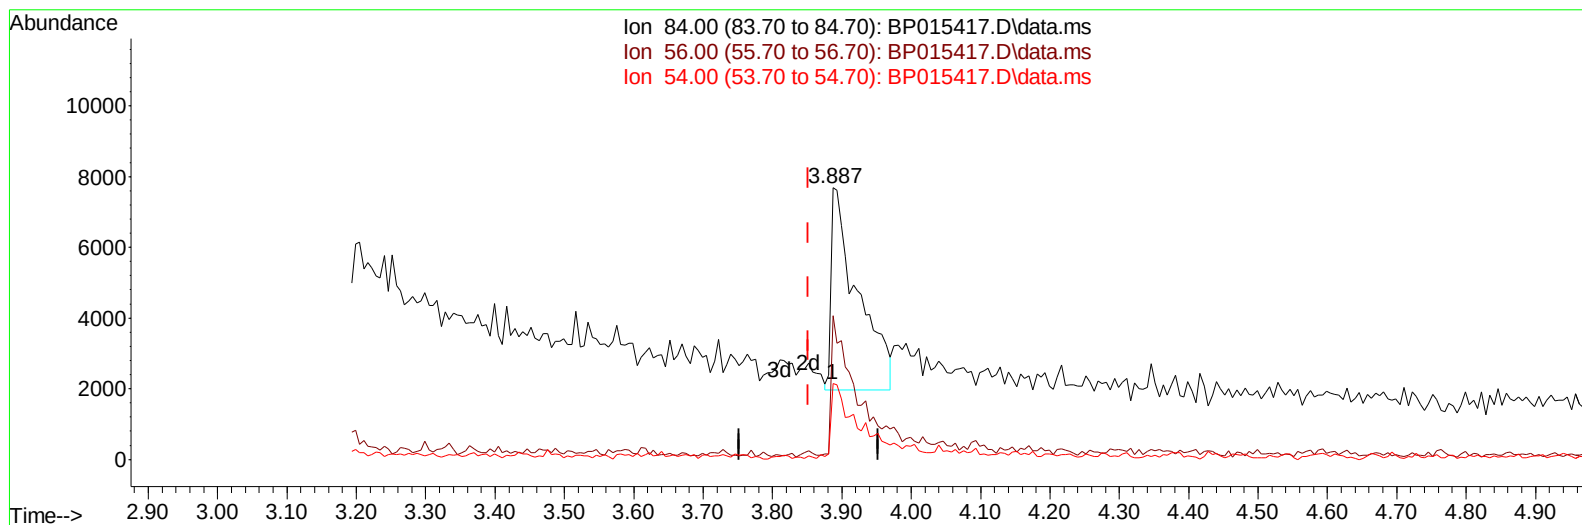

TIC: BP015417.D\data.ms

(4) Pyridine-d5 (S)

3.887min (+ 0.035) 1.41 ng/ul m

response 15079

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.90	52.92
54.00	33.70	28.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
 Data File : BP015417.D
 Acq On : 08 Jun 2023 02:30
 Operator : MA/JU
 Sample : 02950-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW994

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/09/2023
 Supervised By :mohammad ahmed 06/12/2023

Quant Time: Jun 08 03:06:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 07 23:46:15 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.099	152		152282	20.000	ng/ul	0.00
20) Naphthalene-d8	10.928	136		679420	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.739	164		483137	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.498	188		1155042	20.000	ng/ul	0.00
79) Chrysene-d12	21.574	240		1225141	20.000	ng/ul	-0.01
88) Perylene-d12	24.133	264		1397350	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.417	96		9662	2.349	ng/uL	0.00
4) Pyridine-d5	3.887	84		15079m	1.412	ng/ul	0.04
7) Phenol-d5	7.252	99		182120	12.981	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.416	67		120996	14.441	ng/ul	0.00
11) 2-Chlorophenol-d4	7.622	132		145960	14.350	ng/ul	0.00
15) 4-Methylphenol-d8	8.810	113		147734	12.831	ng/ul	0.00
21) Nitrobenzene-d5	9.275	128		76270	14.299	ng/ul	0.00
24) 2-Nitrophenol-d4	10.004	143		89045	14.618	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.546	165		151922	13.672	ng/ul	0.00
31) 4-Chloroaniline-d4	11.069	131		175019	10.973	ng/ul	0.00
46) Dimethylphthalate-d6	14.145	166		620783	16.294	ng/ul	0.00
49) Acenaphthylene-d8	14.434	160		658442	15.806	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143		76005	11.140	ng/ul	0.00
60) Fluorene-d10	15.733	176		537315	16.725	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200		81406	11.125	ng/ul	0.00
73) Anthracene-d10	17.598	188		946196	18.005	ng/ul	0.00
81) Pyrene-d10	19.816	212		1283760	19.578	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.962	264		1341393	19.132	ng/ul	-0.01
Target Compounds							
						Qvalue	
16) Acetophenone	8.934	105		56108	3.053	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
Data File : BP015417.D
Acq On : 08 Jun 2023 02:30
Operator : MA/JU
Sample : 02950-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW994

Manual IntegrationsAPPROVED

Quant Time: Jun 08 03:06:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 07 23:46:15 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/09/2023
Supervised By :mohammad ahmed 06/12/2023

