

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
 Data File : BP015399.D
 Acq On : 07 Jun 2023 15:19
 Operator : MA/JU
 Sample : 02950-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW979

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/08/2023
 Supervised By :mohammad ahmed 06/08/2023

Quant Time: Jun 08 00:24:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 07 23:46:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	176251	20.000	ng/u1	0.00
20) Naphthalene-d8	10.928	136	779255	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.745	164	546439	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.498	188	1275133	20.000	ng/u1	0.00
79) Chrysene-d12	21.580	240	1273766	20.000	ng/u1	0.00
88) Perylene-d12	24.139	264	1416908	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.416	96	15040	3.160	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	0.00
7) Phenol-d5	7.252	99	243639	15.005	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.422	67	165508	17.067	ng/u1	0.00
11) 2-Chlorophenol-d4	7.628	132	200122	16.999	ng/u1	0.00
15) 4-Methylphenol-d8	8.810	113	158718	11.910	ng/u1	0.00
21) Nitrobenzene-d5	9.275	128	105372	17.224	ng/u1	0.00
24) 2-Nitrophenol-d4	10.004	143	121726	17.423	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.551	165	194236	15.240	ng/u1	0.00
31) 4-Chloroaniline-d4	11.069	131	200923	10.983	ng/u1	0.00
46) Dimethylphthalate-d6	14.145	166	840081	19.496	ng/u1	0.00
49) Acenaphthylene-d8	14.439	160	876046	18.593	ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	98890	12.815	ng/u1	0.00
60) Fluorene-d10	15.739	176	717042	19.733	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.863	200	118110	14.621	ng/u1	0.00
73) Anthracene-d10	17.598	188	1239844	21.370	ng/u1	0.00
81) Pyrene-d10	19.821	212	1610889	23.629	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.968	264	1574977	22.153	ng/u1	0.00
Target Compounds					Qvalue	
8) Phenol	7.281	94	18280	1.091	ng/u1	96
16) Acetophenone	8.934	105	127080	5.975	ng/u1	99
80) Fluoranthene	19.498	202	124668	1.501	ng/u1	100
82) Pyrene	19.851	202	224034	2.608	ng/u1	99
85) Benzo(a)anthracene	21.563	228	133881m	1.504	ng/u1	
87) Chrysene	21.616	228	173689	2.064	ng/u1	97
90) Benzo(b)fluoranthene	23.351	252	113573	1.242	ng/u1#	95
93) Benzo(a)pyrene	24.021	252	105582	1.324	ng/u1#	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
Data File : BP015399.D
Acq On : 07 Jun 2023 15:19
Operator : MA/JU
Sample : 02950-02
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
EW979

Quant Time: Jun 08 00:24:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 07 23:46:15 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/08/2023
Supervised By :mohammad ahmed 06/08/2023

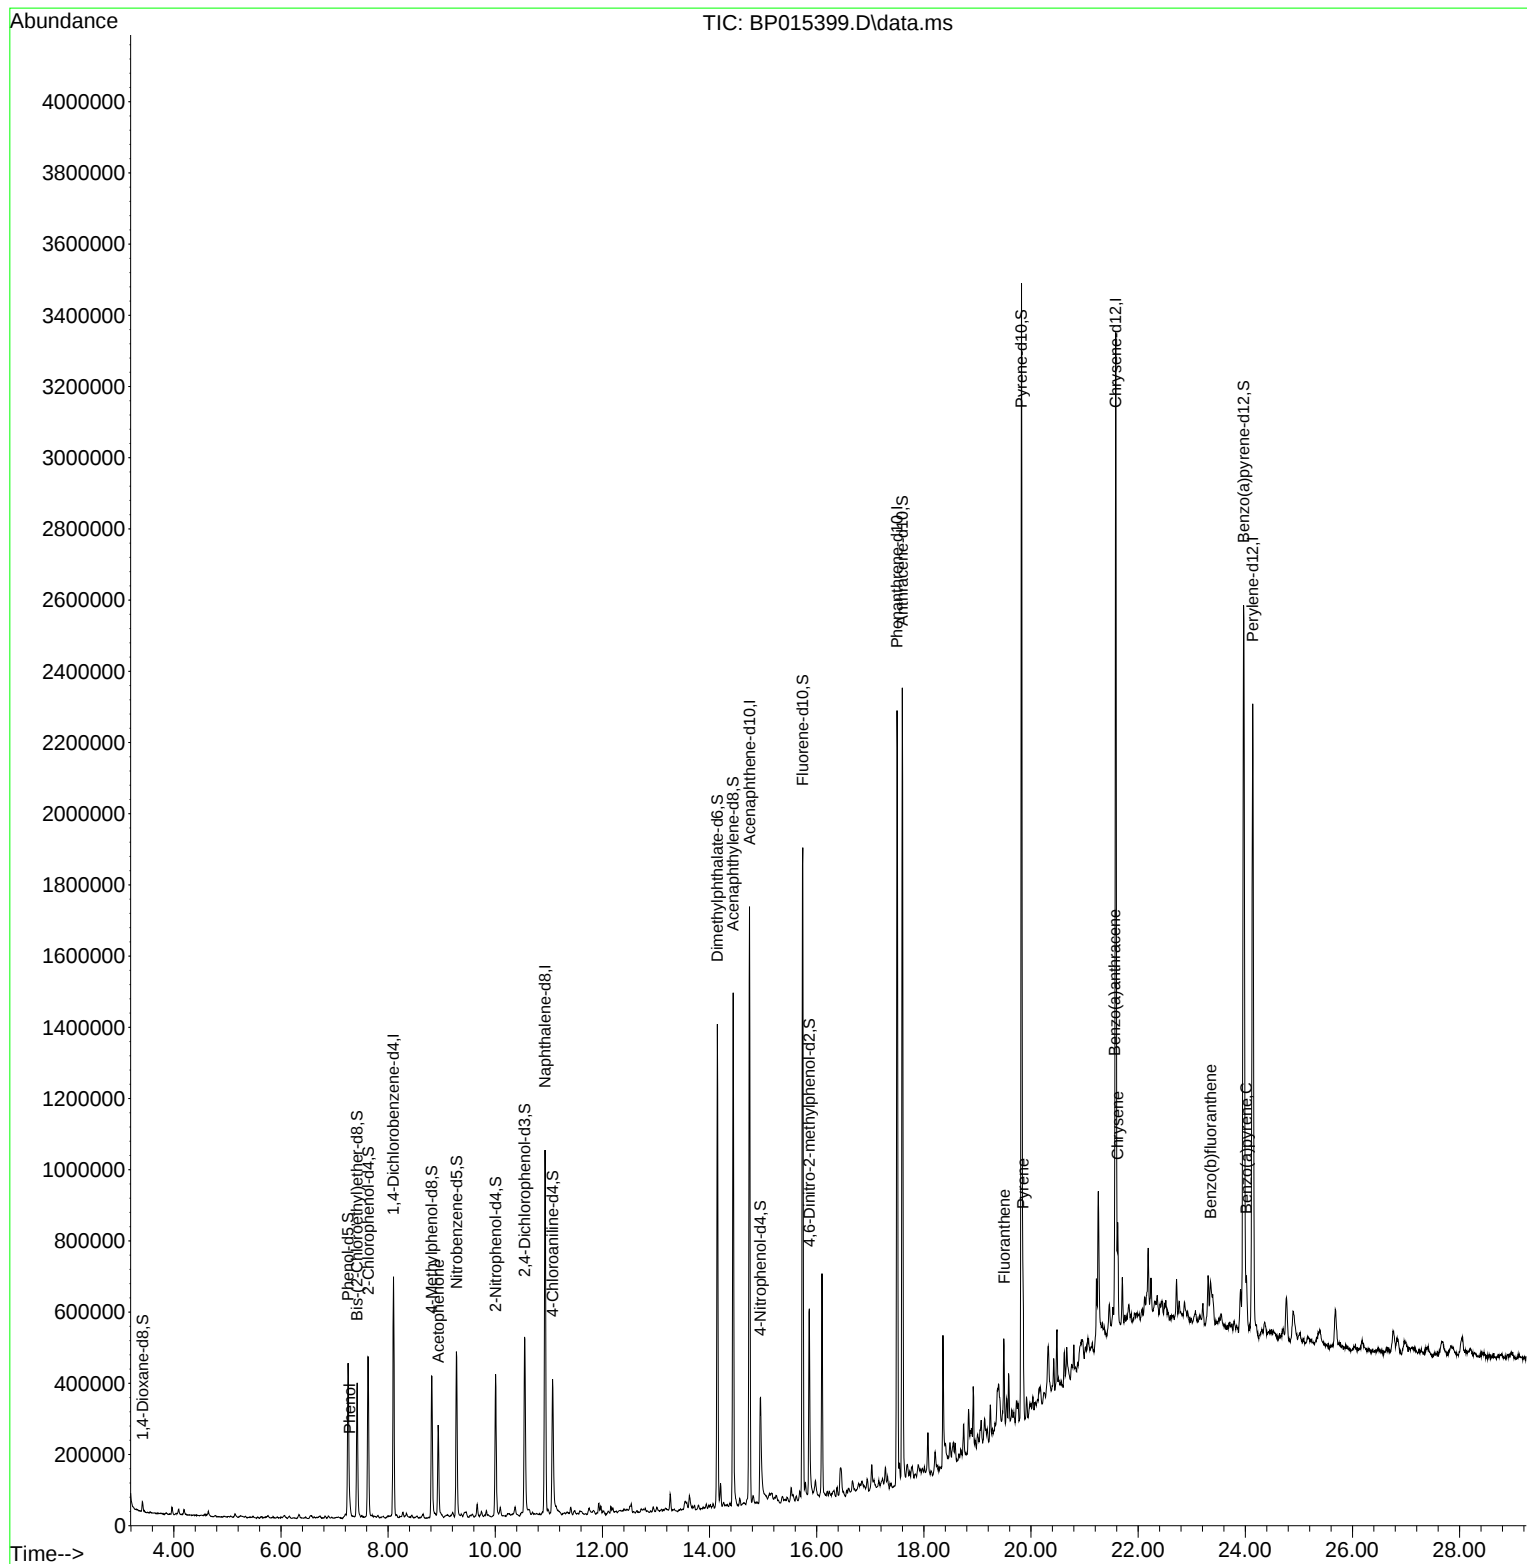

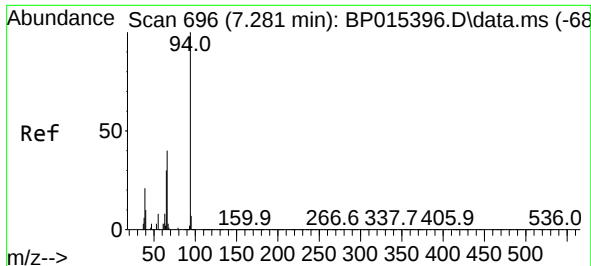

#8
Phenol
Concen: 1.091 ng/ul
RT: 7.281 min Scan# 696
Delta R.T. -0.000 min
Lab File: BP015399.D
Acq: 07 Jun 2023 15:19




Instrument :
BNA_P
ClientSampleId :
EW979

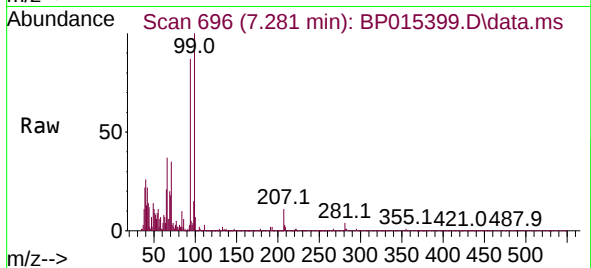


Tgt Ion: 94 Resp: 18280
Ion Ratio Lower Upper
94 100
65 24.7 23.5 35.3
66 42.6 34.2 51.4

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 06/08/2023
Supervised By :mohammad ahmed 06/08/2023

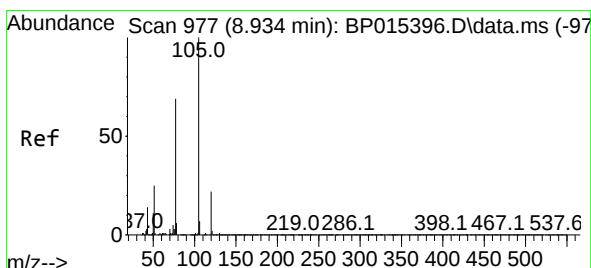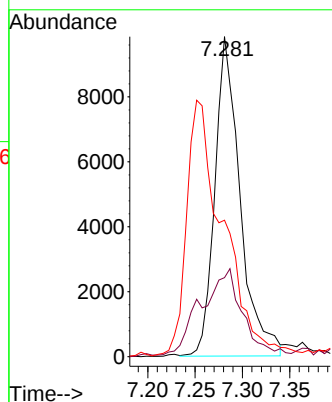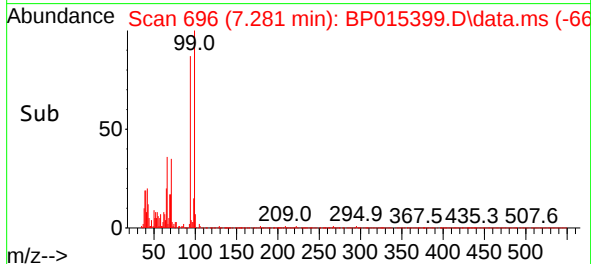


#16
Acetophenone
Concen: 5.975 ng/ul
RT: 8.934 min Scan# 977
Delta R.T. -0.000 min
Lab File: BP015399.D
Acq: 07 Jun 2023 15:19

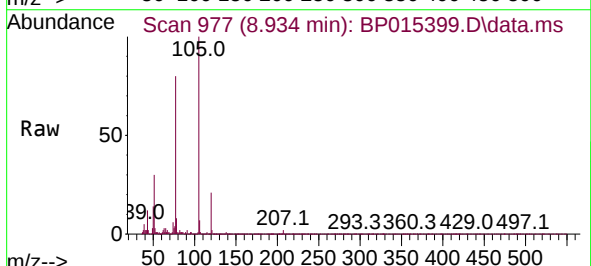


Tgt Ion:105 Resp: 127080
Ion Ratio Lower Upper
105 100
77 79.9 64.9 97.3
51 29.8 23.5 35.3

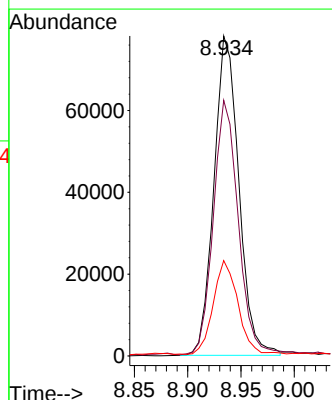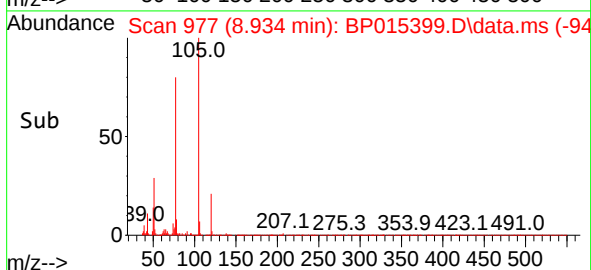

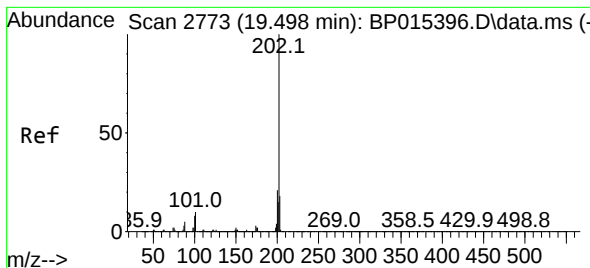

#80
Fluoranthene
Concen: 1.501 ng/u1
RT: 19.498 min Scan# 2773
Delta R.T. -0.000 min
Lab File: BP015399.D
Acq: 07 Jun 2023 15:19




Instrument :
BNA_P
ClientSampleId :
EW979

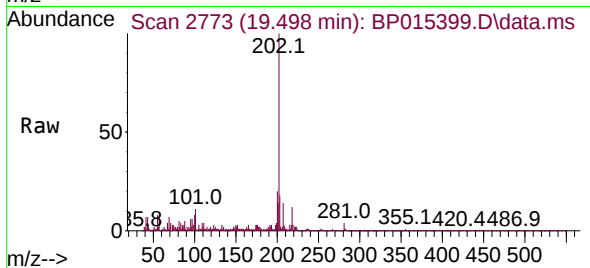

Tgt Ion:202 Resp: 124668
Ion Ratio Lower Upper
202 100
101 10.7 8.6 13.0
100 8.0 6.6 9.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/08/2023
Supervised By :mohammad ahmed 06/08/2023

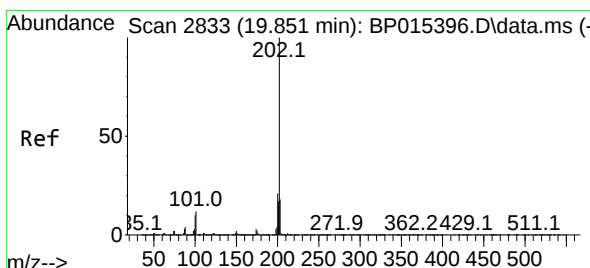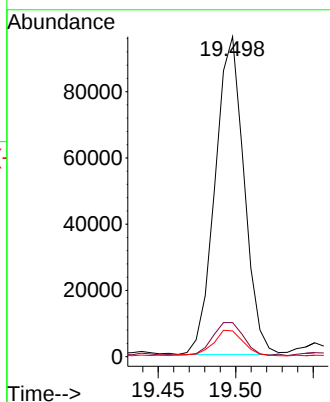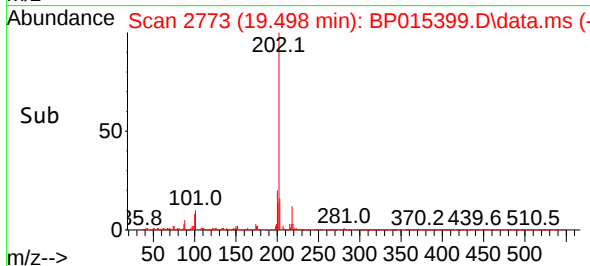

#82
Pyrene
Concen: 2.608 ng/u1
RT: 19.851 min Scan# 2833
Delta R.T. -0.000 min
Lab File: BP015399.D
Acq: 07 Jun 2023 15:19


Tgt Ion:202 Resp: 224034
Ion Ratio Lower Upper
202 100
101 12.6 9.9 14.9
100 9.9 8.4 12.6

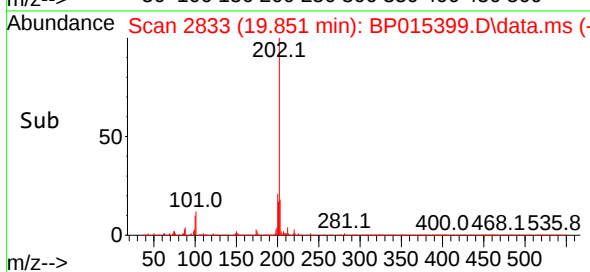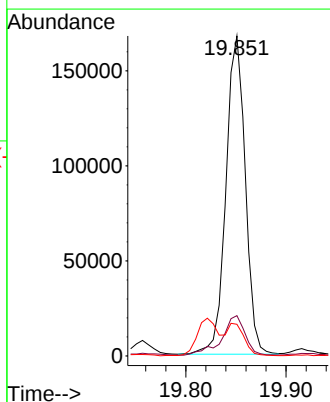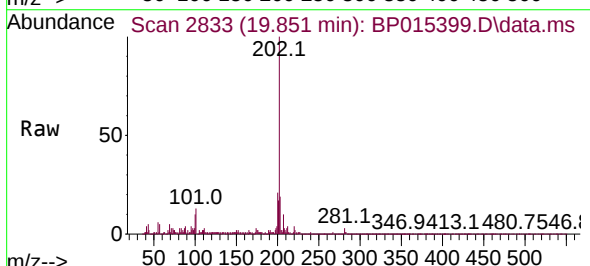

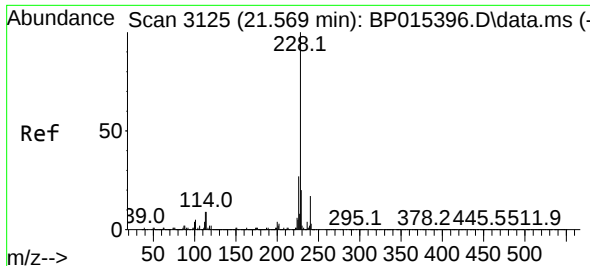

#85
Benzo(a)anthracene
Concen: 1.504 ng/ul m
RT: 21.563 min Scan# 3125
Delta R.T. -0.006 min
Lab File: BP015399.D
Acq: 07 Jun 2023 15:19




Instrument : BNA_P
ClientSampleId : EW979

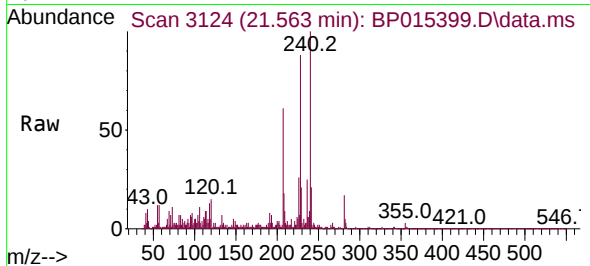

Tgt Ion:228 Resp: 13388
Ion Ratio Lower Upper
228 100
229 24.2 15.8 23.6
226 29.2 21.8 32.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/08/2023
Supervised By :mohammad ahmed 06/08/2023

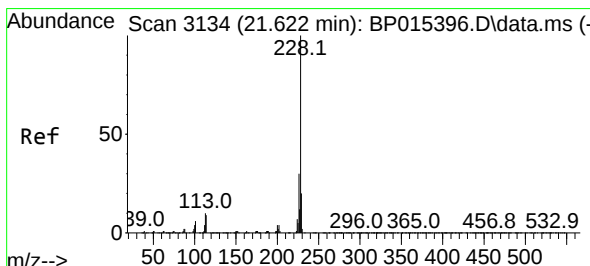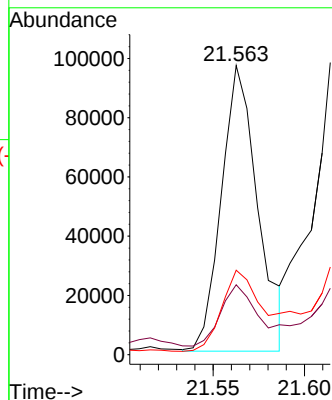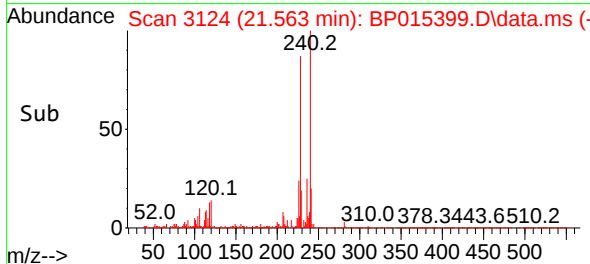

#87
Chrysene
Concen: 2.064 ng/ul
RT: 21.616 min Scan# 3133
Delta R.T. -0.006 min
Lab File: BP015399.D
Acq: 07 Jun 2023 15:19


Tgt Ion:228 Resp: 173689
Ion Ratio Lower Upper
228 100
226 29.9 23.9 35.9
229 22.3 15.1 22.7

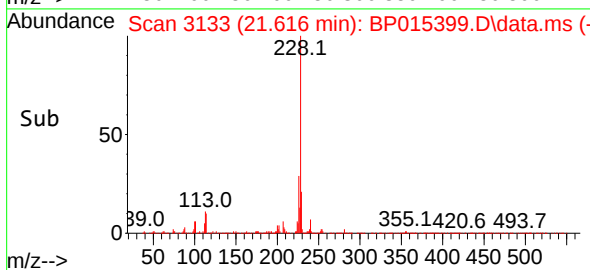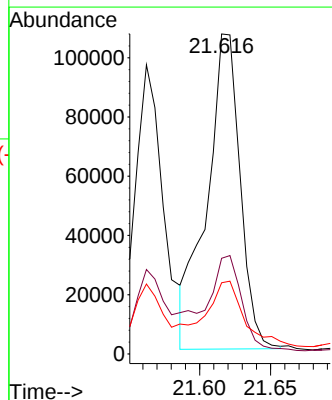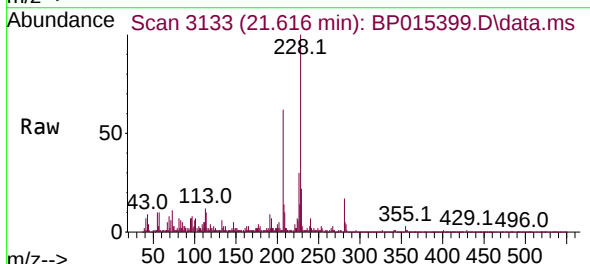

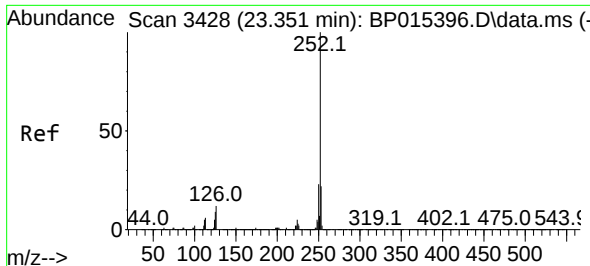

#90
Benzo(b)fluoranthene
Concen: 1.242 ng/ul
RT: 23.351 min Scan# 3428
Delta R.T. -0.000 min
Lab File: BP015399.D
Acq: 07 Jun 2023 15:19




Instrument :
BNA_P
ClientSampleId :
EW979

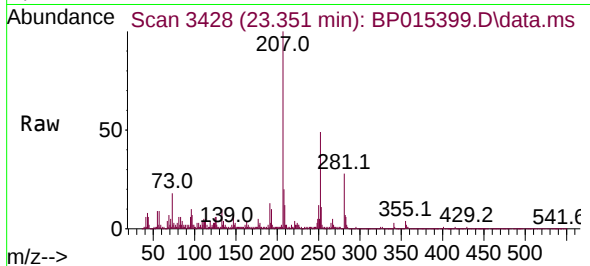

Tgt Ion:252 Resp: 11357
Ion Ratio Lower Upper
252 100
253 23.2 17.4 26.2
125 13.0 7.3 10.9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2023
Supervised By :mohammad ahmed 06/08/2023

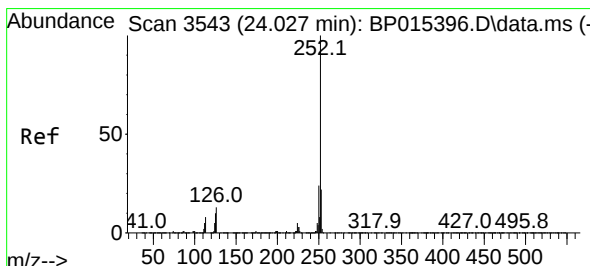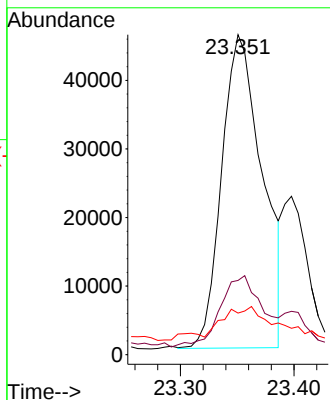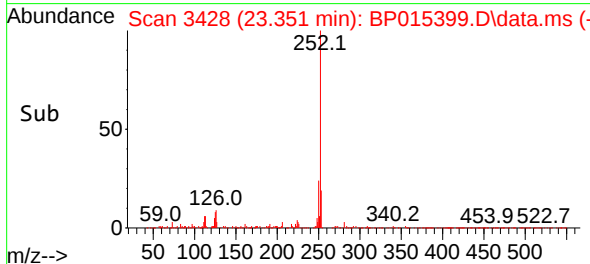

#93
Benzo(a)pyrene
Concen: 1.324 ng/ul
RT: 24.021 min Scan# 3542
Delta R.T. -0.006 min
Lab File: BP015399.D
Acq: 07 Jun 2023 15:19

Tgt Ion:252 Resp: 105582
Ion Ratio Lower Upper
252 100
253 23.5 17.8 26.6
125 13.0 8.1 12.1

