

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
 Data File : BP015401.D
 Acq On : 07 Jun 2023 16:27
 Operator : MA/JU
 Sample : 02950-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW981

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/08/2023
 Supervised By :mohammad ahmed 06/08/2023

Quant Time: Jun 08 00:30:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 07 23:46:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	170922	20.000	ng/u1	0.00
20) Naphthalene-d8	10.928	136	768039	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.746	164	548224	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.498	188	1300758	20.000	ng/u1	0.00
79) Chrysene-d12	21.580	240	1270072	20.000	ng/u1	0.00
88) Perylene-d12	24.133	264	1375986	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.411	96	17721	3.839	ng/uL	0.00
4) Pyridine-d5	3.911	84	12427m	1.036	ng/u1	0.06
7) Phenol-d5	7.252	99	304966	19.367	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.422	67	206607	21.970	ng/u1	0.00
11) 2-Chlorophenol-d4	7.622	132	250168	21.913	ng/u1	0.00
15) 4-Methylphenol-d8	8.816	113	253372	19.606	ng/u1	0.00
21) Nitrobenzene-d5	9.275	128	132369	21.952	ng/u1	0.00
24) 2-Nitrophenol-d4	10.005	143	156821	22.774	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.546	165	253965	20.218	ng/u1	0.00
31) 4-Chloroaniline-d4	11.069	131	315592	17.503	ng/u1	0.00
46) Dimethylphthalate-d6	14.146	166	1091196	25.241	ng/u1	0.00
49) Acenaphthylene-d8	14.440	160	1098536	23.239	ng/u1	0.00
54) 4-Nitrophenol-d4	14.946	143	147949	19.111	ng/u1	0.00
60) Fluorene-d10	15.734	176	881653	24.185	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	163770	19.874	ng/u1	0.00
73) Anthracene-d10	17.598	188	1562919	26.408	ng/u1	0.00
81) Pyrene-d10	19.822	212	2062289	30.338	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.969	264	2016997	29.214	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.934	105	92285	4.475	ng/u1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
Data File : BP015401.D
Acq On : 07 Jun 2023 16:27
Operator : MA/JU
Sample : 02950-04
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
EW981

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2023
Supervised By :mohammad ahmed 06/08/2023

Quant Time: Jun 08 00:30:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 07 23:46:15 2023
Response via : Initial Calibration

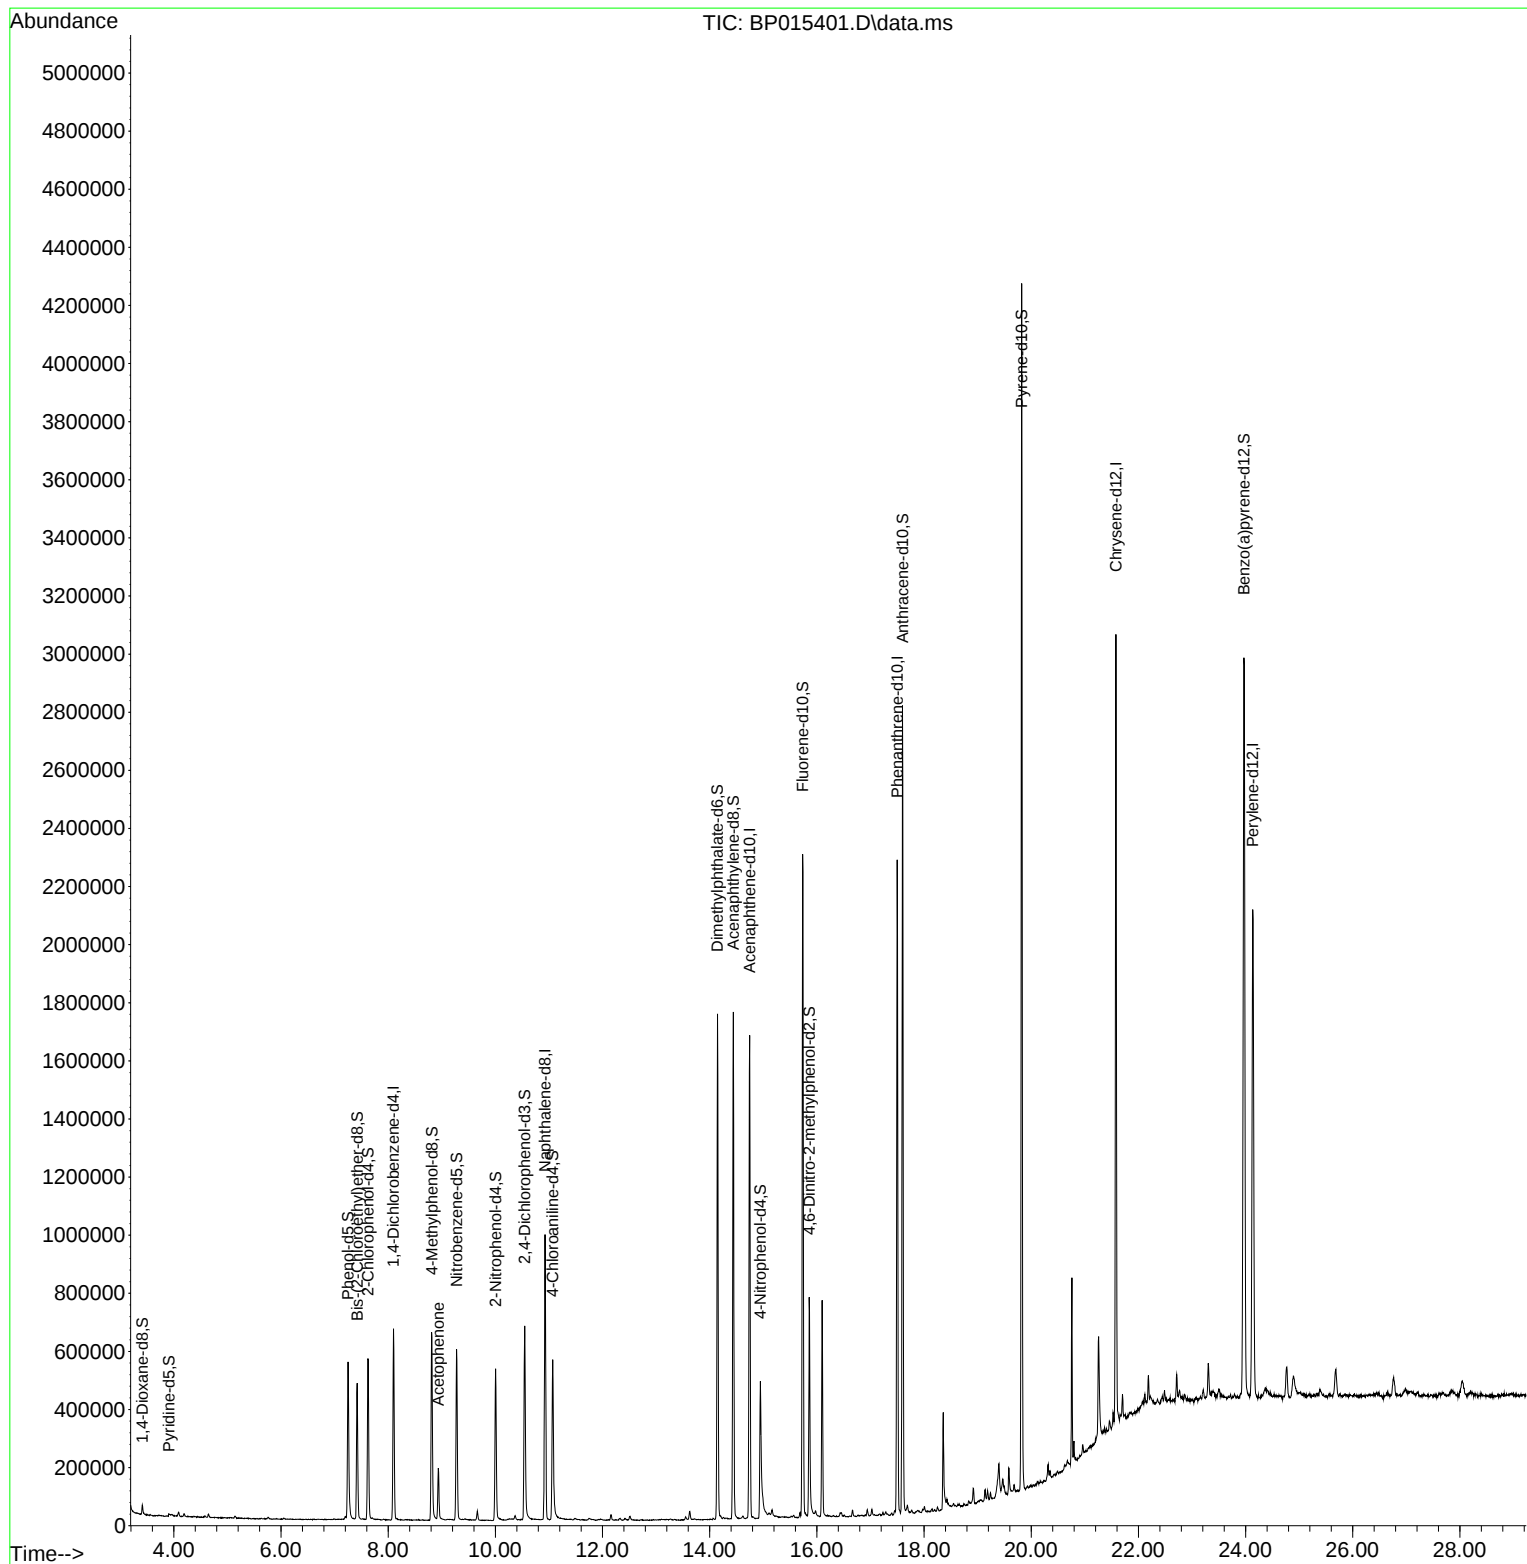

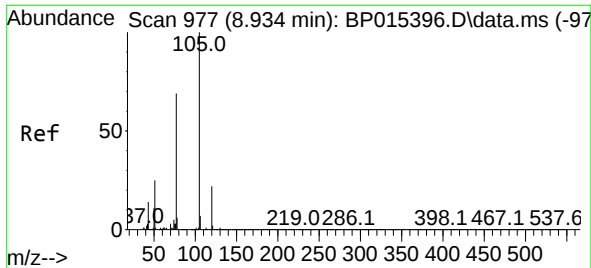

#16
Acetophenone
Concen: 4.475 ng/ul
RT: 8.934 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP015401.D
Acq: 07 Jun 2023 16:27

Instrument :
BNA_P
ClientSampleId :
EW981

Tgt Ion	Ratio	Lower	Upper
105	100		
77	79.5	64.9	97.3
51	29.2	23.5	35.3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2023
Supervised By :mohammad ahmed 06/08/2023

