

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
 Data File : BP015407.D
 Acq On : 07 Jun 2023 19:49
 Operator : MA/JU
 Sample : 02950-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW990

Quant Time: Jun 08 01:06:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 07 23:46:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	180949	20.000	ng/u1	0.00
20) Naphthalene-d8	10.928	136	816051	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.745	164	560510	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.498	188	1290203	20.000	ng/u1	0.00
79) Chrysene-d12	21.580	240	1240929	20.000	ng/u1	0.00
88) Perylene-d12	24.133	264	1322113	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.411	96	15864	3.246	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.252	99	299646	17.975	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.422	67	194259	19.512	ng/u1	0.00
11) 2-Chlorophenol-d4	7.622	132	239448	19.812	ng/u1	0.00
15) 4-Methylphenol-d8	8.810	113	249893	18.265	ng/u1	0.00
21) Nitrobenzene-d5	9.275	128	125068	19.521	ng/u1	0.00
24) 2-Nitrophenol-d4	10.004	143	147766	20.196	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.546	165	256295	19.203	ng/u1	0.00
31) 4-Chloroaniline-d4	11.069	131	307870	16.071	ng/u1	0.00
46) Dimethylphthalate-d6	14.145	166	1027615	23.249	ng/u1	0.00
49) Acenaphthylene-d8	14.440	160	1077711	22.299	ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	126234	15.948	ng/u1	0.00
60) Fluorene-d10	15.734	176	844844	22.667	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	146614	17.938	ng/u1	0.00
73) Anthracene-d10	17.598	188	1392560	23.722	ng/u1	0.00
81) Pyrene-d10	19.822	212	1735961	26.138	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.968	264	1602498	24.157	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.934	105	73598	3.371	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
Data File : BP015407.D
Acq On : 07 Jun 2023 19:49
Operator : MA/JU
Sample : 02950-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW990


Quant Time: Jun 08 01:06:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 07 23:46:15 2023
Response via : Initial Calibration

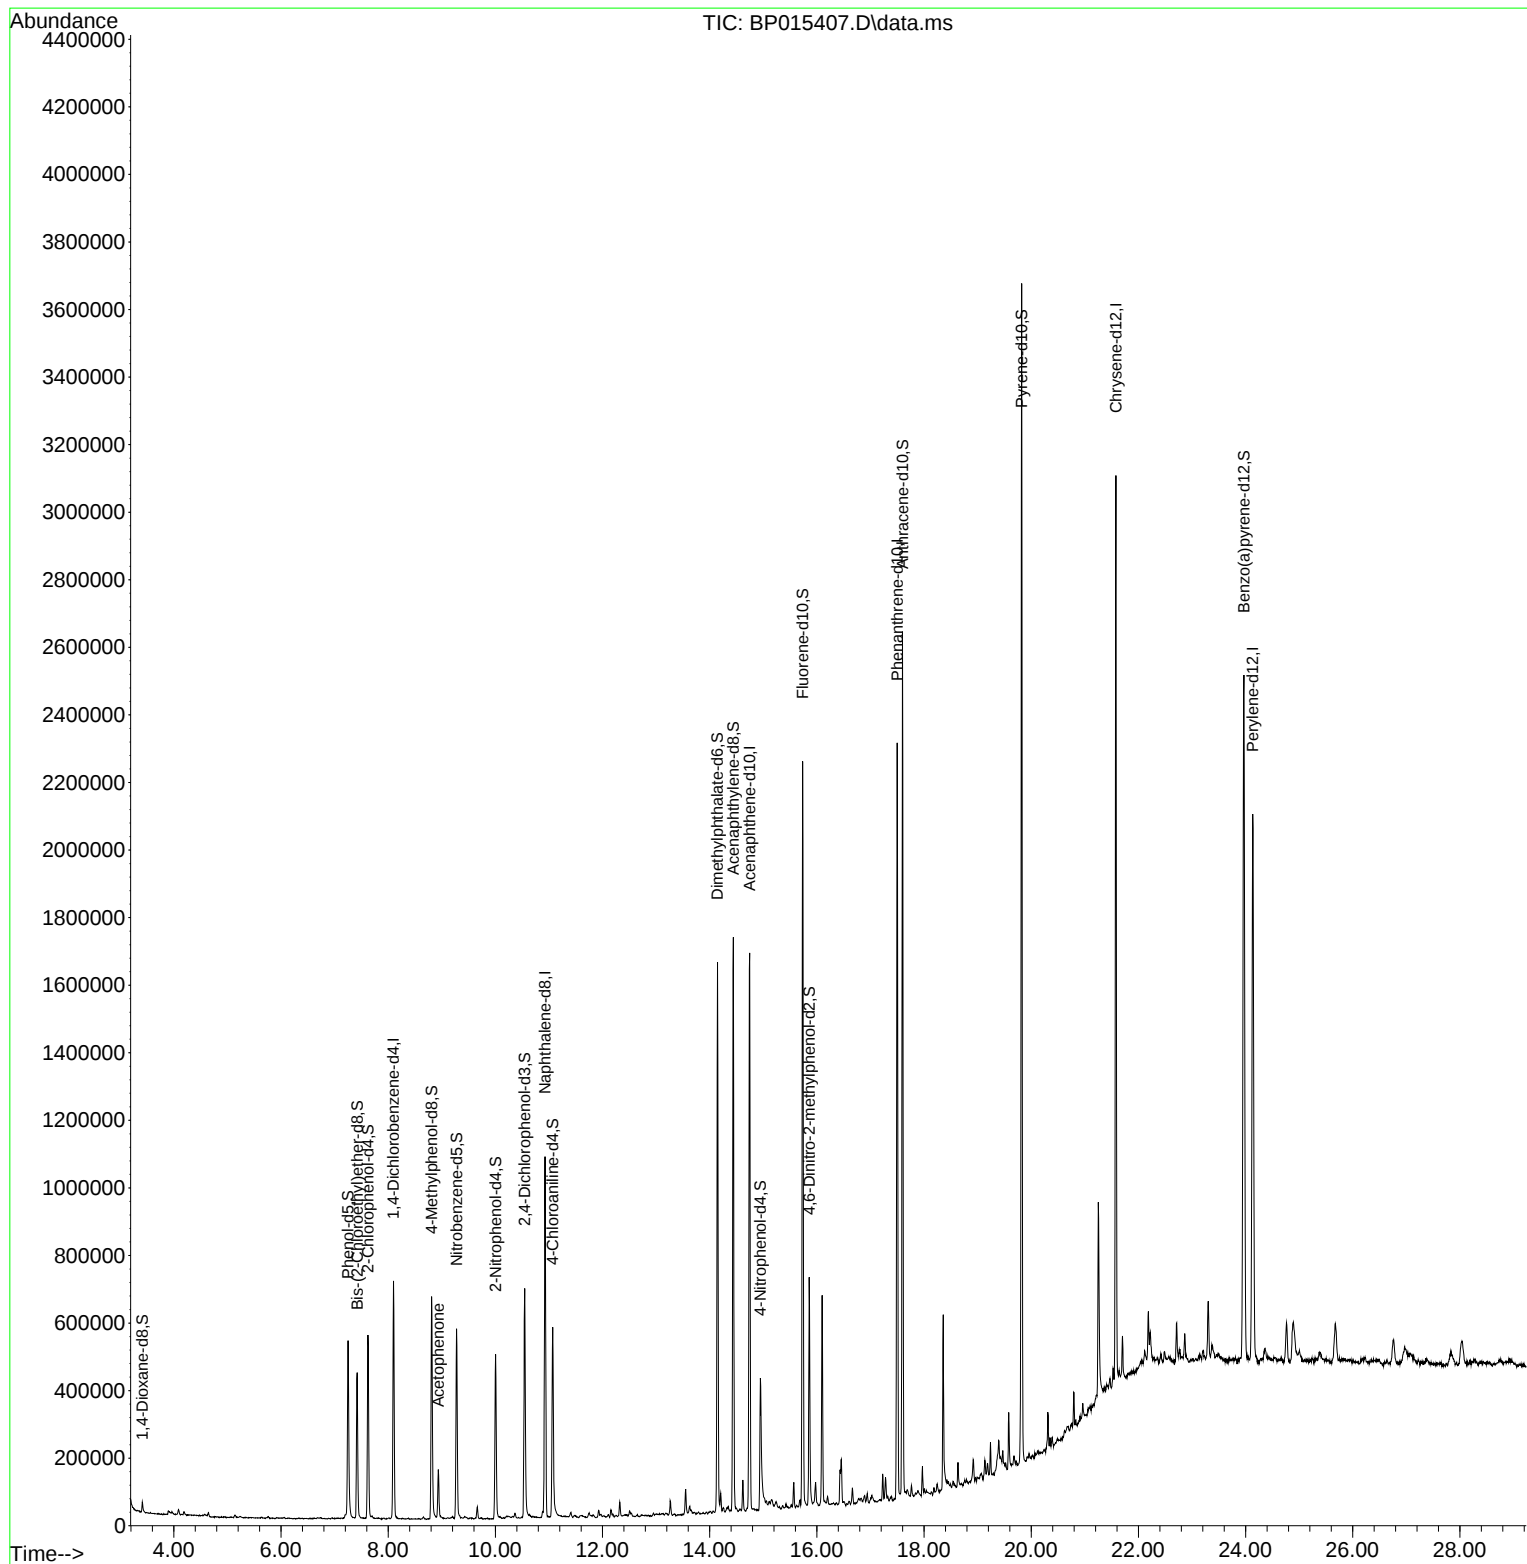

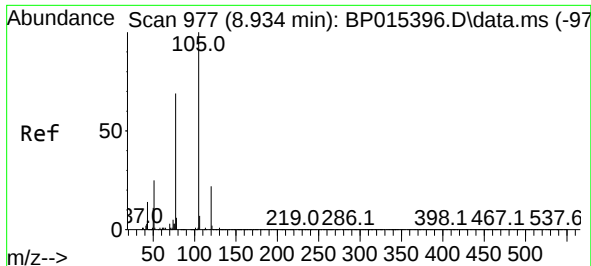

#16
 Acetophenone
 Concen: 3.371 ng/ul
 RT: 8.934 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BP015407.D
 Acq: 07 Jun 2023 19:49

Instrument :
 BNA_P
 ClientSampleId :
 EW990

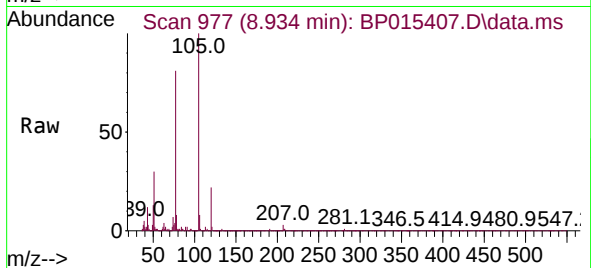

Tgt Ion:	105	Resp:	73598
Ion	Ratio	Lower	Upper
105	100		
77	81.4	64.9	97.3
51	30.0	23.5	35.3

