

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
 Data File : BP015418.D
 Acq On : 08 Jun 2023 03:04
 Operator : MA/JU
 Sample : 02950-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW995

Quant Time: Jun 08 03:33:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 07 23:46:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	102617	20.000	ng/ul	0.00
20) Naphthalene-d8	10.928	136	473201	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.740	164	341498	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.498	188	824605	20.000	ng/ul	0.00
79) Chrysene-d12	21.574	240	868504	20.000	ng/ul	-0.01
88) Perylene-d12	24.127	264	980587	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.411	96	8123	2.931	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.252	99	138705	14.672	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.416	67	91703	16.242	ng/ul	0.00
11) 2-Chlorophenol-d4	7.622	132	111078	16.206	ng/ul	0.00
15) 4-Methylphenol-d8	8.810	113	110533	14.246	ng/ul	0.00
21) Nitrobenzene-d5	9.275	128	57789	15.555	ng/ul	0.00
24) 2-Nitrophenol-d4	10.004	143	67737	15.966	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.551	165	117141	15.136	ng/ul	0.00
31) 4-Chloroaniline-d4	11.069	131	147504	13.278	ng/ul	0.00
46) Dimethylphthalate-d6	14.145	166	528625	19.630	ng/ul	0.00
49) Acenaphthylene-d8	14.434	160	535093	18.172	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	52447	10.876	ng/ul	0.00
60) Fluorene-d10	15.734	176	443577	19.533	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	55480	10.620	ng/ul	0.00
73) Anthracene-d10	17.592	188	771872	20.573	ng/ul	0.00
81) Pyrene-d10	19.816	212	1078909	23.210	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.963	264	1109660	22.553	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.934	105	58121	4.694	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
Data File : BP015418.D
Acq On : 08 Jun 2023 03:04
Operator : MA/JU
Sample : 02950-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW995

Quant Time: Jun 08 03:33:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 07 23:46:15 2023
Response via : Initial Calibration

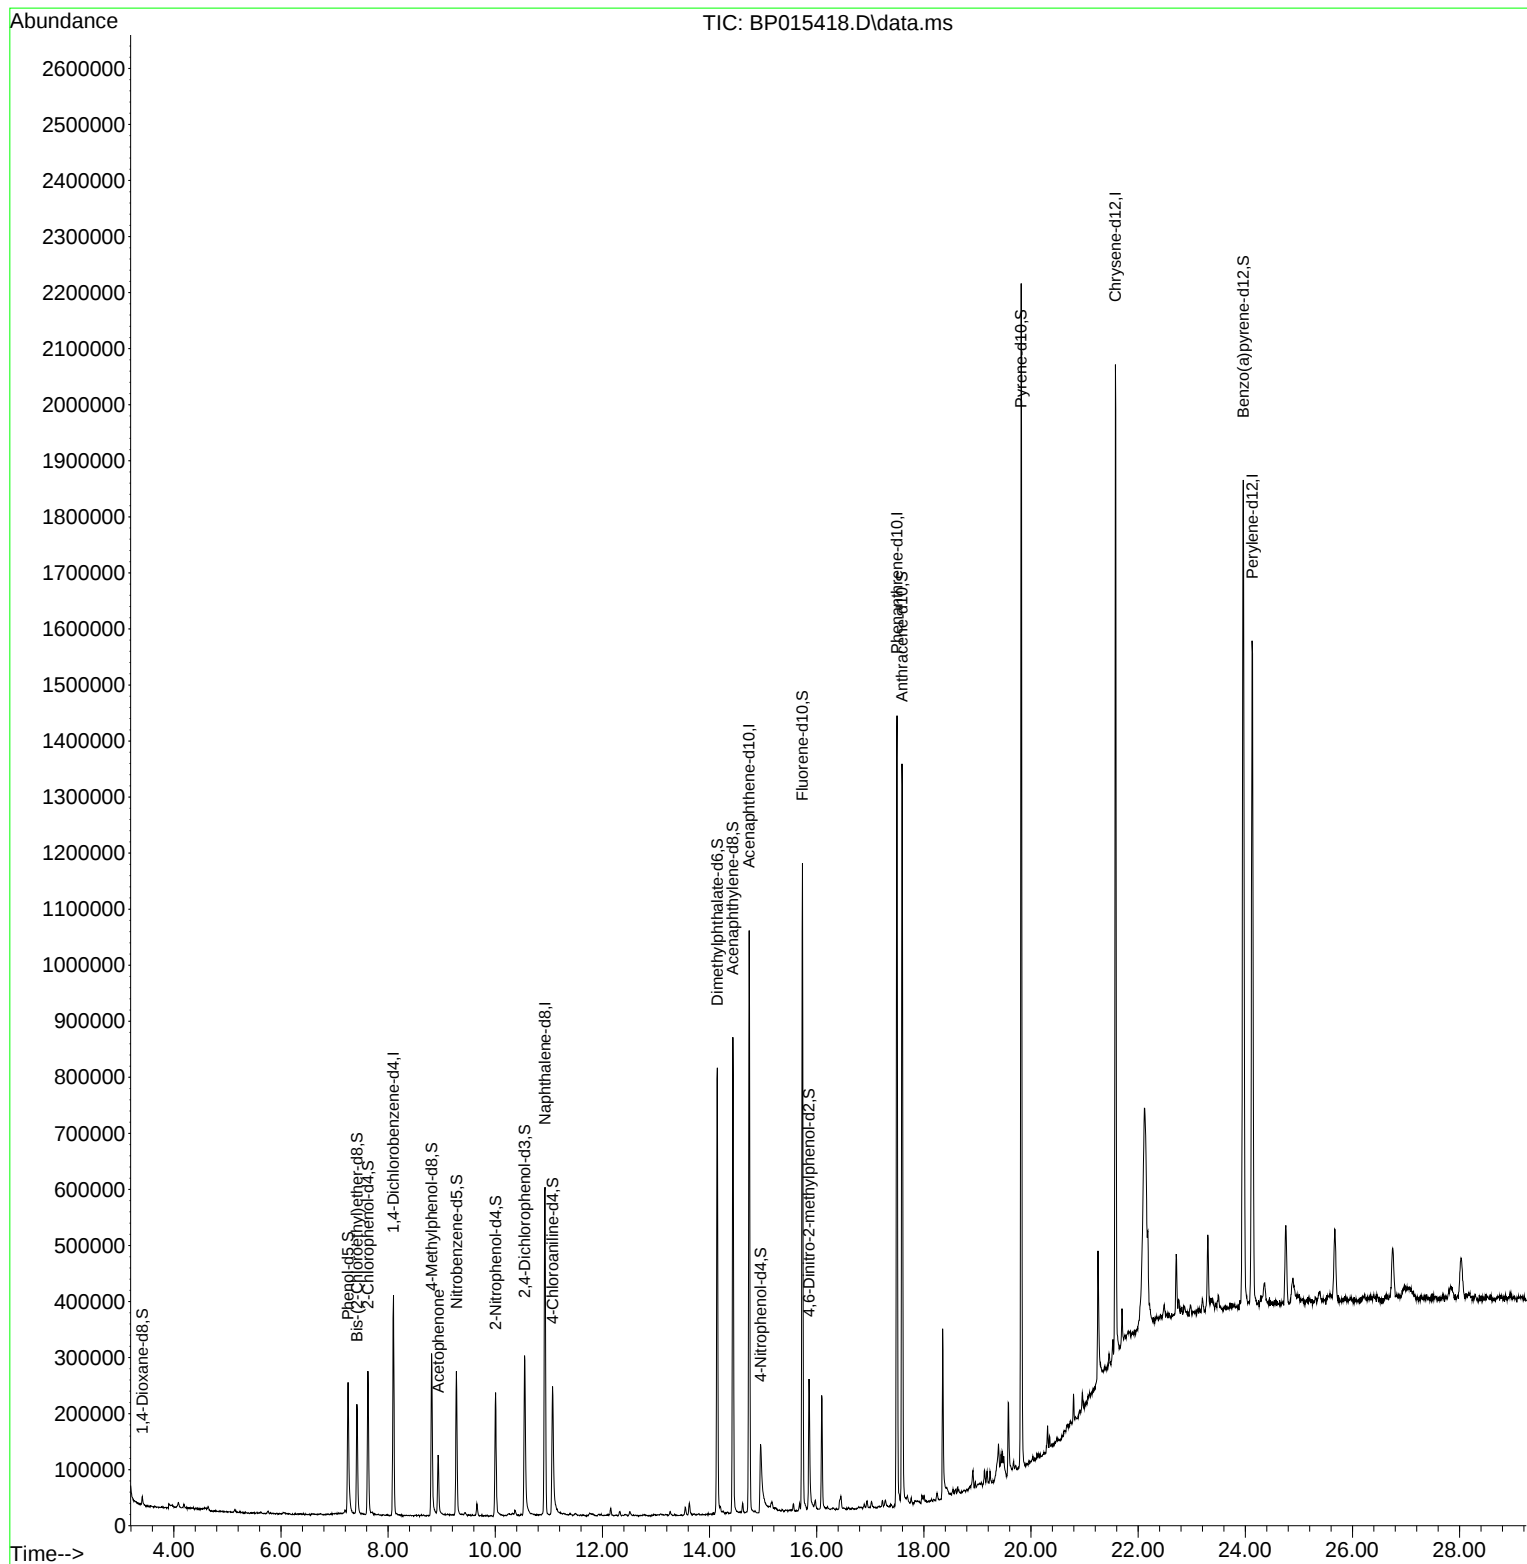

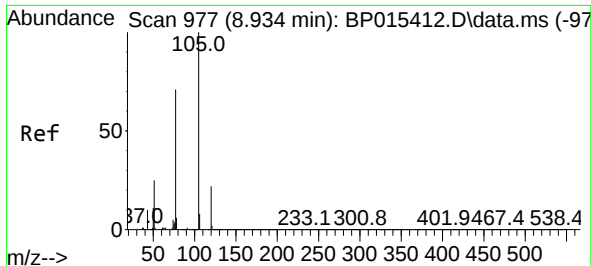

#16
 Acetophenone
 Concen: 4.694 ng/ul
 RT: 8.934 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BP015418.D
 Acq: 08 Jun 2023 03:04

Instrument :
 BNA_P
 ClientSampleId :
 EW995

Tgt Ion:	105	Resp:	58121
Ion Ratio	Lower	Upper	
105	100		
77	78.3	64.9	97.3
51	27.8	23.5	35.3

