

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
 Data File : BP015397.D
 Acq On : 07 Jun 2023 14:12
 Operator : MA/JU
 Sample : PB153099BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK099

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015397.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.411	34	38	51	rVB	50892	77902	1.40%	0.154%
2	3.852	111	113	127	rBV	520780	870900	15.66%	1.716%
3	4.187	167	170	174	rBV2	7234	11085	0.20%	0.022%
4	7.252	684	691	703	rBV	683532	1145377	20.59%	2.257%
5	7.422	713	720	731	rBV	597819	935627	16.82%	1.844%
6	7.628	746	755	765	rBV	708699	1197927	21.53%	2.361%
7	8.099	828	835	845	rBV	475025	763306	13.72%	1.504%
8	8.811	949	956	974	rBV	870156	1512809	27.19%	2.981%
9	9.275	1028	1035	1050	rBV	738499	1245067	22.38%	2.453%
10	10.005	1151	1159	1172	rBV	651285	1110538	19.96%	2.188%
11	10.546	1239	1251	1274	rBV	817085	1561276	28.07%	3.077%
12	10.928	1307	1316	1327	rBV	685469	1155172	20.77%	2.276%
13	11.069	1331	1340	1361	rBV	1027815	1967364	35.36%	3.877%
14	12.516	1580	1586	1600	rBV4	12650	33988	0.61%	0.067%
15	13.628	1768	1775	1782	rBV2	19933	35302	0.63%	0.070%
16	14.146	1853	1863	1878	rBV	2095975	2934771	52.75%	5.783%
17	14.257	1880	1882	1887	rVB6	3843	5985	0.11%	0.012%
18	14.440	1904	1913	1928	rBV	2137452	3161614	56.83%	6.230%
19	14.745	1958	1965	1973	rBV	1165498	1696587	30.50%	3.343%
20	14.945	1992	1999	2031	rBV	536952	1278935	22.99%	2.520%
21	15.734	2126	2133	2148	rBV	2677367	3986077	71.65%	7.855%
22	15.857	2148	2154	2170	rVV	810764	1353920	24.34%	2.668%
23	15.975	2171	2174	2182	rVB5	20379	38934	0.70%	0.077%
24	16.528	2263	2268	2271	rBV7	3951	6149	0.11%	0.012%
25	17.175	2375	2378	2384	rVB8	4277	7590	0.14%	0.015%
26	17.498	2426	2433	2443	rBV	1577631	2250419	40.45%	4.435%
27	17.598	2443	2450	2468	rVV	3236938	4607200	82.82%	9.079%
28	19.398	2752	2756	2761	rBV	46460	63513	1.14%	0.125%
29	19.469	2764	2768	2774	rVB	40298	56689	1.02%	0.112%
30	19.822	2822	2828	2842	rBV	4228018	5563045	100.00%	10.962%
31	21.580	3122	3127	3137	rBV	1737280	2436375	43.80%	4.801%
32	23.969	3526	3533	3549	rVB2	2501199	5312617	95.50%	10.469%
33	24.139	3555	3562	3574	rVB	1089782	2363702	42.49%	4.658%




Sum of corrected areas: 50747762

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
Data File : BP015397.D
Acq On : 07 Jun 2023 14:12
Operator : MA/JU
Sample : PB153099BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK099

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

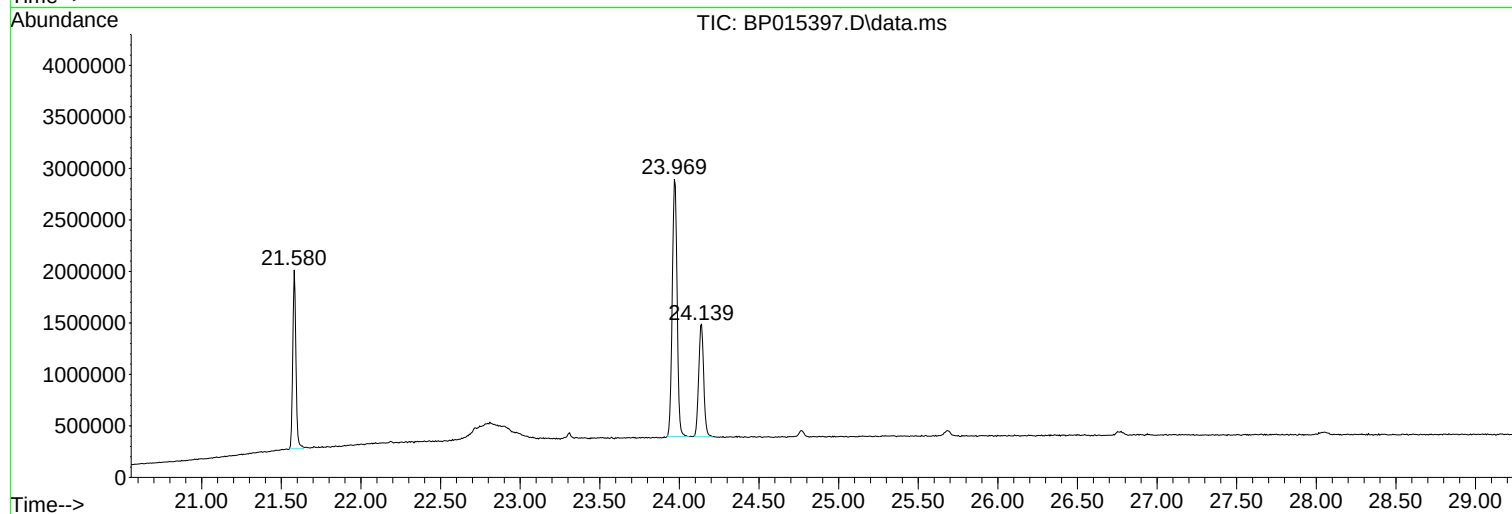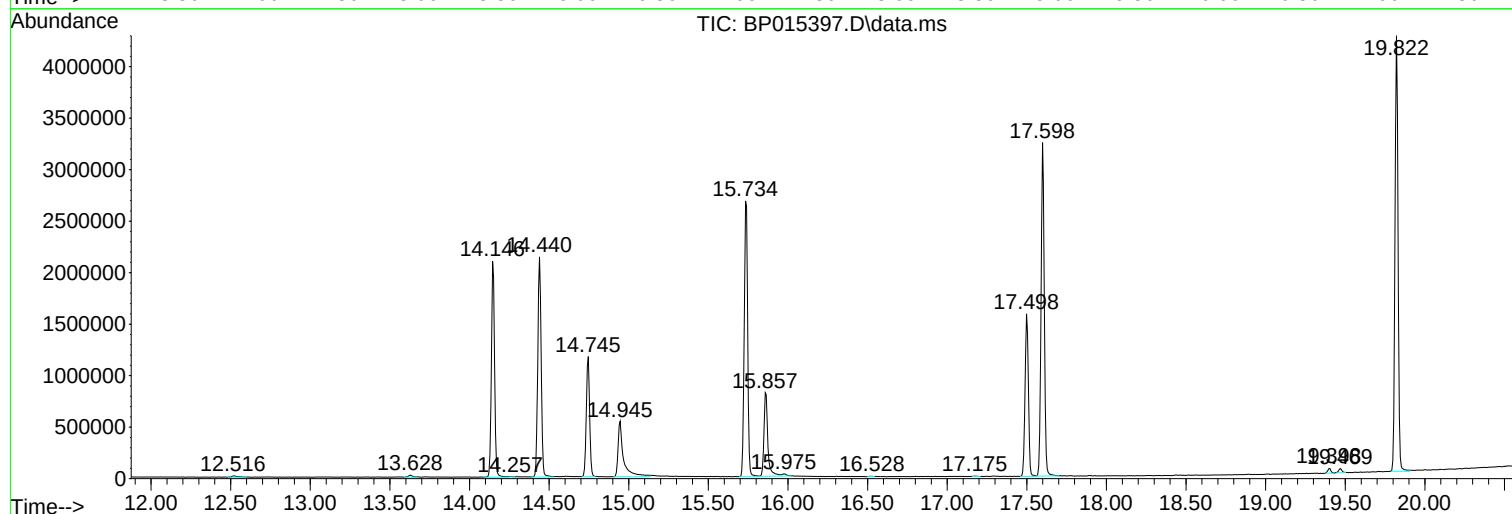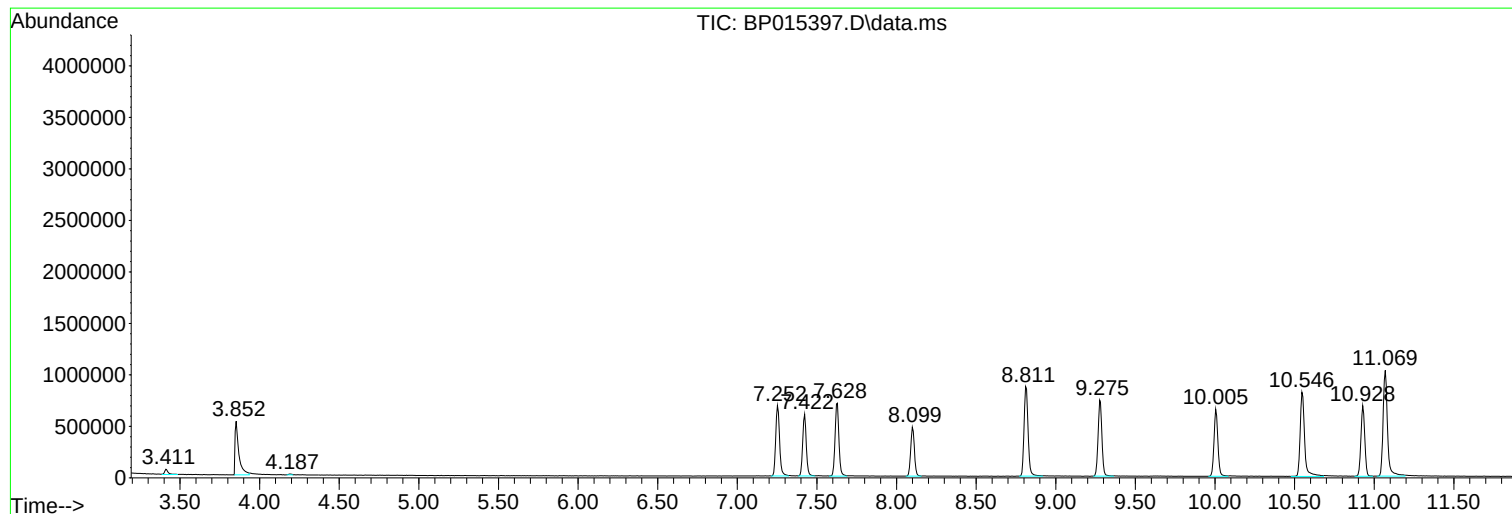

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
Data File : BP015397.D
Acq On : 07 Jun 2023 14:12
Operator : MA/JU
Sample : PB153099BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK099

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
Data File : BP015397.D
Acq On : 07 Jun 2023 14:12
Operator : MA/JU
Sample : PB153099BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK099

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc