

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
 Data File : BP015413.D
 Acq On : 07 Jun 2023 23:10
 Operator : MA/JU
 Sample : PB153099BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK099

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.411	34	38	54	rVB	44342	77433	1.34%	0.146%
2	3.852	110	113	134	rBV	469842	869017	14.98%	1.643%
3	4.187	167	170	175	rVB3	6660	10008	0.17%	0.019%
4	7.252	684	691	706	rBV	652430	1101940	19.00%	2.084%
5	7.416	713	719	732	rVB	551586	892138	15.38%	1.687%
6	7.622	746	754	770	rBV	693712	1158254	19.97%	2.190%
7	8.099	828	835	844	rBV	459369	739699	12.75%	1.399%
8	8.810	949	956	973	rBV	888504	1498730	25.84%	2.834%
9	9.275	1028	1035	1045	rBV	726612	1214963	20.95%	2.297%
10	10.004	1152	1159	1169	rBV	638524	1090128	18.80%	2.061%
11	10.546	1243	1251	1272	rBV	838543	1560394	26.90%	2.950%
12	10.928	1308	1316	1324	rBV	719402	1239897	21.38%	2.344%
13	11.063	1329	1339	1362	rBV	989981	1944651	33.53%	3.677%
14	12.516	1580	1586	1597	rVB2	14273	32689	0.56%	0.062%
15	13.622	1768	1774	1783	rVV2	20053	33020	0.57%	0.062%
16	14.145	1856	1863	1876	rBV	1972283	2796237	48.21%	5.287%
17	14.434	1904	1912	1924	rBV	1985363	3103854	53.52%	5.869%
18	14.740	1957	1964	1973	rBV	1358348	1985562	34.24%	3.754%
19	14.940	1992	1998	2019	rBV	544278	1250159	21.56%	2.364%
20	15.140	2030	2032	2044	rVB	8535	18075	0.31%	0.034%
21	15.734	2126	2133	2146	rBV	2745646	3872022	66.76%	7.321%
22	15.857	2148	2154	2170	rVV	942749	1407969	24.28%	2.662%
23	15.975	2170	2174	2180	rVB4	16019	28746	0.50%	0.054%
24	16.522	2260	2267	2270	rBV9	4460	6384	0.11%	0.012%
25	17.286	2393	2397	2402	rBV7	4941	7476	0.13%	0.014%
26	17.498	2426	2433	2443	rBV	1810268	2643320	45.58%	4.998%
27	17.598	2443	2450	2470	rVB	3144690	4485521	77.34%	8.481%
28	19.398	2751	2756	2762	rBV3	47111	71220	1.23%	0.135%
29	19.469	2763	2768	2774	rVV2	41121	65745	1.13%	0.124%
30	19.822	2821	2828	2838	rBV	4071501	5469867	94.31%	10.342%
31	21.574	3121	3126	3139	rBV	2237207	3246882	55.98%	6.139%
32	23.963	3525	3532	3545	rVB2	2676916	5799755	100.00%	10.966%
33	24.133	3553	3561	3571	rVB	1426898	3165958	54.59%	5.986%


Sum of corrected areas: 52887713

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
Data File : BP015413.D
Acq On : 07 Jun 2023 23:10
Operator : MA/JU
Sample : PB153099BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK099

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

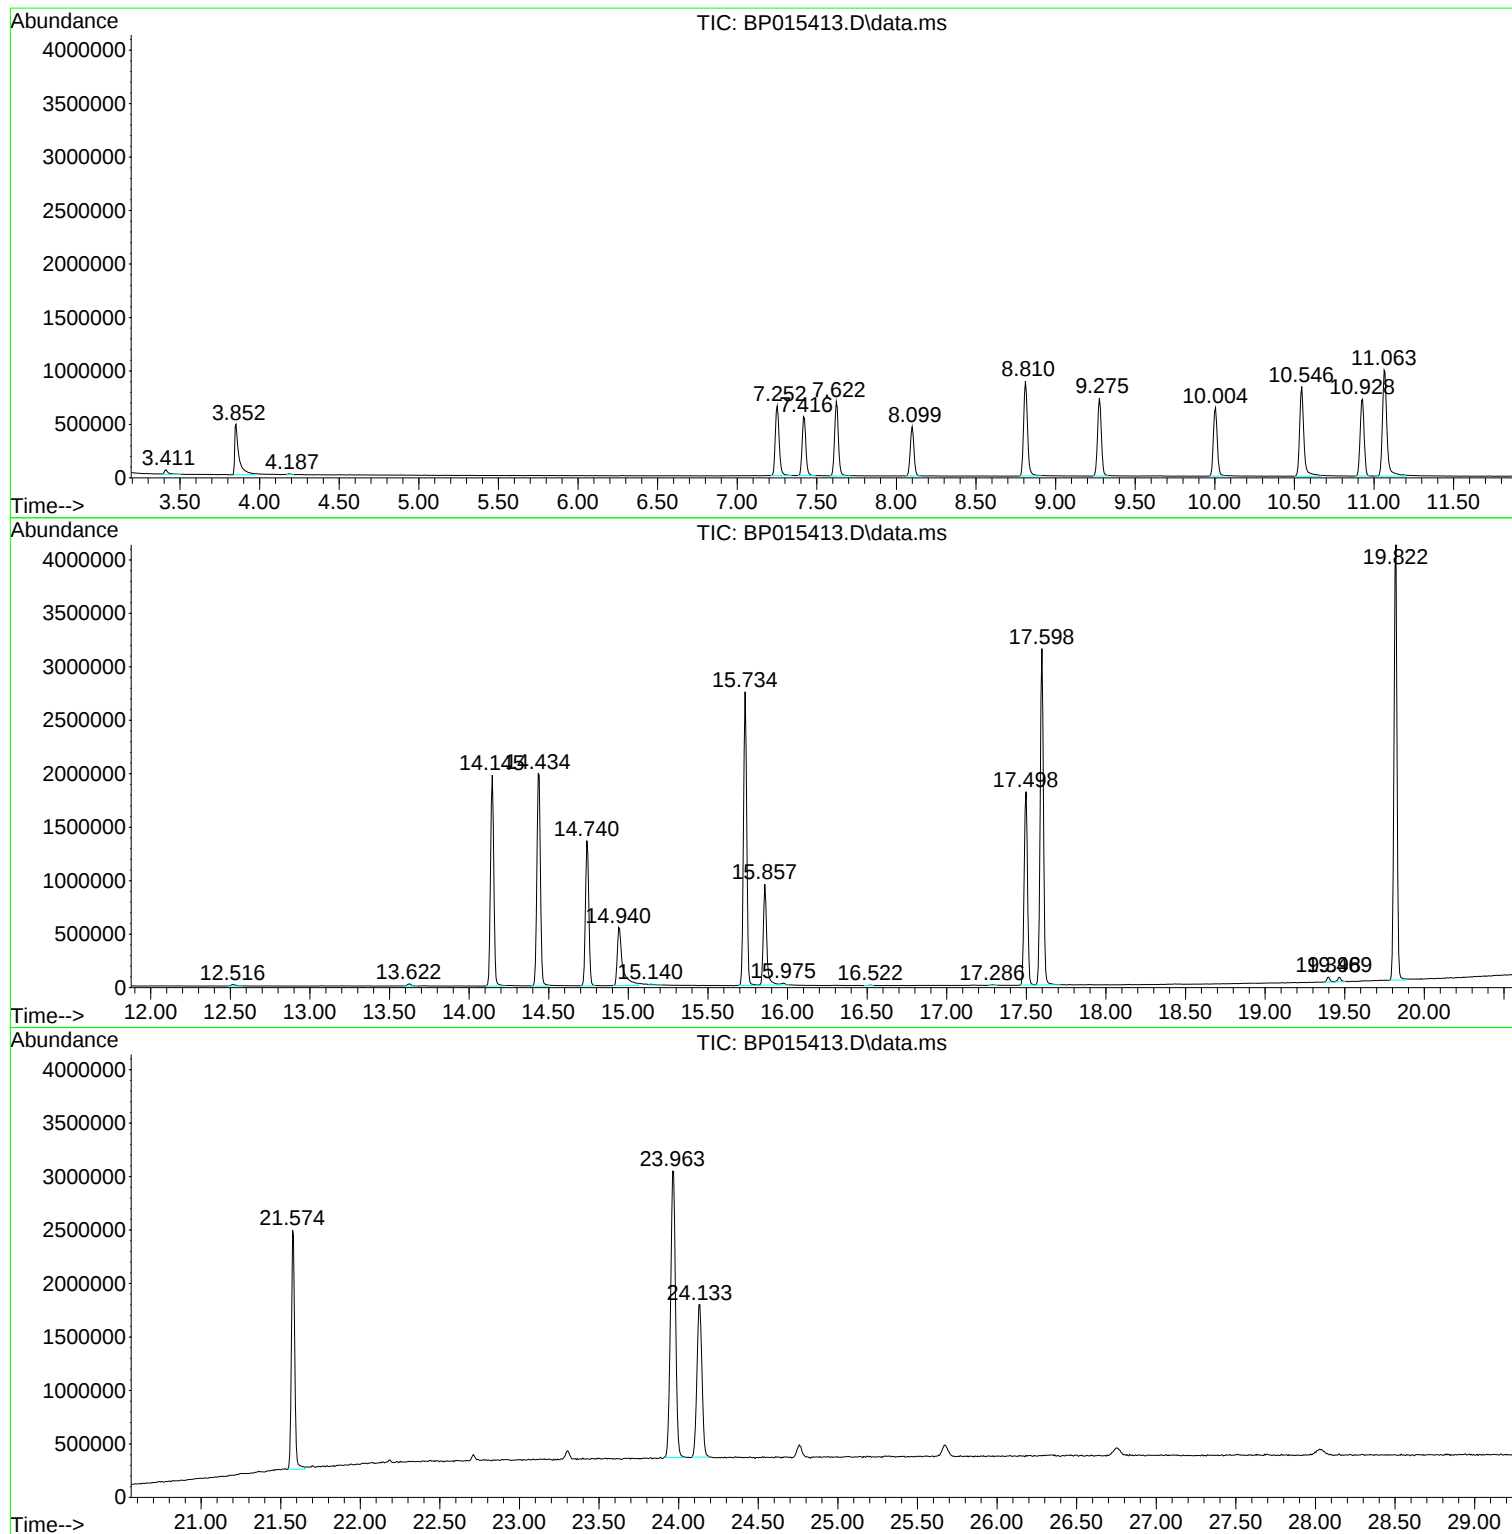

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
Data File : BP015413.D
Acq On : 07 Jun 2023 23:10
Operator : MA/JU
Sample : PB153099BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK099

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060723\
Data File : BP015413.D
Acq On : 07 Jun 2023 23:10
Operator : MA/JU
Sample : PB153099BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK099

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------