

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
 Data File : BP015430.D
 Acq On : 08 Jun 2023 11:33
 Operator : MA/JU
 Sample : 02951-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW999

Quant Time: Jun 09 01:15:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 07 23:46:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	122324	20.000	ng/ul	0.00
20) Naphthalene-d8	10.928	136	580179	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.740	164	406375	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.498	188	976861	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240	1032806	20.000	ng/ul	0.00
88) Perylene-d12	24.133	264	1122712	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.411	96	11922	3.609	ng/uL	0.00
4) Pyridine-d5	3.852	84	119	0.014	ng/ul	0.00
7) Phenol-d5	7.252	99	196515	17.438	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.416	67	131594	19.553	ng/ul	0.00
11) 2-Chlorophenol-d4	7.622	132	162674	19.910	ng/ul	0.00
15) 4-Methylphenol-d8	8.810	113	161981	17.514	ng/ul	0.00
21) Nitrobenzene-d5	9.275	128	87319	19.170	ng/ul	0.00
24) 2-Nitrophenol-d4	10.005	143	104925	20.171	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.546	165	176929	18.646	ng/ul	0.00
31) 4-Chloroaniline-d4	11.069	131	192957	14.167	ng/ul	0.00
46) Dimethylphthalate-d6	14.145	166	699609	21.832	ng/ul	0.00
49) Acenaphthylene-d8	14.434	160	730156	20.838	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	76183	13.276	ng/ul	0.00
60) Fluorene-d10	15.734	176	593617	21.967	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	98964	15.992	ng/ul	0.00
73) Anthracene-d10	17.598	188	981411	22.081	ng/ul	0.00
81) Pyrene-d10	19.816	212	870953	15.756	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.963	264	534372	9.486	ng/ul	-0.01
Target Compounds						
					Qvalue	
8) Phenol	7.281	94	12980	1.116	ng/ul	95
16) Acetophenone	8.934	105	86528	5.862	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
Data File : BP015430.D
Acq On : 08 Jun 2023 11:33
Operator : MA/JU
Sample : 02951-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW999

Quant Time: Jun 09 01:15:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 07 23:46:15 2023
Response via : Initial Calibration




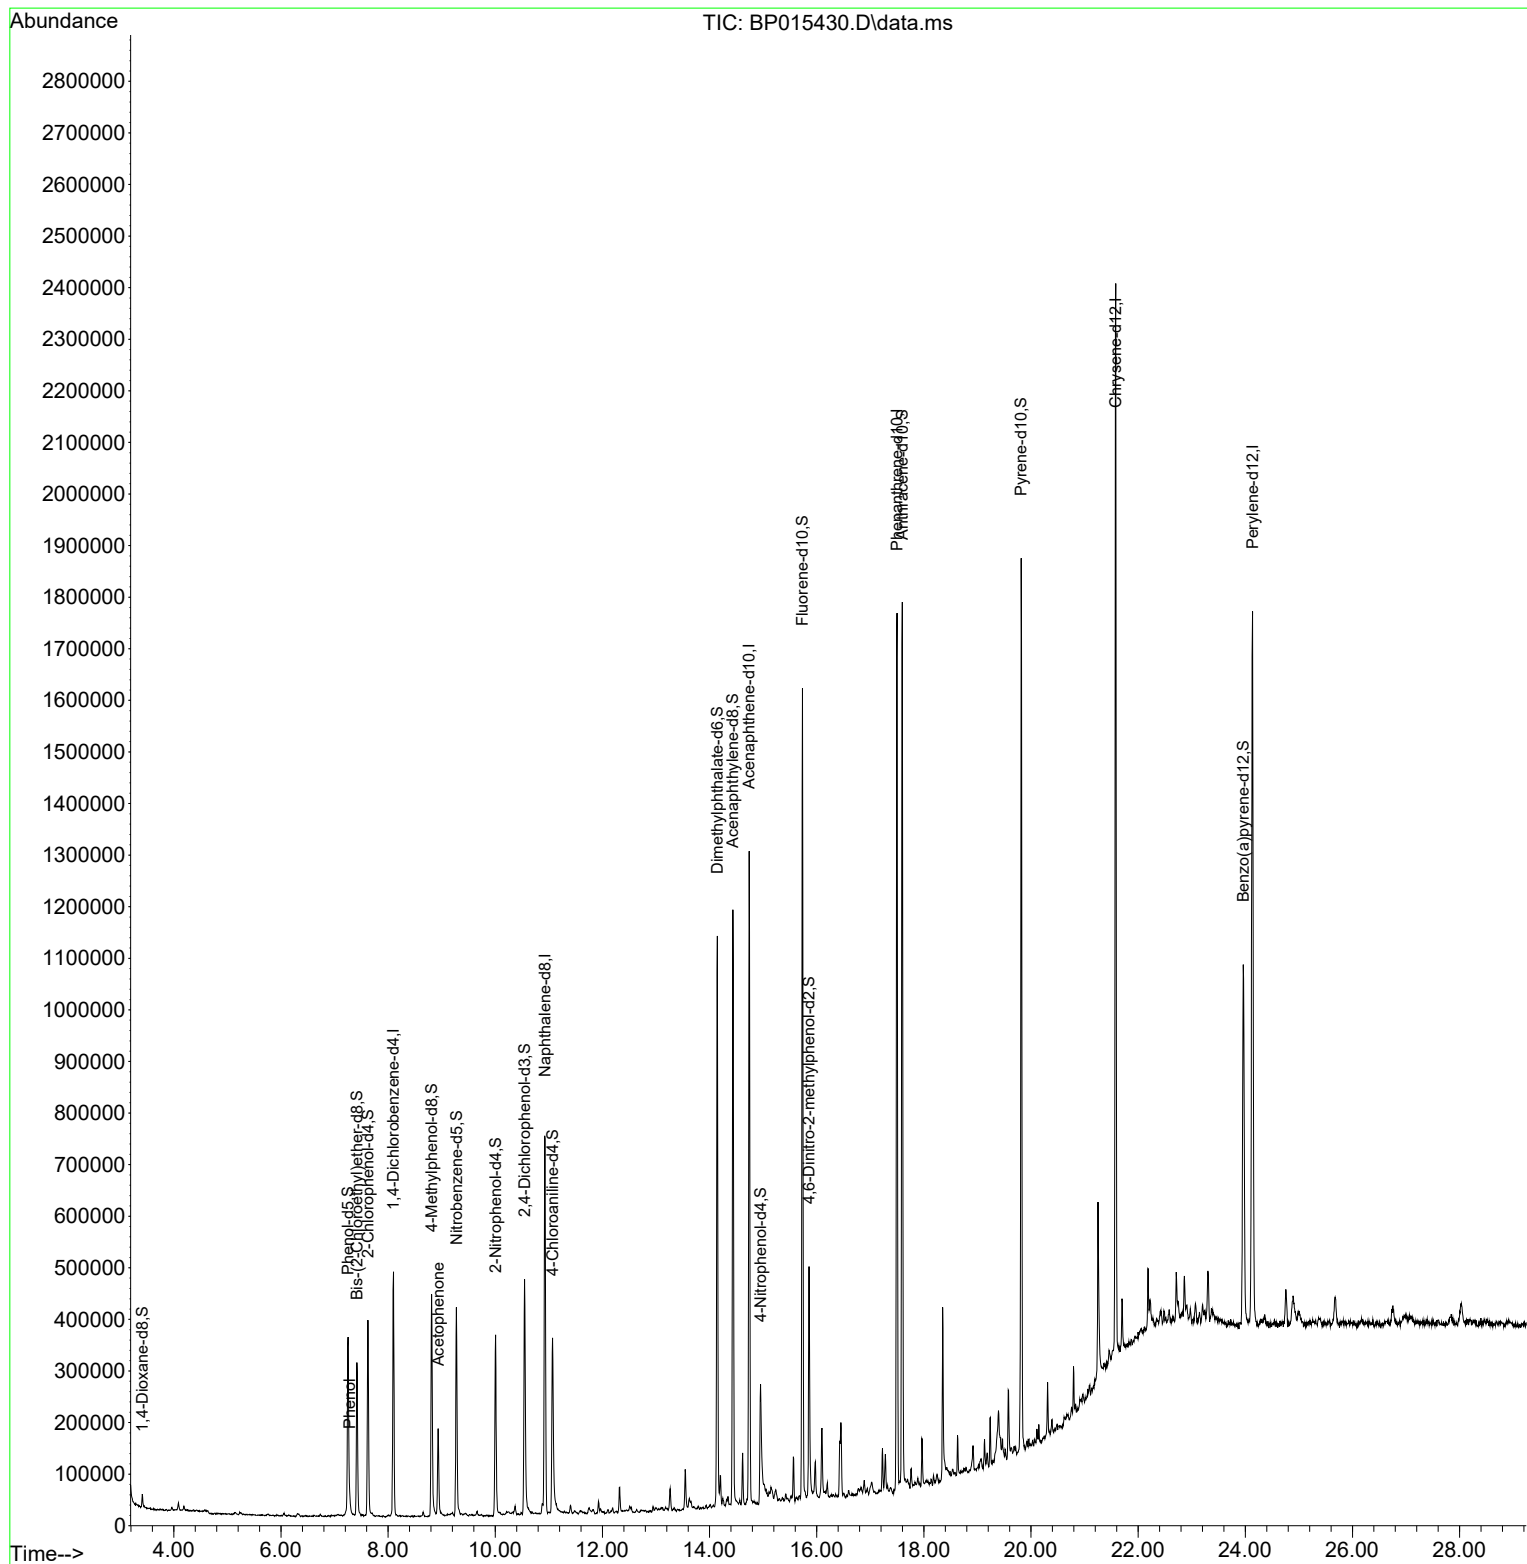


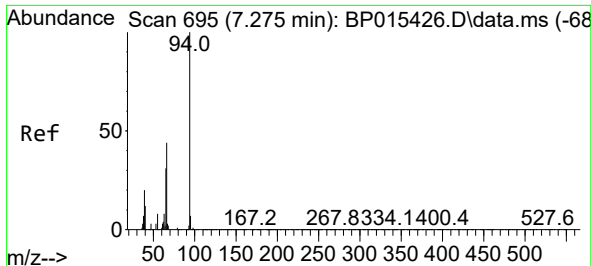

#8
Phenol
Concen: 1.116 ng/ul
RT: 7.281 min Scan# 695
Delta R.T. -0.000 min
Lab File: BP015430.D
Acq: 08 Jun 2023 11:33

Instrument :
BNA_P
ClientSampleId :
EW999

Tgt Ion: 94 Resp: 12980
Ion Ratio Lower Upper
94 100
65 31.8 23.5 35.3
66 46.1 34.2 51.4

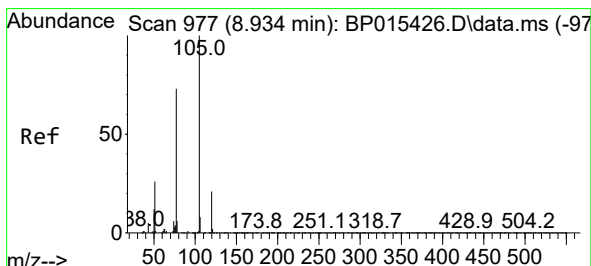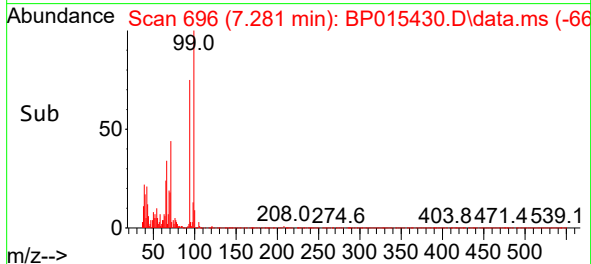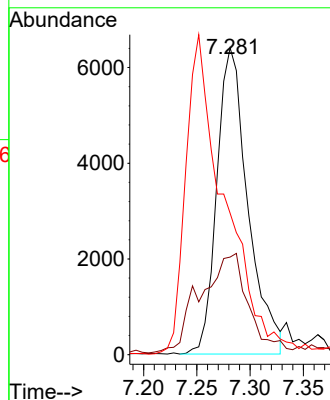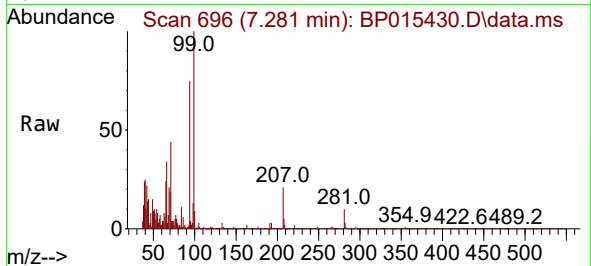

#16
Acetophenone
Concen: 5.862 ng/ul
RT: 8.934 min Scan# 977
Delta R.T. -0.000 min
Lab File: BP015430.D
Acq: 08 Jun 2023 11:33

Tgt Ion: 105 Resp: 86528
Ion Ratio Lower Upper
105 100
77 79.5 64.9 97.3
51 29.1 23.5 35.3

