

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
 Data File : BP015444.D
 Acq On : 08 Jun 2023 20:33
 Operator : MA/JU
 Sample : 02950-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW992

Quant Time: Jun 09 01:20:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 07 23:46:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	129037	20.000	ng/ul	0.00
20) Naphthalene-d8	10.922	136	586323	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.740	164	403873	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.492	188	954372	20.000	ng/ul	-0.01
79) Chrysene-d12	21.575	240	960690	20.000	ng/ul	-0.01
88) Perylene-d12	24.127	264	1037126	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.411	96	13276	3.810	ng/uL	0.00
4) Pyridine-d5	3.864	84	46603	5.149	ng/ul	0.01
7) Phenol-d5	7.246	99	245761	20.674	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.417	67	159604	22.481	ng/ul	0.00
11) 2-Chlorophenol-d4	7.622	132	197378	22.901	ng/ul	0.00
15) 4-Methylphenol-d8	8.811	113	212212	21.751	ng/ul	0.00
21) Nitrobenzene-d5	9.275	128	101898	22.136	ng/ul	0.00
24) 2-Nitrophenol-d4	9.999	143	118074	22.461	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.546	165	209626	21.860	ng/ul	0.00
31) 4-Chloroaniline-d4	11.063	131	261646	19.009	ng/ul	0.00
46) Dimethylphthalate-d6	14.140	166	788058	24.744	ng/ul	-0.01
49) Acenaphthylene-d8	14.434	160	842449	24.191	ng/ul	0.00
54) 4-Nitrophenol-d4	14.946	143	87508	15.344	ng/ul	0.00
60) Fluorene-d10	15.728	176	661108	24.616	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.857	200	107584	17.794	ng/ul	0.00
73) Anthracene-d10	17.592	188	1093251	25.177	ng/ul	0.00
81) Pyrene-d10	19.816	212	1370786	26.660	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.957	264	1340450	25.759	ng/ul	-0.02
Target Compounds						
					Qvalue	
16) Acetophenone	8.934	105	66032	4.241	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
Data File : BP015444.D
Acq On : 08 Jun 2023 20:33
Operator : MA/JU
Sample : 02950-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW992


Quant Time: Jun 09 01:20:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 07 23:46:15 2023
Response via : Initial Calibration

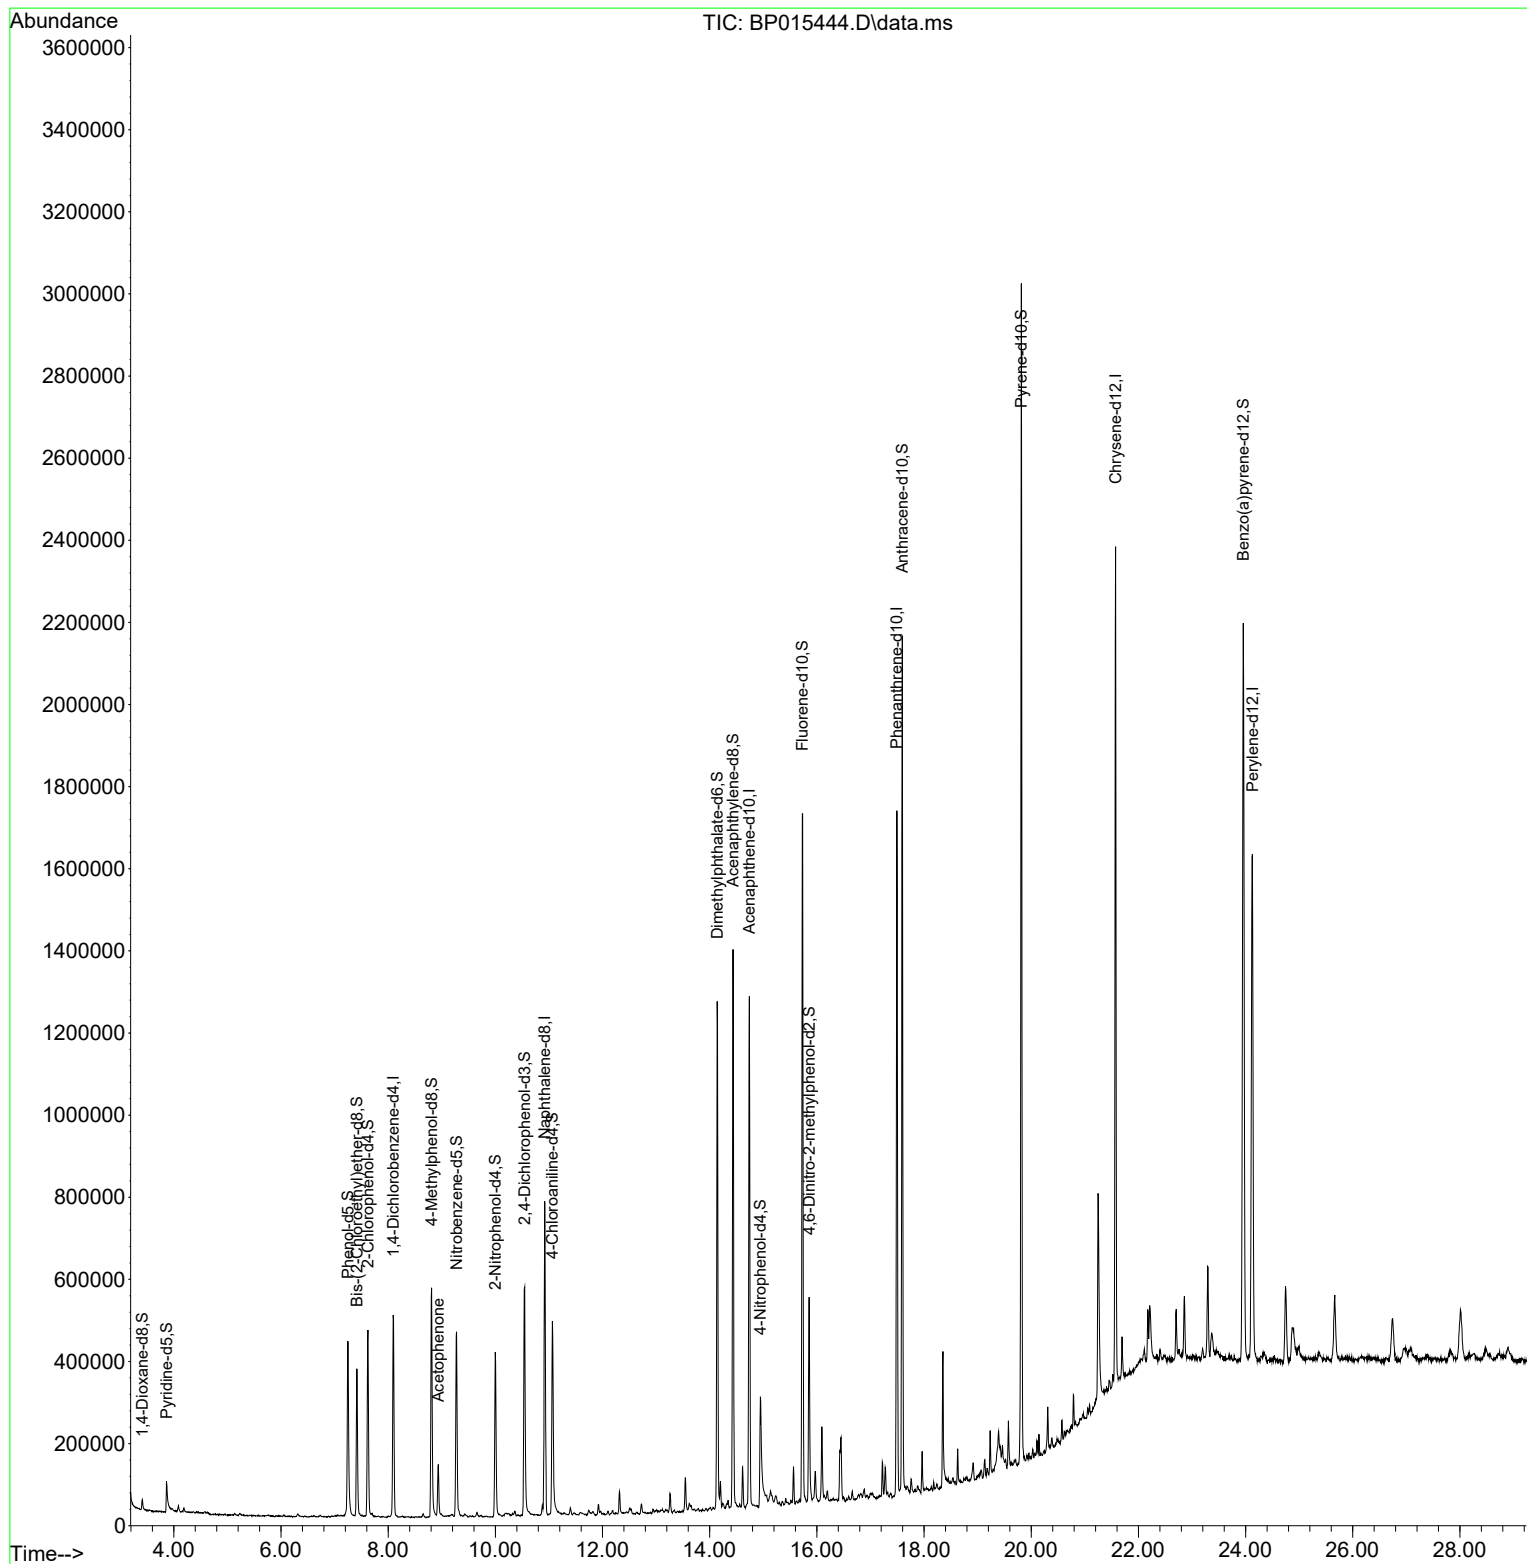

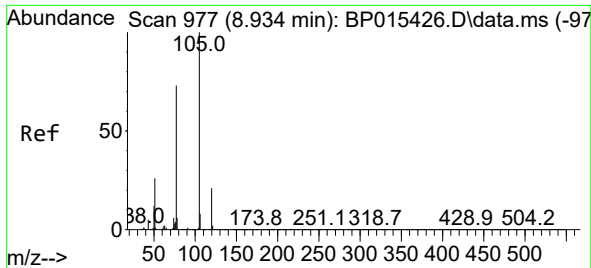

#16
 Acetophenone
 Concen: 4.241 ng/ul
 RT: 8.934 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BP015444.D
 Acq: 08 Jun 2023 20:33

Instrument :
 BNA_P
 ClientSampleId :
 EW992

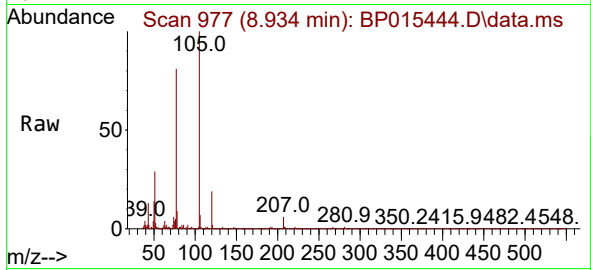

Tgt Ion:	105	Resp:	66032
Ion	Ratio	Lower	Upper
105	100		
77	81.0	64.9	97.3
51	28.9	23.5	35.3

