

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
 Data File : BP015433.D
 Acq On : 08 Jun 2023 13:15
 Operator : MA/JU
 Sample : 02960-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0FN8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/09/2023
 Supervised By :Sohil Jodhani 06/09/2023

Quant Time: Jun 09 01:34:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 07 23:46:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	116809	20.000	ng/u1	0.00
20) Naphthalene-d8	10.928	136	526953	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.740	164	382925	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.498	188	921509	20.000	ng/u1	0.00
79) Chrysene-d12	21.580	240	931048	20.000	ng/u1	0.00
88) Perylene-d12	24.133	264	981325	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.411	96	8075	2.560	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.252	99	138024	12.826	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.416	67	93886	14.609	ng/u1	0.00
11) 2-Chlorophenol-d4	7.622	132	112231	14.385	ng/u1	0.00
15) 4-Methylphenol-d8	8.810	113	89504	10.134	ng/u1	0.00
21) Nitrobenzene-d5	9.275	128	59914	14.482	ng/u1	0.00
24) 2-Nitrophenol-d4	10.005	143	69589	14.729	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.546	165	115319	13.381	ng/u1	0.00
31) 4-Chloroaniline-d4	11.069	131	137859	11.144	ng/u1	0.00
46) Dimethylphthalate-d6	14.145	166	523007	17.320	ng/u1	0.00
49) Acenaphthylene-d8	14.434	160	534509	16.188	ng/u1	0.00
54) 4-Nitrophenol-d4	14.963	143	41495m	7.674	ng/u1	0.02
60) Fluorene-d10	15.734	176	434903	17.080	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.863	200	58174	9.965	ng/u1	0.00
73) Anthracene-d10	17.598	188	738681	17.618	ng/u1	0.00
81) Pyrene-d10	19.816	212	980097	19.668	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.963	264	907734	18.435	ng/u1	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.940	105	52545	3.728	ng/u1	96
86) Bis(2-ethylhexyl)phtha...	21.457	149	776531	18.928	ng/u1	99
89) Di-n-octyl phthalate	22.427	149	65988	1.023	ng/u1	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
Data File : BP015433.D
Acq On : 08 Jun 2023 13:15
Operator : MA/JU
Sample : 02960-04
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
H0FN8

Quant Time: Jun 09 01:34:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 07 23:46:15 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/09/2023
Supervised By :Sohil Jodhani 06/09/2023

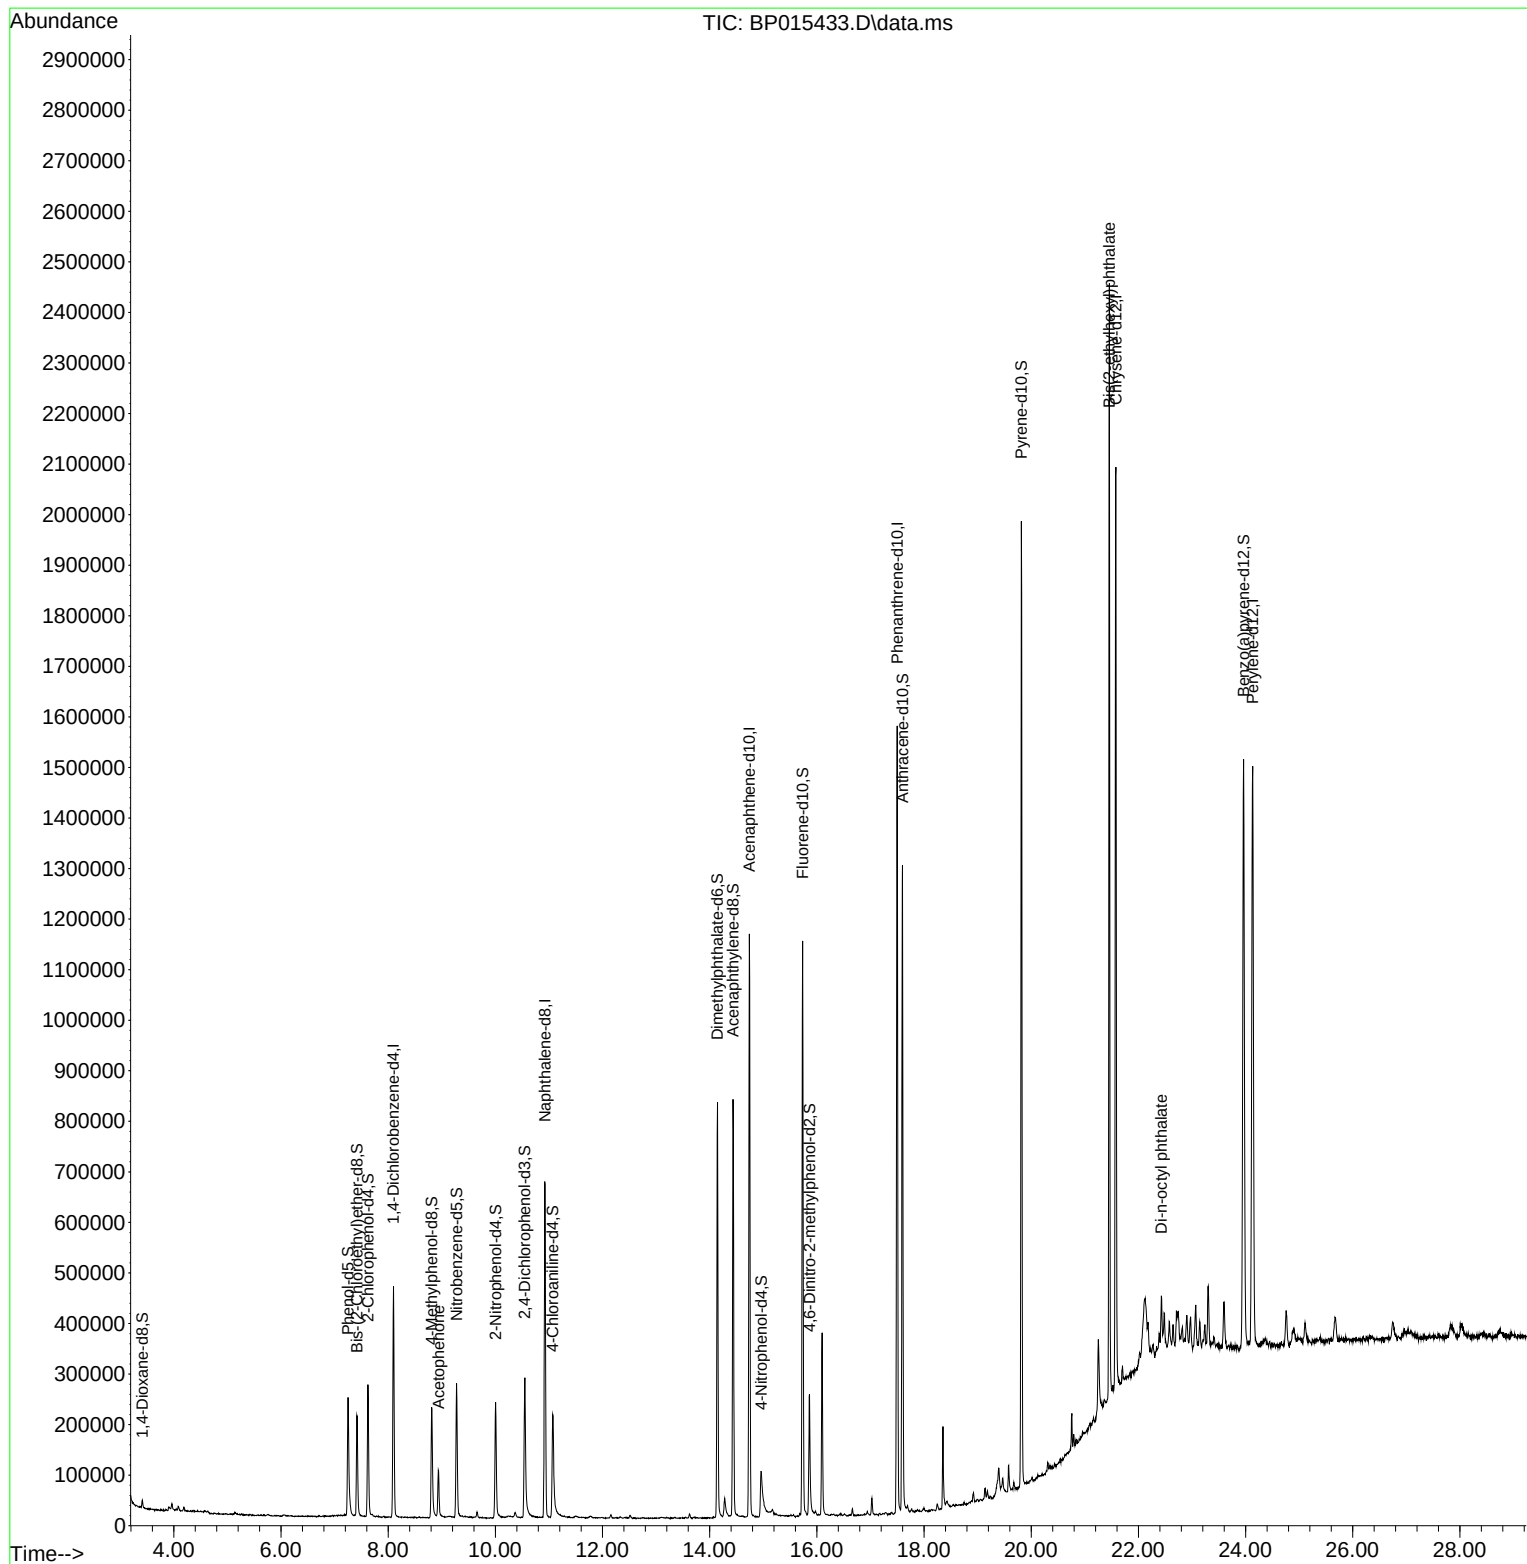

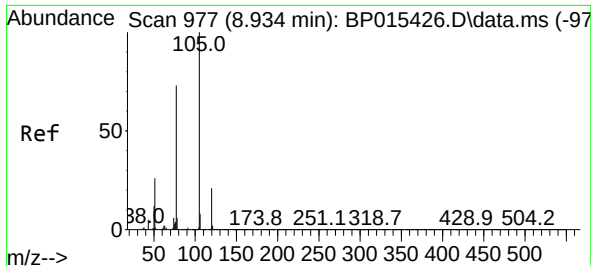





#16
Acetophenone
Concen: 3.728 ng/ul
RT: 8.940 min Scan# 91
Delta R.T. 0.006 min
Lab File: BP015433.D
Acq: 08 Jun 2023 13:15

Instrument :
BNA_P
ClientSampleId :
H0FN8

Tgt Ion:	105	Resp:	5254
Ion Ratio	Lower	Upper	
105	100		
77	76.9	64.9	97.3
51	27.7	23.5	35.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/09/2023
Supervised By :Sohil Jodhani 06/09/2023

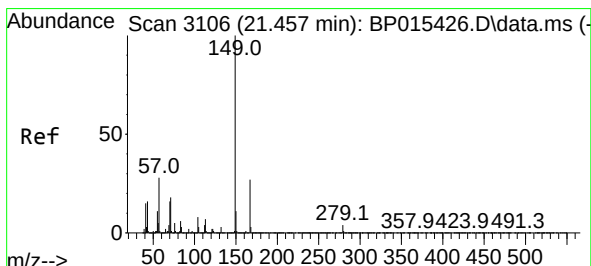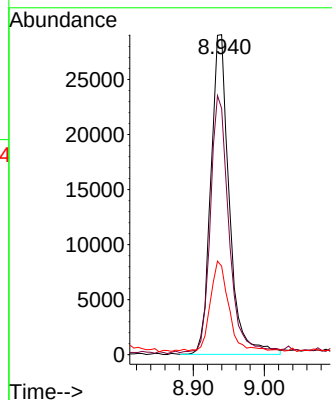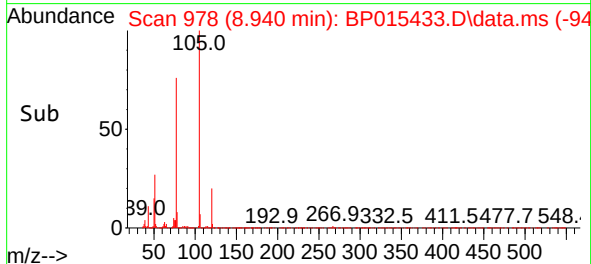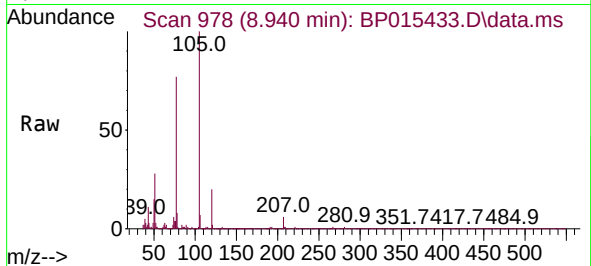

#86
Bis(2-ethylhexyl)phthalate
Concen: 18.928 ng/ul
RT: 21.457 min Scan# 3106
Delta R.T. -0.006 min
Lab File: BP015433.D
Acq: 08 Jun 2023 13:15

Tgt Ion:	149	Resp:	776531
Ion Ratio	Lower	Upper	
149	100		
167	26.9	21.8	32.8
279	4.4	3.7	5.5

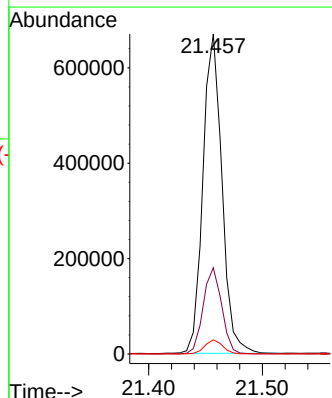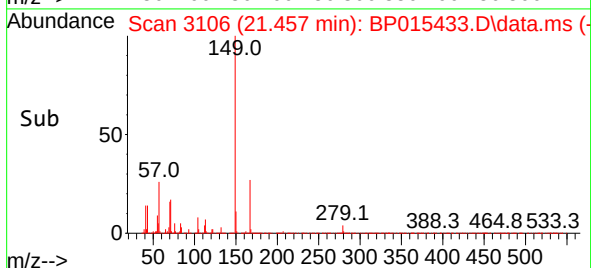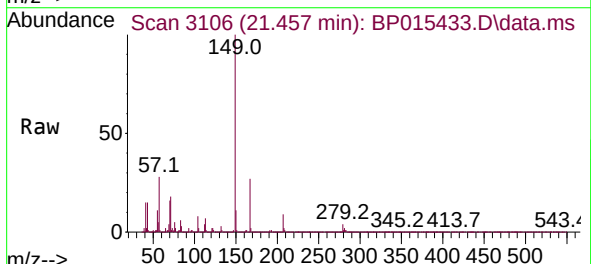

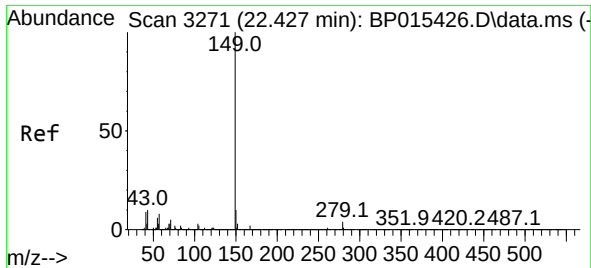

#89
Di-n-octyl phthalate
Concen: 1.023 ng/ul
RT: 22.427 min Scan# 31
Delta R.T. -0.006 min
Lab File: BP015433.D
Acq: 08 Jun 2023 13:15

Instrument :
BNA_P
ClientSampleId :
H0FN8

Tgt Ion:149 Resp: 6598

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/09/2023
Supervised By :Sohil Jodhani 06/09/2023

