

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
 Data File : BP015441.D
 Acq On : 08 Jun 2023 18:52
 Operator : MA/JU
 Sample : 02960-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0FN7

Quant Time: Jun 09 01:53:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 07 23:46:15 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 06/09/2023
 Supervised By :Sohil Jodhani 06/09/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	172828	20.000	ng/u1	0.00
20) Naphthalene-d8	10.922	136	770007	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.740	164	535223	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.498	188	1241632	20.000	ng/u1	0.00
79) Chrysene-d12	21.574	240	1259182	20.000	ng/u1	-0.01
88) Perylene-d12	24.127	264	1368864	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.411	96	6791m	1.455	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.252	99	128092	8.045	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.416	67	84827	8.921	ng/u1	0.00
11) 2-Chlorophenol-d4	7.622	132	103636	8.978	ng/u1	0.00
15) 4-Methylphenol-d8	8.810	113	86730	6.637	ng/u1	0.00
21) Nitrobenzene-d5	9.275	128	53782	8.896	ng/u1	0.00
24) 2-Nitrophenol-d4	10.005	143	59228	8.579	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.546	165	106620	8.466	ng/u1	0.00
31) 4-Chloroaniline-d4	11.069	131	106886	5.913	ng/u1	0.00
46) Dimethylphthalate-d6	14.145	166	419446	9.938	ng/u1	0.00
49) Acenaphthylene-d8	14.434	160	446406	9.673	ng/u1	0.00
54) 4-Nitrophenol-d4	14.963	143	22071m	2.920	ng/u1	0.02
60) Fluorene-d10	15.734	176	357600	10.048	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.863	200	34411	4.375	ng/u1	0.00
73) Anthracene-d10	17.592	188	549510	9.727	ng/u1	0.00
81) Pyrene-d10	19.816	212	771339	11.445	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.957	264	740570	10.782	ng/u1	-0.02
Target Compounds					Qvalue	
16) Acetophenone	8.934	105	110018	5.276	ng/u1	99
72) Phenanthrene	17.539	178	75120	1.127	ng/u1	99
80) Fluoranthene	19.492	202	260495	3.173	ng/u1	98
82) Pyrene	19.845	202	236845	2.789	ng/u1	99
85) Benzo(a)anthracene	21.557	228	131239	1.491	ng/u1	99
87) Chrysene	21.616	228	156452	1.880	ng/u1	97
90) Benzo(b)fluoranthene	23.339	252	207478	2.348	ng/u1#	94
93) Benzo(a)pyrene	24.010	252	127262	1.652	ng/u1	98
96) Benzo(g,h,i)perylene	27.657	276	91013	1.108	ng/u1	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
Data File : BP015441.D
Acq On : 08 Jun 2023 18:52
Operator : MA/JU
Sample : 02960-03
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
H0FN7

Quant Time: Jun 09 01:53:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 07 23:46:15 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/09/2023
Supervised By :Sohil Jodhani 06/09/2023

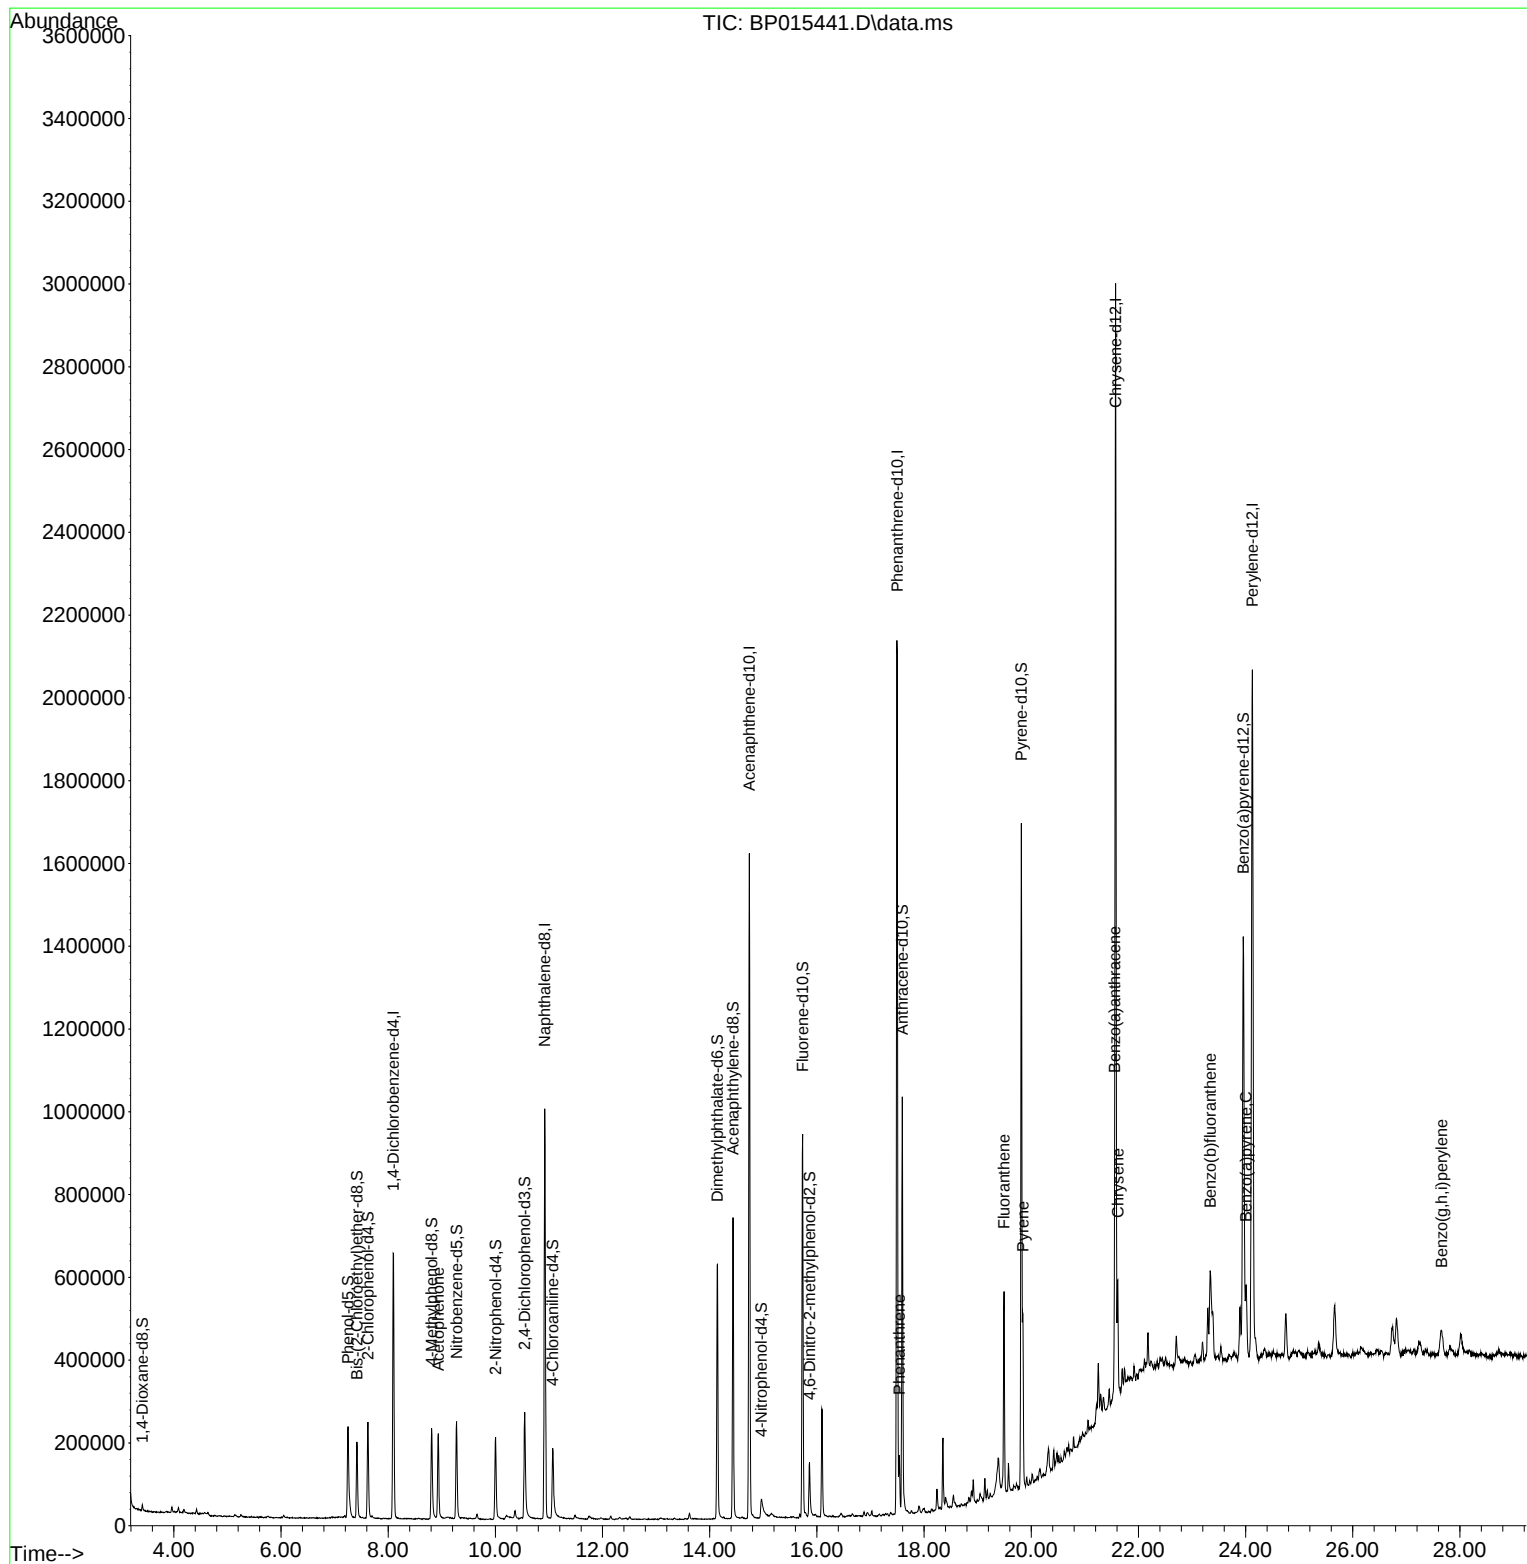

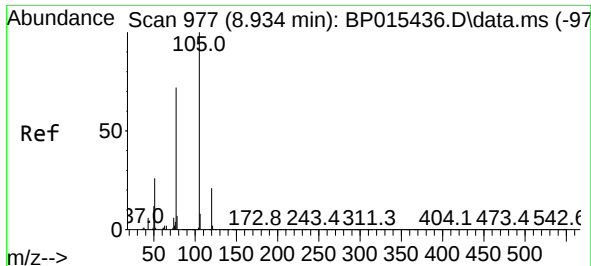





#16
Acetophenone
Concen: 5.276 ng/ul
RT: 8.934 min Scan# 977
Delta R.T. -0.000 min
Lab File: BP015441.D
Acq: 08 Jun 2023 18:52

Instrument :
BNA_P
ClientSampleId :
H0FN7

Tgt Ion:	105	Resp:	110018
Ion Ratio	Lower	Upper	
105	100		
77	80.4	64.9	97.3
51	29.2	23.5	35.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/09/2023
Supervised By :Sohil Jodhani 06/09/2023

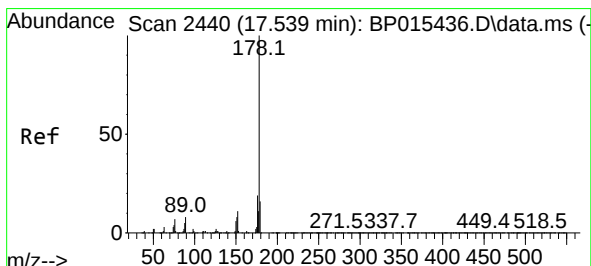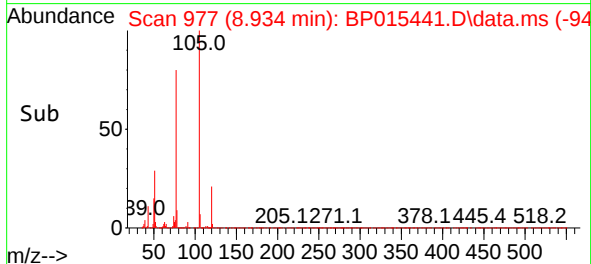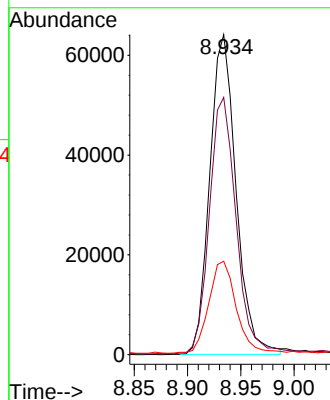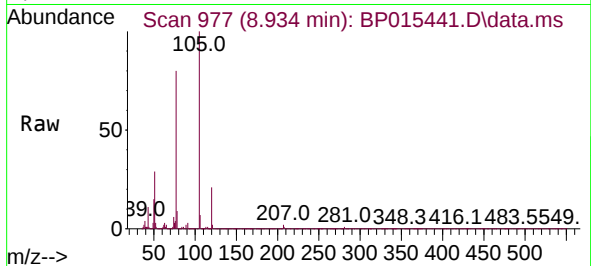

#72
Phenanthrene
Concen: 1.127 ng/ul
RT: 17.539 min Scan# 2440
Delta R.T. -0.006 min
Lab File: BP015441.D
Acq: 08 Jun 2023 18:52


Tgt Ion:	178	Resp:	75120
Ion Ratio	Lower	Upper	
178	100		
179	15.0	12.3	18.5
176	18.9	15.4	23.0

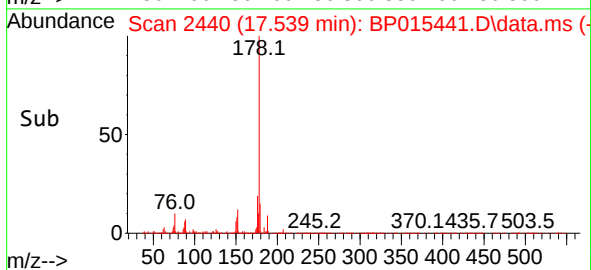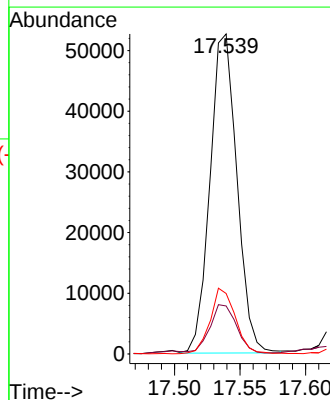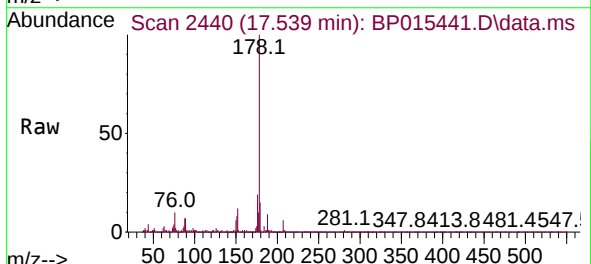

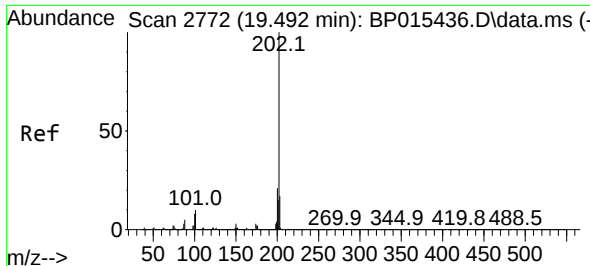

#80
Fluoranthene
Concen: 3.173 ng/u1
RT: 19.492 min Scan# 2772
Delta R.T. -0.006 min
Lab File: BP015441.D
Acq: 08 Jun 2023 18:52




Instrument :
BNA_P
ClientSampleId :
H0FN7

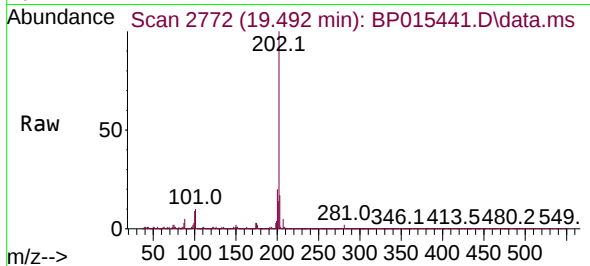

Tgt Ion:202 Resp: 260495
Ion Ratio Lower Upper
202 100
101 10.1 8.6 13.0
100 8.6 6.6 9.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/09/2023
Supervised By :Sohil Jodhani 06/09/2023

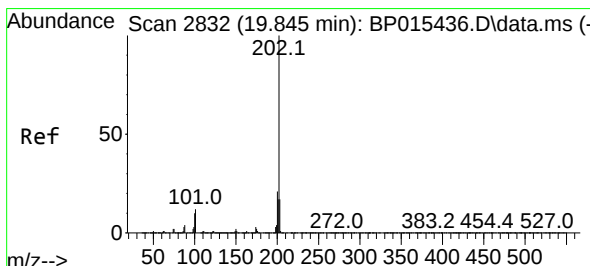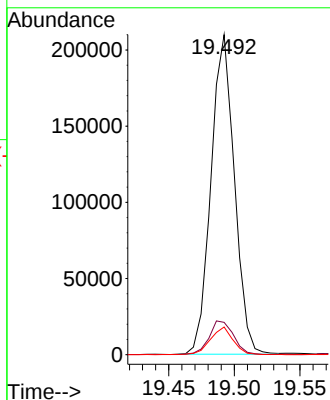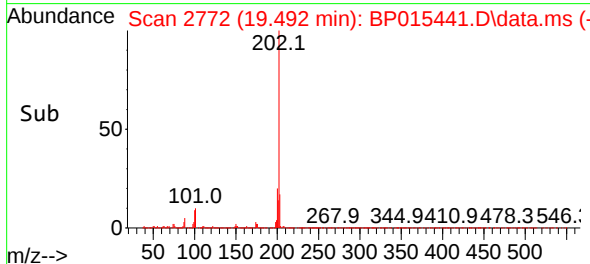

#82
Pyrene
Concen: 2.789 ng/u1
RT: 19.845 min Scan# 2832
Delta R.T. -0.006 min
Lab File: BP015441.D
Acq: 08 Jun 2023 18:52

Tgt Ion:202 Resp: 236845
Ion Ratio Lower Upper
202 100
101 12.1 9.9 14.9
100 10.0 8.4 12.6

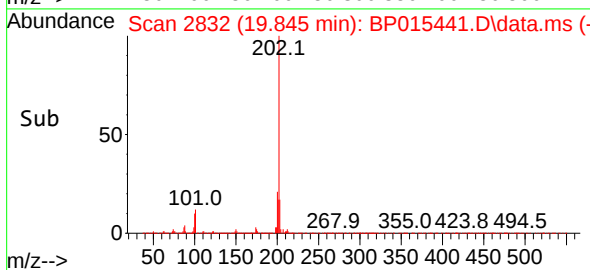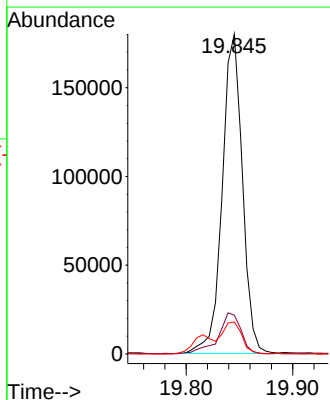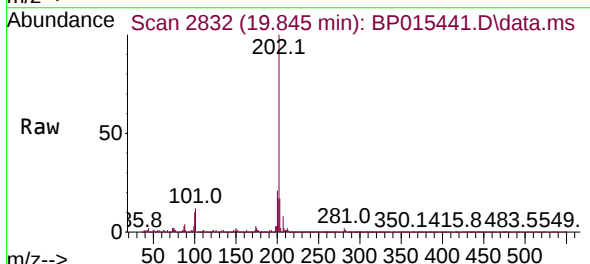

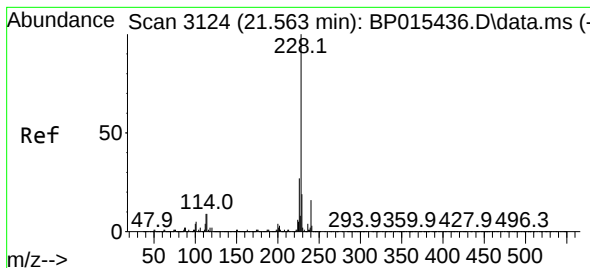

#85

Benzo(a)anthracene

Concen: 1.491 ng/ul

RT: 21.557 min Scan# 3123

Delta R.T. -0.012 min

Lab File: BP015441.D

Acq: 08 Jun 2023 18:52

Instrument :

BNA_P

ClientSampleId :





H0FN7

Tgt Ion:	228	Resp:	131239
Ion Ratio	Lower	Upper	
228	100		
229	20.4	15.8	23.6
226	26.5	21.8	32.6

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/09/2023
Supervised By :Sohil Jodhani 06/09/2023

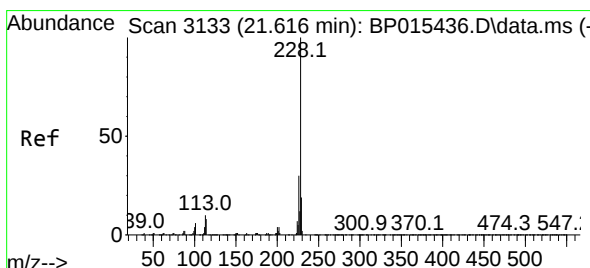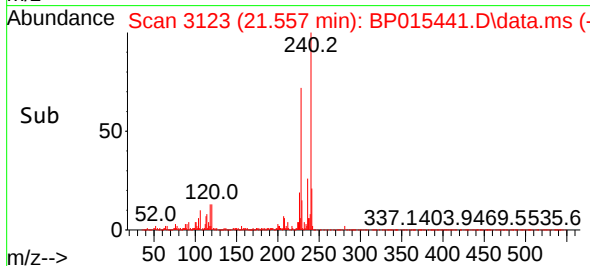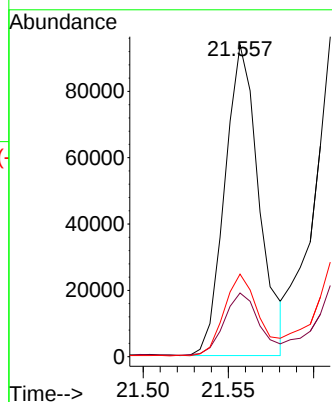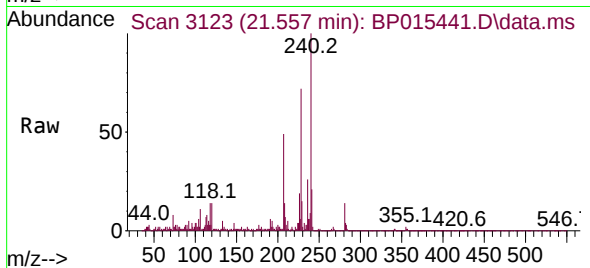

#87

Chrysene

Concen: 1.880 ng/ul




RT: 21.616 min Scan# 3133


Delta R.T. -0.006 min

Lab File: BP015441.D

Acq: 08 Jun 2023 18:52

Tgt Ion:	228	Resp:	156452
Ion Ratio	Lower	Upper	
228	100		
226	29.4	23.9	35.9
229	22.0	15.1	22.7

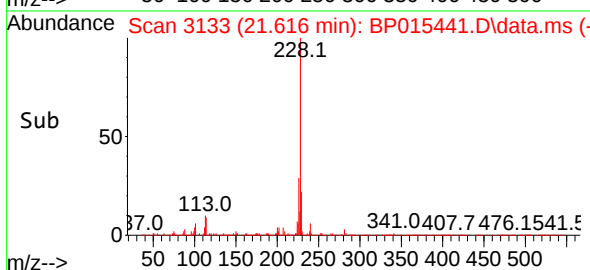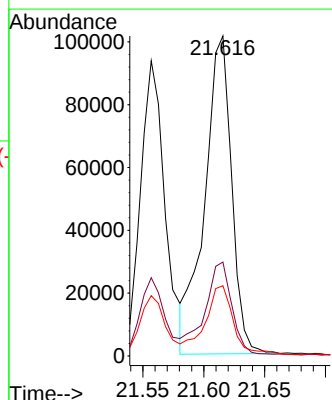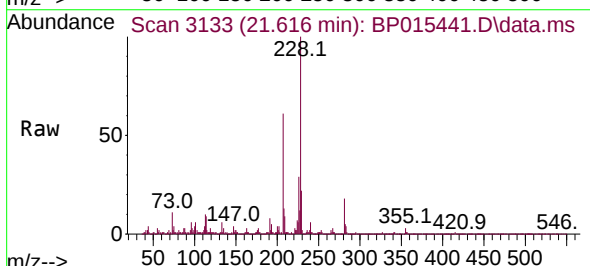

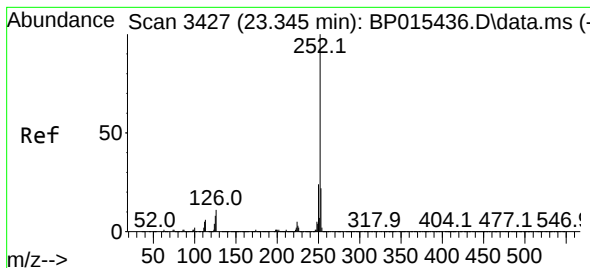

#90

Benzo(b)fluoranthene

Concen: 2.348 ng/ul

RT: 23.339 min Scan# 3427

Delta R.T. -0.012 min

Lab File: BP015441.D

Acq: 08 Jun 2023 18:52

Instrument :

BNA_P

ClientSampleId :





H0FN7

Tgt Ion:252	Resp: 207478
Ion Ratio	Lower Upper
252 100	
253 23.6	17.4 26.2
125 12.7	7.3 10.9

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/09/2023
Supervised By :Sohil Jodhani 06/09/2023

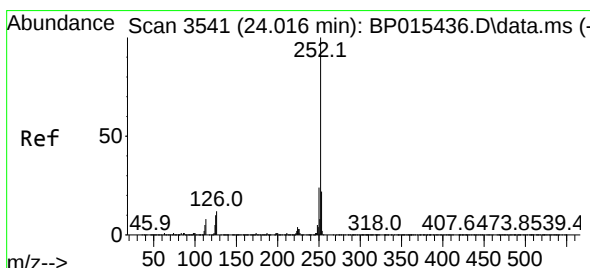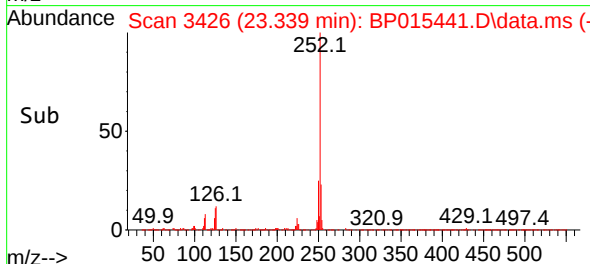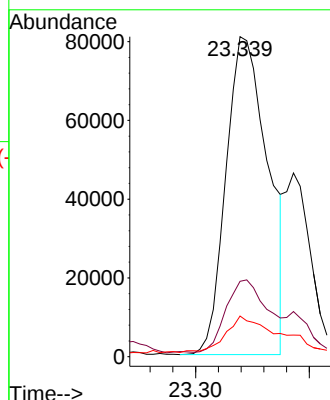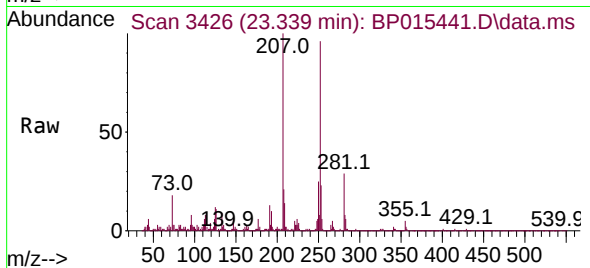

#93

Benzo(a)pyrene

Concen: 1.652 ng/ul




RT: 24.010 min Scan# 3540


Delta R.T. -0.018 min

Lab File: BP015441.D

Acq: 08 Jun 2023 18:52


Tgt Ion:252	Resp: 127262
Ion Ratio	Lower Upper
252 100	
253 21.2	17.8 26.6
125 10.7	8.1 12.1

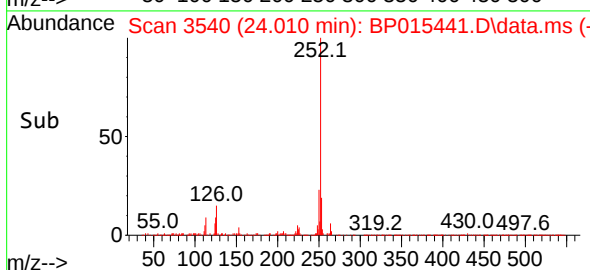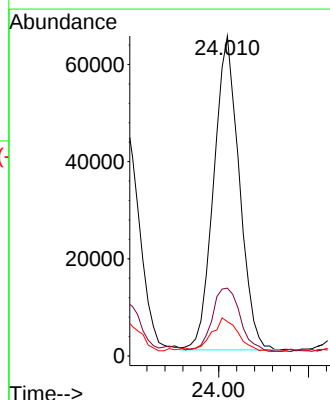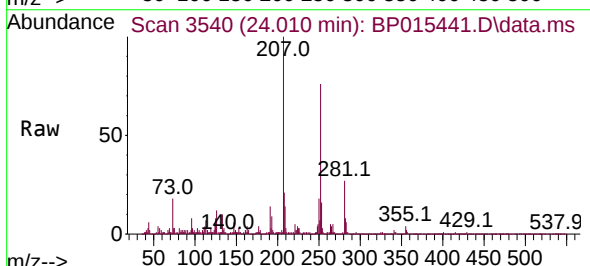

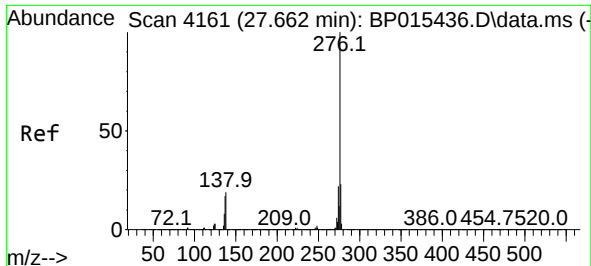

#96
 Benzo(g,h,i)perylene
 Concen: 1.108 ng/ul
 RT: 27.657 min Scan# 4160
 Delta R.T. -0.029 min
 Lab File: BP015441.D
 Acq: 08 Jun 2023 18:52

Instrument :
 BNA_P
 ClientSampleId :
 H0FN7

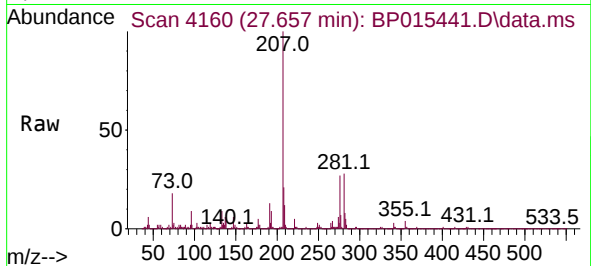

Tgt Ion:	276	Resp:	9101
Ion Ratio	Lower	Upper	
276	100		
138	16.1	15.6	23.4
277	25.0	19.0	28.6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/09/2023
 Supervised By :Sohil Jodhani 06/09/2023

