

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
 Data File : BP015427.D
 Acq On : 08 Jun 2023 09:53
 Operator : MA/JU
 Sample : PB153179BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK179

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	4	7	14	rVB2	16856	27434	0.58%	0.059%
2	3.411	34	38	46	rVB	38372	59278	1.25%	0.128%
3	3.846	110	112	132	rBV	400935	728512	15.36%	1.571%
4	4.187	166	170	174	rVB2	8410	12089	0.25%	0.026%
5	7.252	684	691	709	rVB	558773	957748	20.20%	2.065%
6	7.422	713	720	731	rVB	461629	760523	16.04%	1.640%
7	7.622	746	754	765	rBV	594723	984176	20.76%	2.122%
8	8.099	828	835	846	rBV	524314	845023	17.82%	1.822%
9	8.810	949	956	975	rBV	755198	1311575	27.66%	2.828%
10	9.275	1029	1035	1049	rBV	630759	1051238	22.17%	2.267%
11	10.005	1151	1159	1176	rBV	554205	950574	20.05%	2.050%
12	10.546	1242	1251	1270	rBV	701885	1340519	28.27%	2.890%
13	10.928	1309	1316	1326	rBV	808899	1318098	27.80%	2.842%
14	11.069	1333	1340	1357	rBV	720407	1396767	29.46%	3.012%
15	12.522	1581	1587	1598	rBV5	10919	27467	0.58%	0.059%
16	13.628	1768	1775	1787	rBV2	17044	33330	0.70%	0.072%
17	13.722	1787	1791	1798	rVB9	3217	6192	0.13%	0.013%
18	14.151	1854	1864	1878	rBV	1684776	2417671	50.99%	5.213%
19	14.440	1906	1913	1926	rBV2	1771372	2660297	56.10%	5.736%
20	14.745	1958	1965	1976	rBV	1379997	1985594	41.88%	4.281%
21	14.945	1992	1999	2025	rBV	430920	1073502	22.64%	2.315%
22	15.740	2127	2134	2149	rVV	2325723	3336407	70.36%	7.194%
23	15.863	2149	2155	2167	rBV	725107	1121443	23.65%	2.418%
24	15.981	2172	2175	2183	rVB2	16453	26570	0.56%	0.057%
25	16.522	2264	2267	2273	rVB8	4260	6791	0.14%	0.015%
26	17.175	2374	2378	2384	rBV9	4554	8948	0.19%	0.019%
27	17.292	2393	2398	2402	rBV5	4363	7805	0.16%	0.017%
28	17.504	2427	2434	2444	rBV	1791875	2598620	54.80%	5.603%
29	17.604	2444	2451	2467	rVV	2666257	3890278	82.04%	8.388%
30	19.404	2752	2757	2761	rBV2	40513	53201	1.12%	0.115%
31	19.469	2765	2768	2775	rVV2	32238	50144	1.06%	0.108%
32	19.828	2822	2829	2839	rBV	3480650	4741647	100.00%	10.223%
33	21.580	3122	3127	3135	rBV2	2060638	2983635	62.92%	6.433%
34	23.974	3526	3534	3548	rVB2	2205721	4728229	99.72%	10.195%
35	24.139	3555	3562	3572	rVB	1363573	2878614	60.71%	6.207%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
Data File : BP015427.D
Acq On : 08 Jun 2023 09:53
Operator : MA/JU
Sample : PB153179BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK179

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 46379939

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
Data File : BP015427.D
Acq On : 08 Jun 2023 09:53
Operator : MA/JU
Sample : PB153179BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK179

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

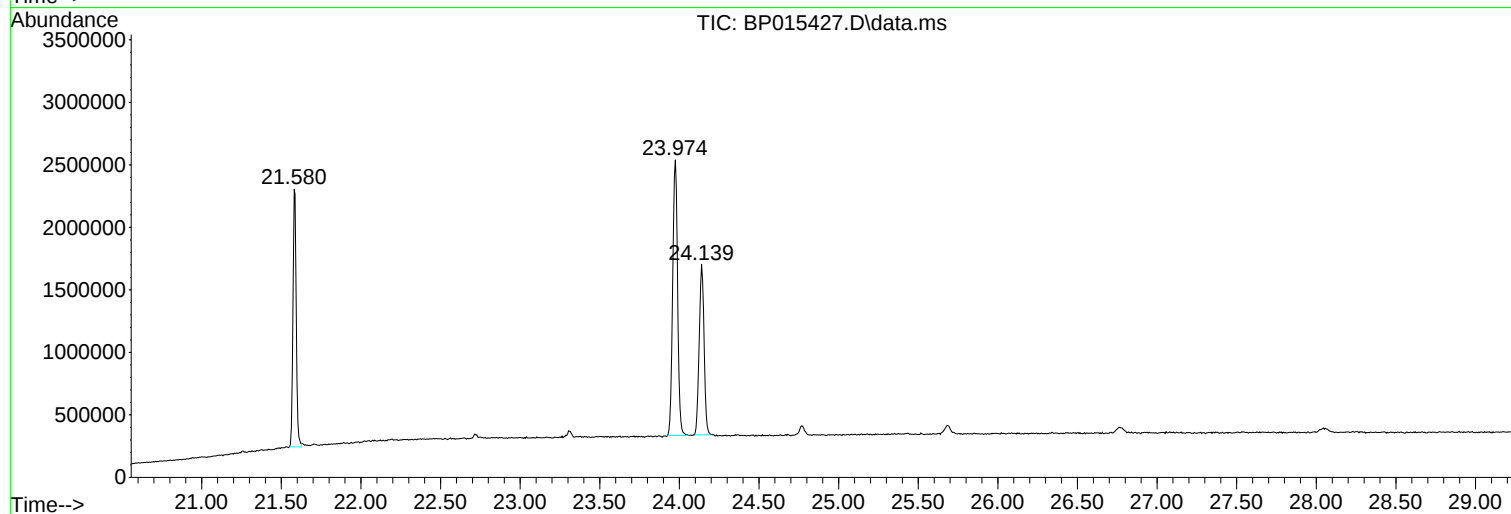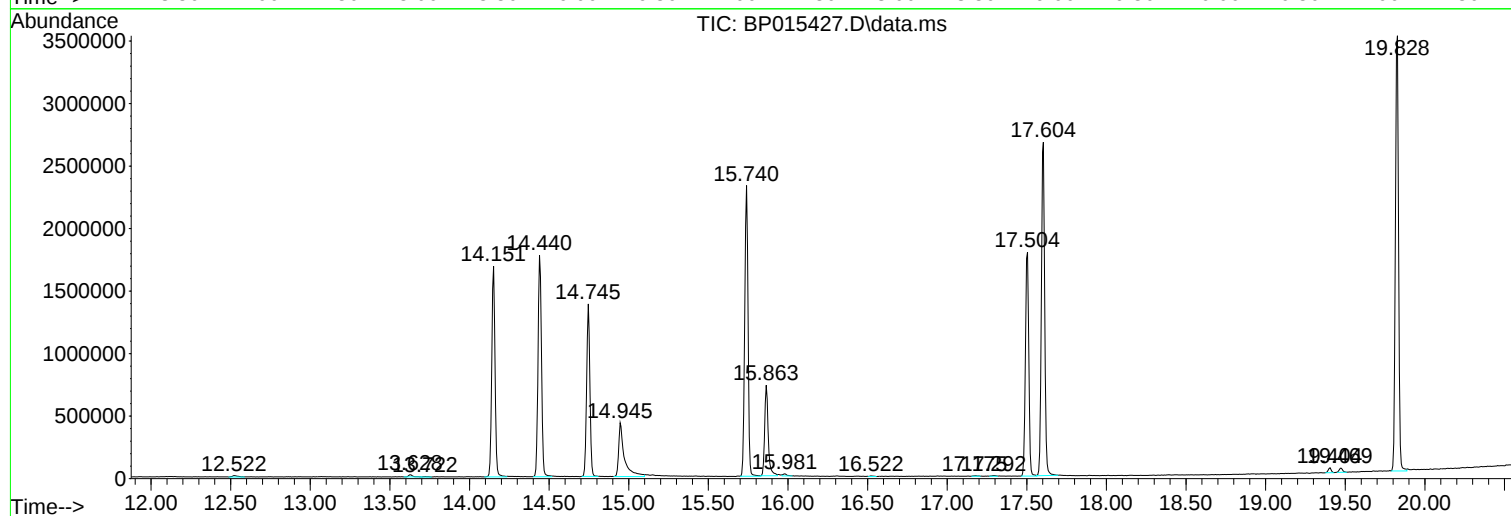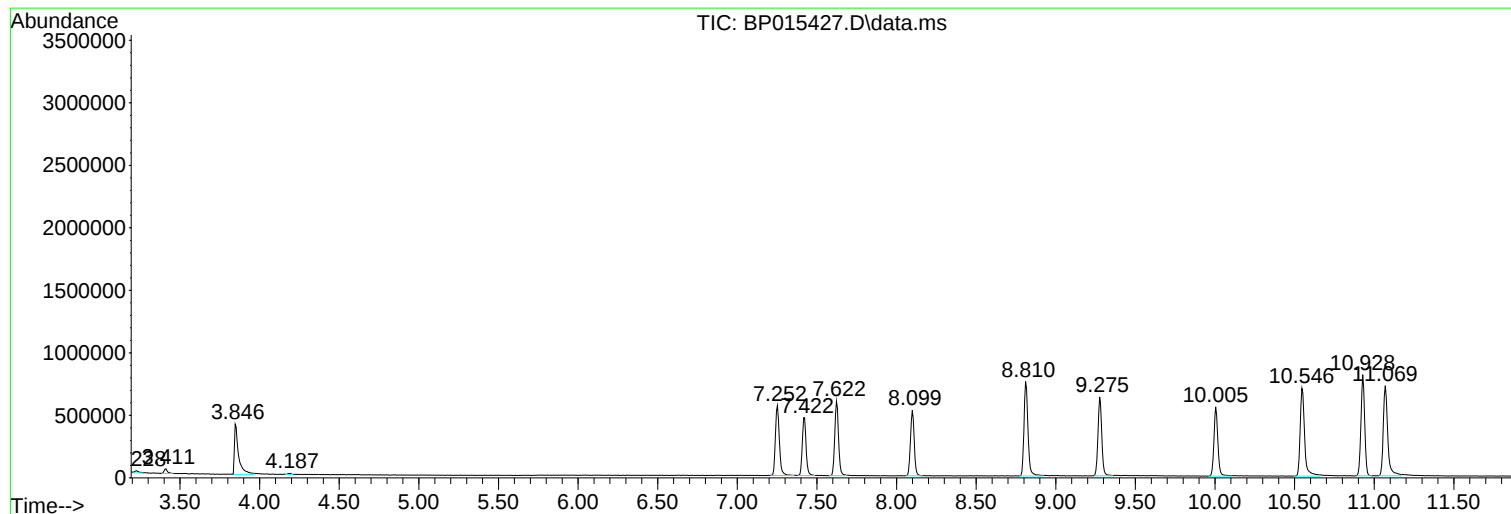

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
Data File : BP015427.D
Acq On : 08 Jun 2023 09:53
Operator : MA/JU
Sample : PB153179BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK179

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
Data File : BP015427.D
Acq On : 08 Jun 2023 09:53
Operator : MA/JU
Sample : PB153179BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK179

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------