

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
 Data File : BP015428.D
 Acq On : 08 Jun 2023 10:26
 Operator : MA/JU
 Sample : PB153136BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK136

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015428.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	4	6	14	rVB3	11016	18922	0.36%	0.042%
2	3.411	34	38	43	rBV	32884	45604	0.87%	0.101%
3	3.846	109	112	135	rBV	377945	709867	13.57%	1.569%
4	4.187	166	170	173	rBV3	5010	7338	0.14%	0.016%
5	7.252	684	691	712	rVB	530427	928572	17.76%	2.052%
6	7.416	712	719	732	rBV	462472	734520	14.05%	1.623%
7	7.622	746	754	766	rBV	578616	950482	18.17%	2.100%
8	8.099	828	835	844	rBV	423096	703421	13.45%	1.554%
9	8.811	948	956	969	rBV	730615	1250957	23.92%	2.764%
10	9.275	1026	1035	1050	rBV	598360	1024699	19.59%	2.264%
11	10.005	1150	1159	1171	rBV	524671	923359	17.66%	2.040%
12	10.546	1243	1251	1273	rBV	666084	1301163	24.88%	2.875%
13	10.922	1306	1315	1324	rBV	672272	1113384	21.29%	2.460%
14	11.063	1331	1339	1362	rBV	684202	1383792	26.46%	3.058%
15	12.516	1579	1586	1597	rBV4	9225	25185	0.48%	0.056%
16	13.622	1768	1774	1781	rVB2	12308	20726	0.40%	0.046%
17	14.146	1856	1863	1878	rBV	1666312	2366305	45.25%	5.229%
18	14.434	1905	1912	1924	rBV	1803868	2600879	49.73%	5.747%
19	14.740	1956	1964	1974	rBV	1158840	1685361	32.23%	3.724%
20	14.940	1991	1998	2026	rBV	450129	1112940	21.28%	2.459%
21	15.734	2126	2133	2146	rBV	2254901	3294473	63.00%	7.280%
22	15.857	2148	2154	2170	rVV	750700	1178462	22.53%	2.604%
23	15.975	2170	2174	2179	rVB4	14062	26871	0.51%	0.059%
24	17.275	2392	2395	2401	rBV5	4261	8034	0.15%	0.018%
25	17.498	2425	2433	2443	rBV	1563310	2259251	43.20%	4.992%
26	17.598	2443	2450	2465	rVV	2634822	3918628	74.93%	8.659%
27	19.398	2752	2756	2761	rBV2	39237	51180	0.98%	0.113%
28	19.469	2764	2768	2775	rVB	33785	48793	0.93%	0.108%
29	19.822	2821	2828	2836	rBV	3464815	4832950	92.41%	10.680%
30	21.580	3121	3127	3136	rBV	1902578	2708034	51.78%	5.984%
31	23.969	3525	3533	3549	rVB2	2519238	5229691	100.00%	11.556%
32	24.133	3554	3561	3574	rVB	1268255	2789779	53.35%	6.165%


Sum of corrected areas: 45253622

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
Data File : BP015428.D
Acq On : 08 Jun 2023 10:26
Operator : MA/JU
Sample : PB153136BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

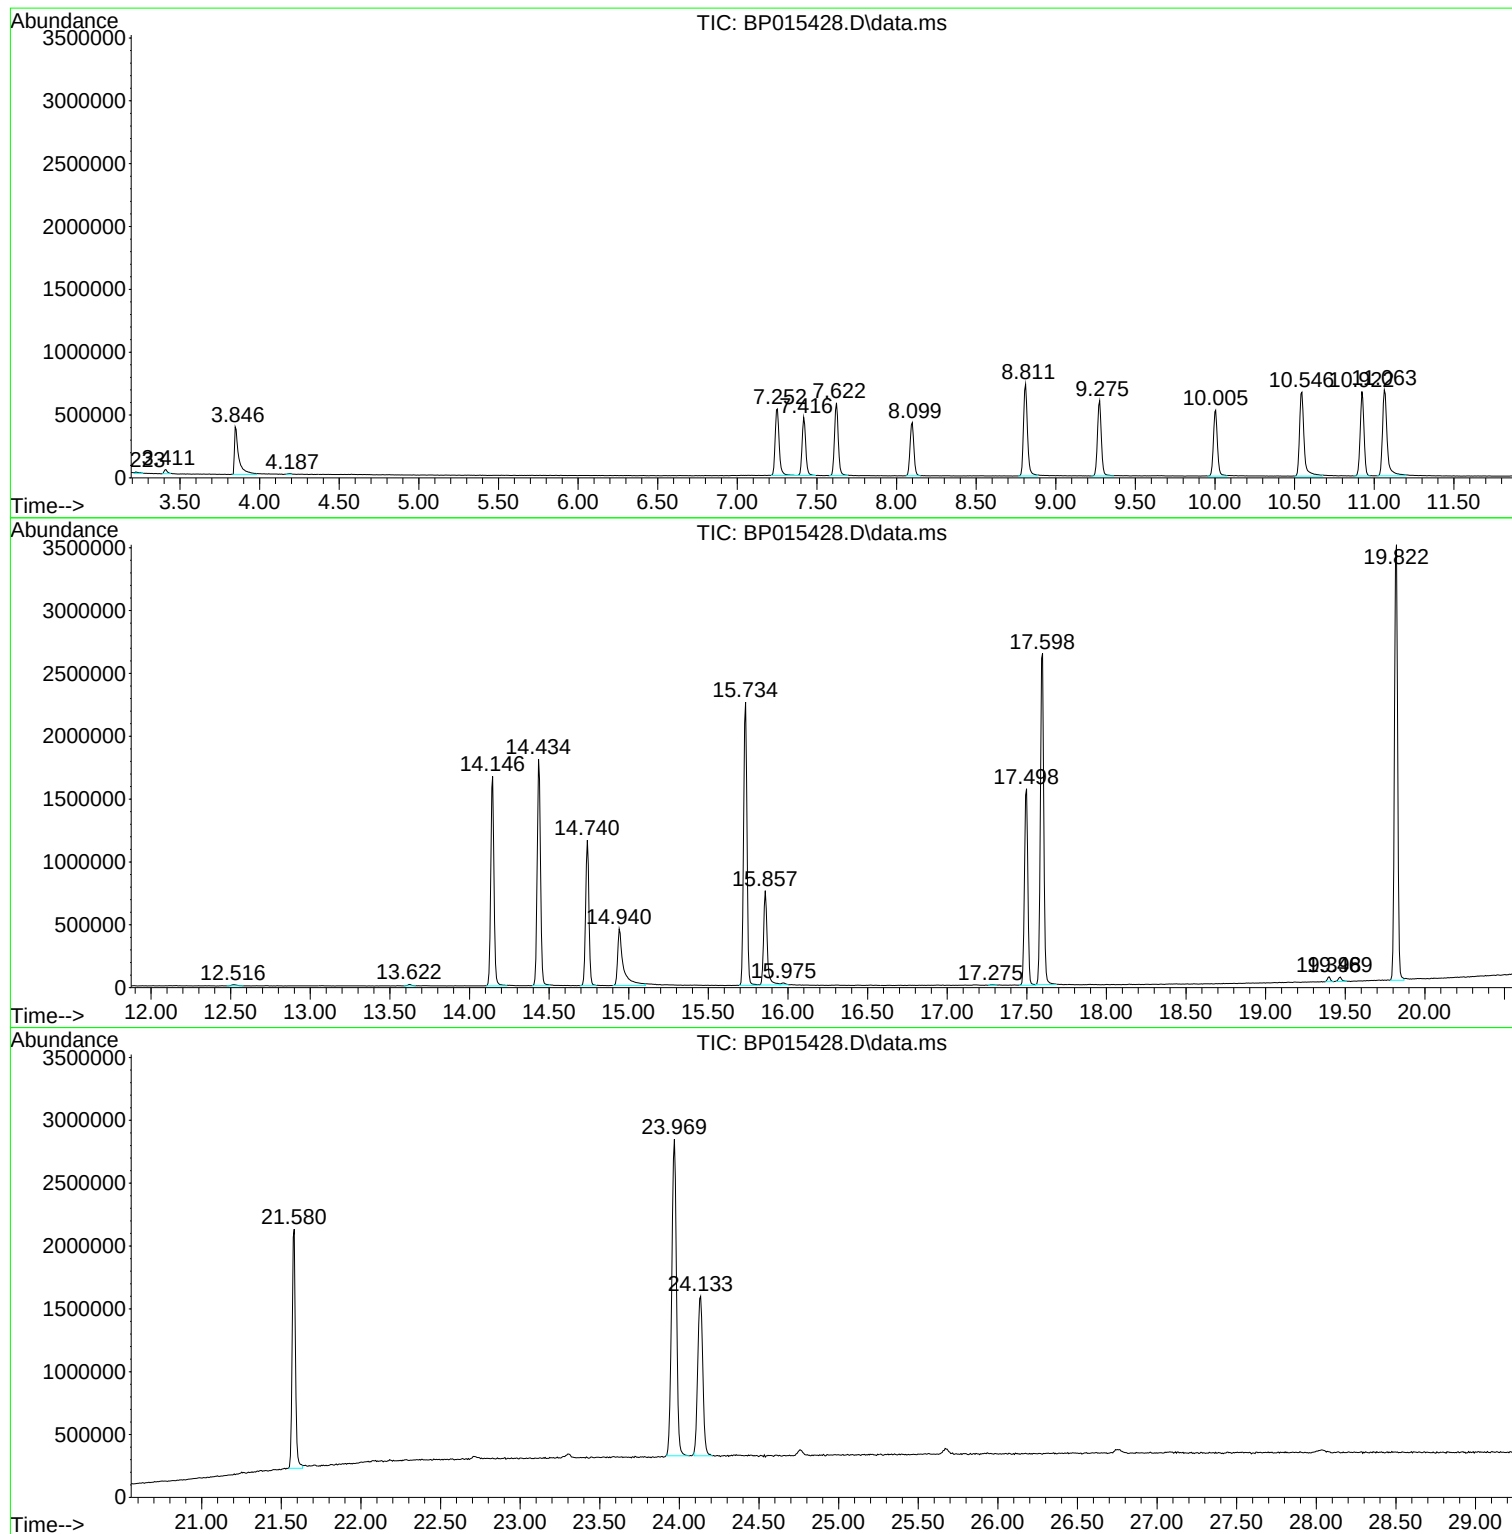

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
Data File : BP015428.D
Acq On : 08 Jun 2023 10:26
Operator : MA/JU
Sample : PB153136BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060823\
Data File : BP015428.D
Acq On : 08 Jun 2023 10:26
Operator : MA/JU
Sample : PB153136BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------