




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
 Data File : BP015465.D
 Acq On : 09 Jun 2023 23:37
 Operator : MA/JU
 Sample : 03097-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEN2

Manual IntegrationsAPPROVED

Quant Time: Jun 10 00:23:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/12/2023
 Supervised By :mohammad ahmed 06/13/2023

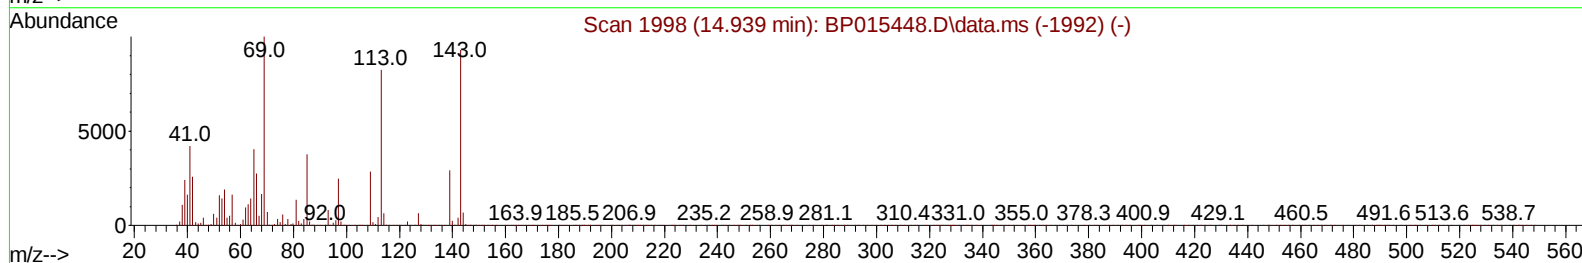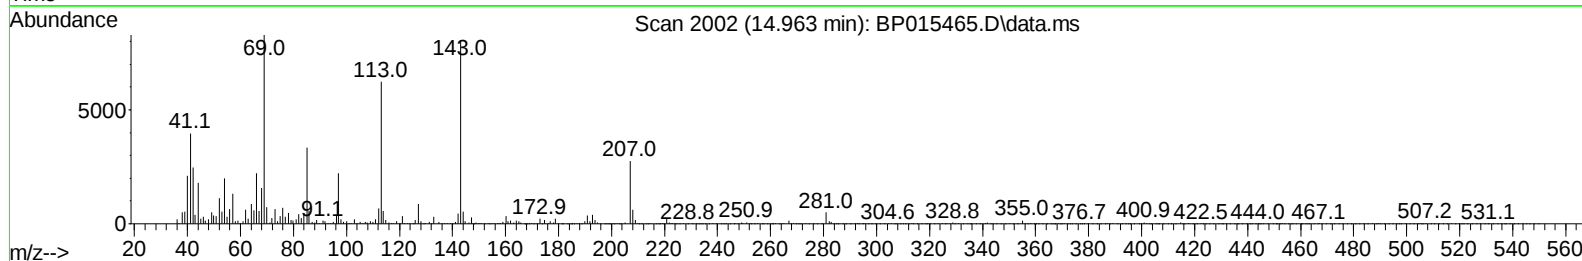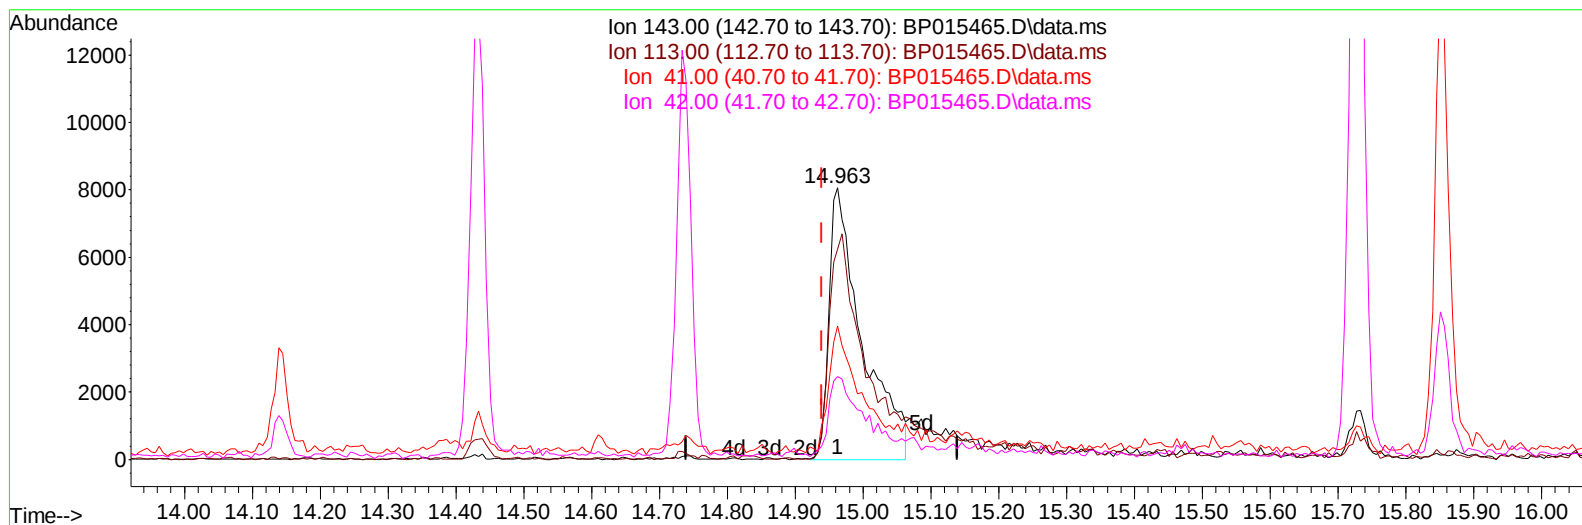

TIC: BP015465.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.963min (+ 0.023) 3.96 ng/ul m

response 27385

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	86.60	77.38
41.00	42.20	49.14
42.00	29.40	30.51

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
 Data File : BP015465.D
 Acq On : 09 Jun 2023 23:37
 Operator : MA/JU
 Sample : 03097-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEN2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/12/2023
 Supervised By :mohammad ahmed 06/13/2023

Quant Time: Jun 10 00:24:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 09 23:33:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.092	152	151980	20.000	ng/ul	0.00
20) Naphthalene-d8	10.922	136	690673	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.739	164	489103	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.492	188	1154468	20.000	ng/ul	0.00
79) Chrysene-d12	21.574	240	1151348	20.000	ng/ul	0.00
88) Perylene-d12	24.121	264	1179776	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	8212	2.001	ng/uL	0.00
4) Pyridine-d5	3.857	84	71011	6.661	ng/ul	0.01
7) Phenol-d5	7.251	99	83175	5.940	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.416	67	258803	30.950	ng/ul	0.00
11) 2-Chlorophenol-d4	7.622	132	243876	24.024	ng/ul	0.00
15) 4-Methylphenol-d8	8.810	113	174882	15.219	ng/ul	0.00
21) Nitrobenzene-d5	9.269	128	174608	32.201	ng/ul	0.00
24) 2-Nitrophenol-d4	9.998	143	192567	31.097	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.539	165	312705	27.683	ng/ul	0.00
31) 4-Chloroaniline-d4	11.063	131	353279	21.788	ng/ul	0.00
46) Dimethylphthalate-d6	14.139	166	1358346	35.219	ng/ul	0.00
49) Acenaphthylene-d8	14.433	160	1406774	33.357	ng/ul	0.00
54) 4-Nitrophenol-d4	14.963	143	27385m	3.965	ng/ul	0.02
60) Fluorene-d10	15.727	176	1134162	34.872	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	232260	31.757	ng/ul	0.00
73) Anthracene-d10	17.592	188	1960396	37.322	ng/ul	0.00
81) Pyrene-d10	19.815	212	2414347	39.180	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.956	264	2264589	38.256	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015465.D
Acq On : 09 Jun 2023 23:37
Operator : MA/JU
Sample : 03097-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEN2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/12/2023
Supervised By :mohammad ahmed 06/13/2023

Quant Time: Jun 10 00:24:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 09 23:33:38 2023
Response via : Initial Calibration

