

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
 Data File : BP015449.D
 Acq On : 09 Jun 2023 12:47
 Operator : MA/JU
 Sample : PB153136BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK136

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	33	37	50	rVB	60443	87244	1.15%	0.119%
2	3.846	109	112	138	rBV	724987	1226993	16.18%	1.673%
3	4.187	166	170	174	rBV	9482	13435	0.18%	0.018%
4	7.252	683	691	708	rBV	949263	1626546	21.45%	2.218%
5	7.416	713	719	732	rVB	802689	1263099	16.66%	1.722%
6	7.622	746	754	766	rBV	1020507	1650485	21.77%	2.250%
7	8.099	827	835	845	rBV	770673	1283498	16.93%	1.750%
8	8.810	948	956	977	rBV	1294926	2185671	28.83%	2.980%
9	9.275	1027	1035	1048	rBV	1058678	1757132	23.18%	2.396%
10	10.004	1151	1159	1171	rBV	927175	1584189	20.89%	2.160%
11	10.546	1243	1251	1271	rBV	1238136	2266906	29.90%	3.091%
12	10.928	1307	1316	1331	rVB	1185401	1991868	26.27%	2.716%
13	11.069	1331	1340	1361	rBV	1223838	2370991	31.27%	3.233%
14	12.522	1580	1587	1596	rBV2	18582	42965	0.57%	0.059%
15	13.628	1768	1775	1781	rBV2	9462	16232	0.21%	0.022%
16	14.151	1853	1864	1878	rBV	2780549	3861913	50.94%	5.265%
17	14.439	1905	1913	1933	rBV	2924442	4327101	57.07%	5.900%
18	14.745	1958	1965	1975	rBV	1996907	2902268	38.28%	3.957%
19	14.945	1992	1999	2024	rBV	922488	1928611	25.44%	2.629%
20	15.739	2127	2134	2148	rBV	3692801	5355051	70.63%	7.301%
21	15.863	2148	2155	2169	rVV	1374510	2040801	26.92%	2.782%
22	15.981	2171	2175	2181	rVB3	20635	35152	0.46%	0.048%
23	16.310	2223	2231	2235	rBV3	4663	10111	0.13%	0.014%
24	16.522	2263	2267	2272	rBV8	4911	8840	0.12%	0.012%
25	16.933	2333	2337	2341	rBV7	5120	8045	0.11%	0.011%
26	17.175	2375	2378	2383	rVB7	6469	8434	0.11%	0.011%
27	17.298	2395	2399	2406	rVB3	6916	12428	0.16%	0.017%
28	17.504	2427	2434	2444	rBV	2674157	3763919	49.64%	5.132%
29	17.604	2444	2451	2464	rVV	4253579	6146496	81.07%	8.380%
30	18.145	2540	2543	2549	rBV8	5625	9464	0.12%	0.013%
31	18.375	2578	2582	2585	rBV6	5019	8118	0.11%	0.011%
32	19.404	2752	2757	2762	rBV	63486	87964	1.16%	0.120%
33	19.474	2765	2769	2778	rVB	56732	82903	1.09%	0.113%
34	19.827	2823	2829	2837	rBV	5630575	7392461	97.50%	10.079%
35	21.586	3122	3128	3139	rBV	3163193	4255445	56.13%	5.802%
36	23.980	3526	3535	3551	rVB2	3622650	7581943	100.00%	10.337%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015449.D
Acq On : 09 Jun 2023 12:47
Operator : MA/JU
Sample : PB153136BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK136

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Title : SVOA CALIBRATION

37	24.145	3555	3563	3573	rVB	1917139	4151742	54.76%	5.660%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 73346464

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015449.D
Acq On : 09 Jun 2023 12:47
Operator : MA/JU
Sample : PB153136BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

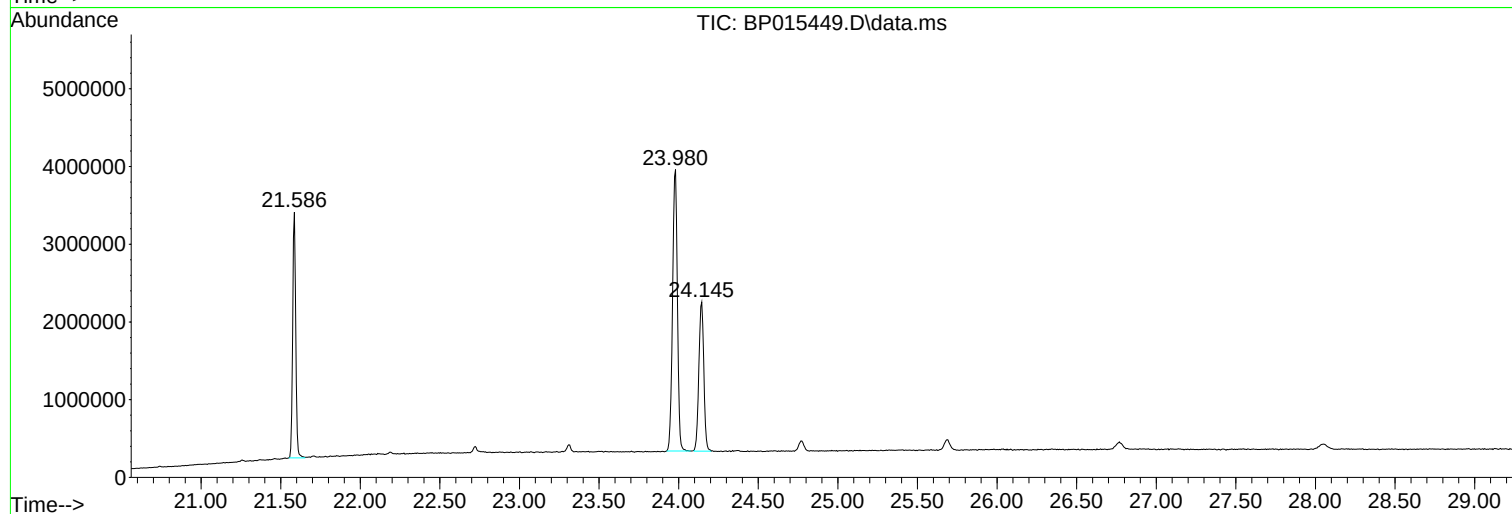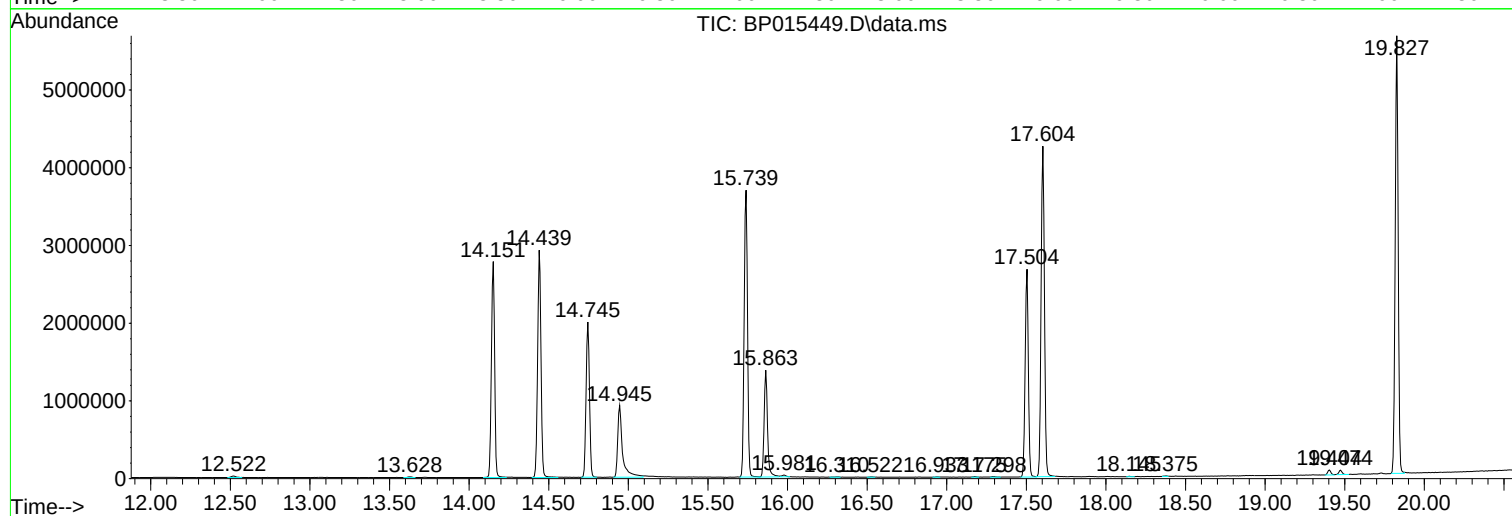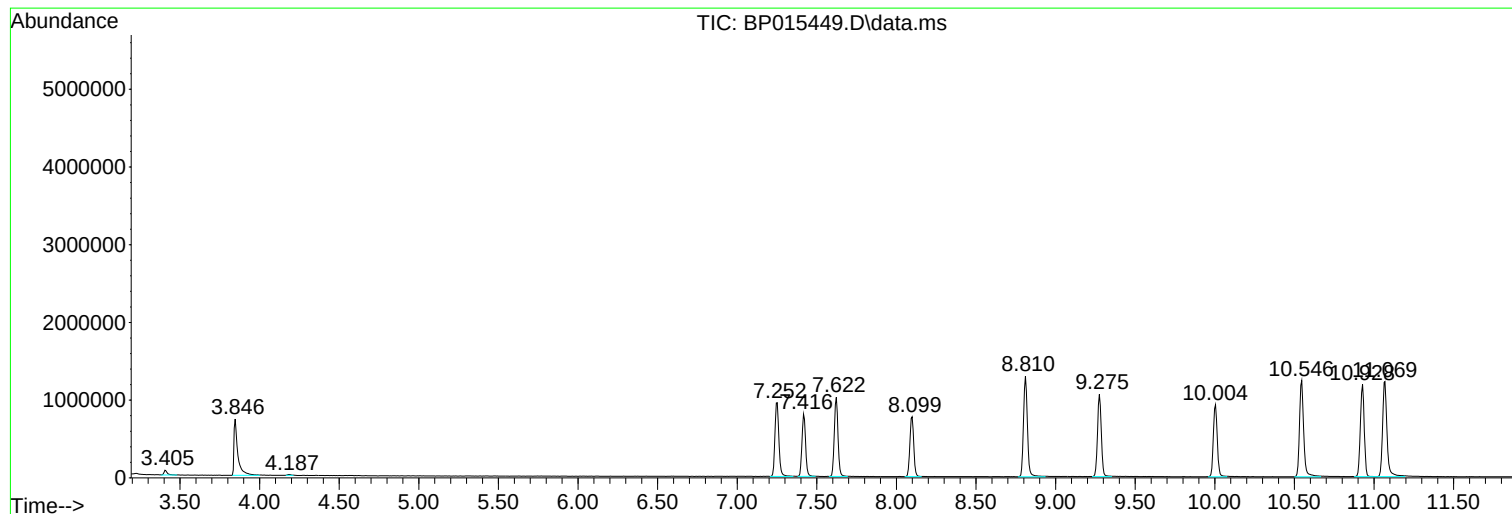

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015449.D
Acq On : 09 Jun 2023 12:47
Operator : MA/JU
Sample : PB153136BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015449.D
Acq On : 09 Jun 2023 12:47
Operator : MA/JU
Sample : PB153136BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK136

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------