

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
 Data File : BP015452.D
 Acq On : 09 Jun 2023 15:11
 Operator : MA/JU
 Sample : PB153326BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK326

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	4	6	17	rVB2	17713	31828	0.52%	0.052%
2	3.405	34	37	45	rBV	47271	71523	1.17%	0.118%
3	3.846	109	112	135	rBV	584088	1032925	16.93%	1.701%
4	7.246	684	690	707	rBV	756330	1284837	21.05%	2.116%
5	7.416	713	719	734	rVB	646201	1011849	16.58%	1.666%
6	7.622	746	754	771	rBV	800938	1322670	21.67%	2.178%
7	8.093	828	834	844	rBV	660449	1111539	18.21%	1.831%
8	8.810	948	956	972	rBV	1017400	1749018	28.66%	2.880%
9	9.275	1027	1035	1046	rBV	841135	1412744	23.15%	2.327%
10	9.434	1058	1062	1067	rVB7	6210	10558	0.17%	0.017%
11	9.998	1151	1158	1168	rBV	738150	1266658	20.76%	2.086%
12	10.540	1242	1250	1270	rBV	940955	1817345	29.78%	2.993%
13	10.922	1306	1315	1323	rBV	1072576	1754816	28.76%	2.890%
14	11.063	1332	1339	1362	rBV	983038	1913152	31.35%	3.151%
15	12.516	1578	1586	1595	rBV	13510	32662	0.54%	0.054%
16	13.622	1766	1774	1782	rBV3	23381	41342	0.68%	0.068%
17	14.145	1853	1863	1876	rBV	2226279	3121601	51.15%	5.141%
18	14.434	1905	1912	1928	rBV	2347743	3512484	57.56%	5.785%
19	14.739	1956	1964	1978	rBV	1801104	2617080	42.89%	4.310%
20	14.939	1991	1998	2031	rBV	658701	1531198	25.09%	2.522%
21	15.733	2126	2133	2147	rVV	3046786	4354668	71.36%	7.172%
22	15.857	2147	2154	2171	rVV	1055874	1612845	26.43%	2.656%
23	15.969	2171	2173	2179	rVB3	17949	25863	0.42%	0.043%
24	16.522	2263	2267	2271	rVB7	4796	6224	0.10%	0.010%
25	17.175	2373	2378	2384	rVB10	4181	8949	0.15%	0.015%
26	17.280	2394	2396	2404	rVB6	4620	8656	0.14%	0.014%
27	17.498	2426	2433	2443	rBV	2326002	3375097	55.31%	5.558%
28	17.598	2443	2450	2464	rVV	3487899	4973689	81.50%	8.191%
29	18.363	2578	2580	2589	rBV9	6923	16987	0.28%	0.028%
30	19.398	2752	2756	2760	rBV2	49383	64645	1.06%	0.106%
31	19.469	2764	2768	2775	rVB	44799	61520	1.01%	0.101%
32	19.821	2821	2828	2837	rBV	4468883	6102404	100.00%	10.050%
33	21.580	3121	3127	3138	rBV	2740572	3836012	62.86%	6.317%
34	23.968	3525	3533	3544	rVB2	2797562	5961526	97.69%	9.818%
35	24.133	3553	3561	3573	rVB	1729896	3664426	60.05%	6.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015452.D
Acq On : 09 Jun 2023 15:11
Operator : MA/JU
Sample : PB153326BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK326

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 60721340

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015452.D
Acq On : 09 Jun 2023 15:11
Operator : MA/JU
Sample : PB153326BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK326

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

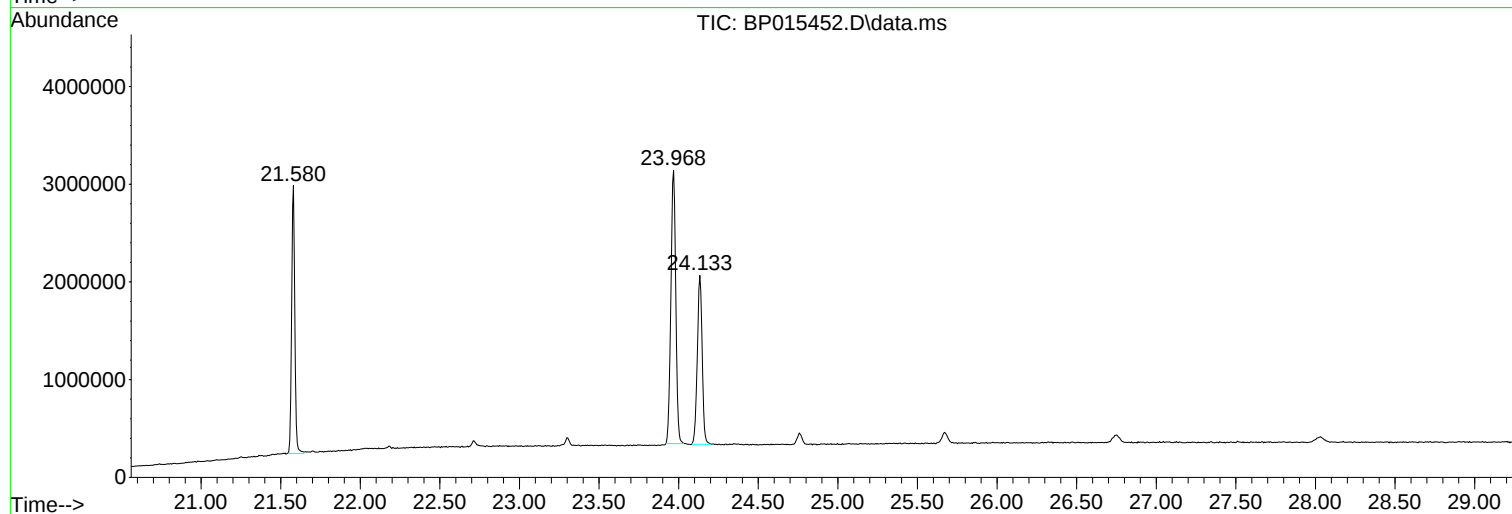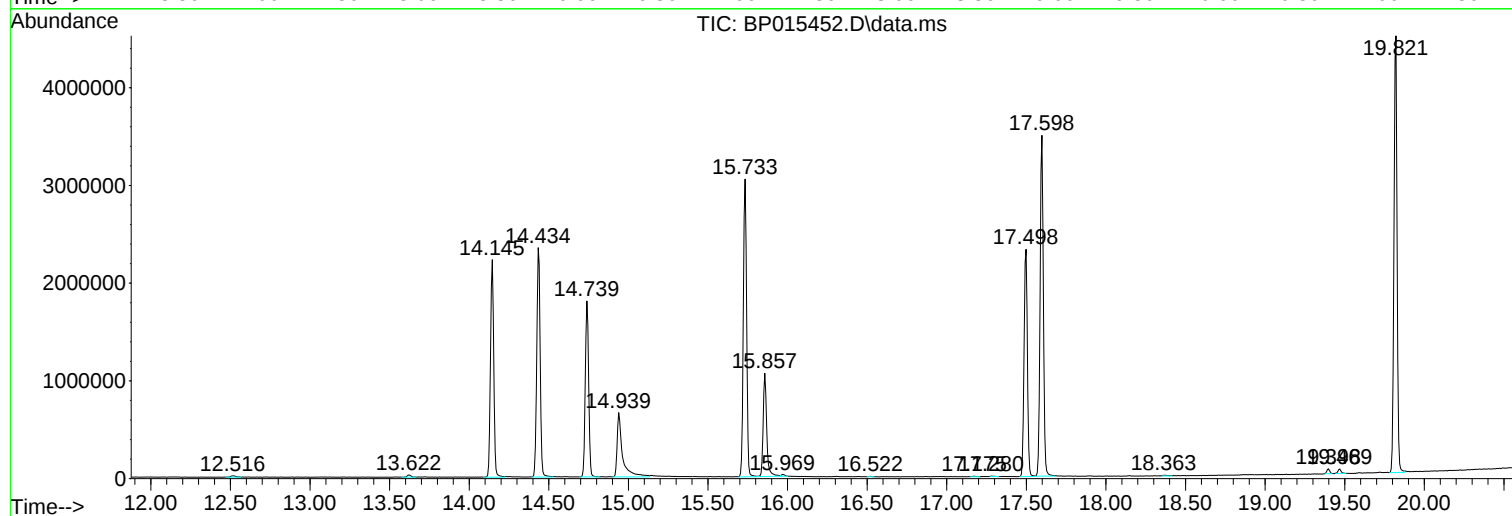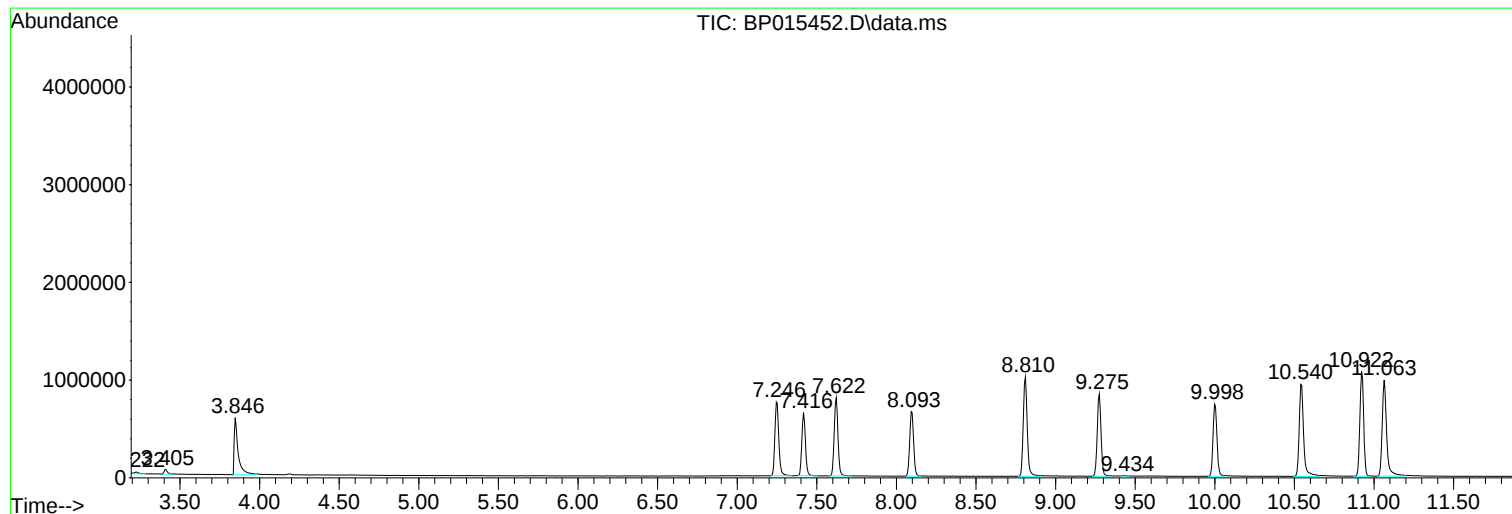

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015452.D
Acq On : 09 Jun 2023 15:11
Operator : MA/JU
Sample : PB153326BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK326

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015452.D
Acq On : 09 Jun 2023 15:11
Operator : MA/JU
Sample : PB153326BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK326

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------