

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
 Data File : BP015453.D
 Acq On : 09 Jun 2023 15:45
 Operator : MA/JU
 Sample : 03097-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.411	34	38	43	rBV2	12295	19311	0.35%	0.046%
2	3.858	111	114	132	rBV	119768	232802	4.24%	0.555%
3	4.081	149	152	158	rVB4	8411	12955	0.24%	0.031%
4	4.187	166	170	175	rBV3	6454	11023	0.20%	0.026%
5	7.252	684	691	702	rBV2	118992	217182	3.96%	0.518%
6	7.416	713	719	731	rBV	462726	744668	13.57%	1.775%
7	7.622	747	754	766	rBV	453578	762307	13.89%	1.817%
8	8.093	828	834	845	rBV	349190	587958	10.71%	1.401%
9	8.811	949	956	973	rBV	384495	689999	12.57%	1.645%
10	8.934	973	977	983	rVB5	7850	13799	0.25%	0.033%
11	9.269	1027	1034	1048	rBV	603338	1069893	19.49%	2.550%
12	9.658	1095	1100	1105	rVB7	4727	7878	0.14%	0.019%
13	9.999	1151	1158	1175	rBV	467177	833834	15.19%	1.987%
14	10.540	1243	1250	1275	rBV	629496	1240042	22.59%	2.956%
15	10.922	1308	1315	1329	rVB	551806	940469	17.13%	2.242%
16	11.063	1332	1339	1369	rBV	607585	1242056	22.63%	2.960%
17	12.228	1532	1537	1547	rVB	4115	10303	0.19%	0.025%
18	12.516	1582	1586	1595	rVB3	10786	20807	0.38%	0.050%
19	13.034	1669	1674	1679	rBV7	10389	16202	0.30%	0.039%
20	13.093	1679	1684	1691	rVB8	2859	6839	0.12%	0.016%
21	13.269	1710	1714	1722	rVB	8667	12782	0.23%	0.030%
22	13.622	1766	1774	1784	rBV3	20710	47331	0.86%	0.113%
23	14.140	1855	1862	1879	rBV	1663881	2515245	45.82%	5.995%
24	14.434	1906	1912	1930	rBV	1890032	2780585	50.65%	6.627%
25	14.740	1957	1964	1974	rBV	930752	1401859	25.54%	3.341%
26	14.969	1996	2003	2018	rBV5	33886	142269	2.59%	0.339%
27	15.475	2084	2089	2094	rBV3	7057	12865	0.23%	0.031%
28	15.551	2099	2102	2106	rVB3	9397	13534	0.25%	0.032%
29	15.734	2126	2133	2146	rBV	2459243	3633974	66.20%	8.661%
30	15.857	2148	2154	2168	rVV	534469	911296	16.60%	2.172%
31	15.969	2170	2173	2180	rVB6	17092	32785	0.60%	0.078%
32	16.428	2248	2251	2255	rBV6	6874	8887	0.16%	0.021%
33	16.510	2261	2265	2273	rBV6	4251	9552	0.17%	0.023%
34	17.075	2358	2361	2366	rBV6	4566	6133	0.11%	0.015%
35	17.169	2372	2377	2380	rBV6	5267	8931	0.16%	0.021%
36	17.228	2383	2387	2391	rBV3	9474	11630	0.21%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
 Data File : BP015453.D
 Acq On : 09 Jun 2023 15:45
 Operator : MA/JU
 Sample : 03097-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

37	17.287	2391	2397	2399	rBV7	5356	8960	0.16%	0.021%
38	17.387	2410	2414	2416	rBV5	3570	5687	0.10%	0.014%
39	17.434	2418	2422	2425	rVV6	5636	6717	0.12%	0.016%
40	17.492	2426	2432	2443	rVV	1312570	1825062	33.25%	4.350%
41	17.592	2443	2449	2466	rVV	2899810	4482828	81.66%	10.685%
42	17.763	2475	2478	2482	rVB	10058	12194	0.22%	0.029%
43	17.963	2509	2512	2517	rBV3	11553	13755	0.25%	0.033%
44	18.134	2538	2541	2546	rBV4	15299	20474	0.37%	0.049%
45	18.322	2569	2573	2575	rBV5	14698	19665	0.36%	0.047%
46	18.357	2575	2579	2581	rVV2	48021	71214	1.30%	0.170%
47	18.381	2581	2583	2587	rVV	42662	52297	0.95%	0.125%
48	18.428	2587	2591	2596	rVB	31574	42295	0.77%	0.101%
49	18.628	2623	2625	2630	rVB6	5572	5855	0.11%	0.014%
50	18.810	2653	2656	2659	rBV3	7146	9660	0.18%	0.023%
51	18.851	2661	2663	2667	rVV4	10237	13612	0.25%	0.032%
52	19.392	2751	2755	2761	rBV	46670	66403	1.21%	0.158%
53	19.463	2763	2767	2773	rVB	41989	62271	1.13%	0.148%
54	19.581	2783	2787	2794	rBV3	35840	60367	1.10%	0.144%
55	19.816	2821	2827	2837	rBV	4114105	5489378	100.00%	13.084%
56	21.575	3121	3126	3137	rBV	1422377	2117304	38.57%	5.046%
57	23.963	3524	3532	3547	rVB2	2556691	5347663	97.42%	12.746%
58	24.127	3553	3560	3571	rVB	891147	1992327	36.29%	4.749%




Sum of corrected areas: 41955973

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015453.D
Acq On : 09 Jun 2023 15:45
Operator : MA/JU
Sample : 03097-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

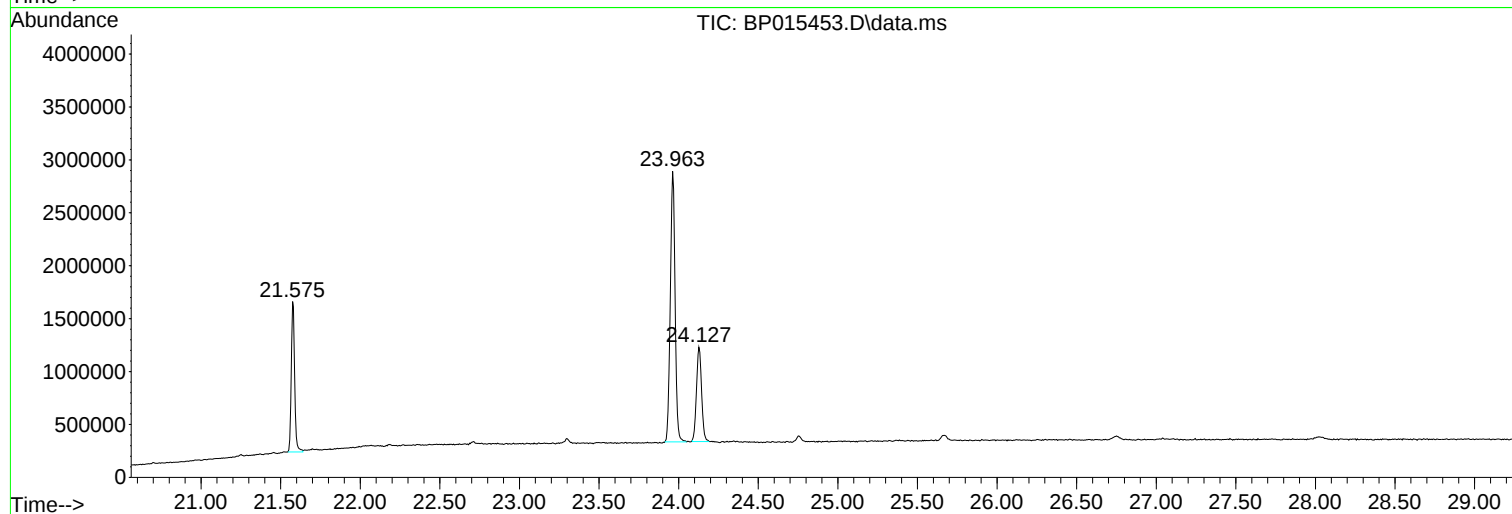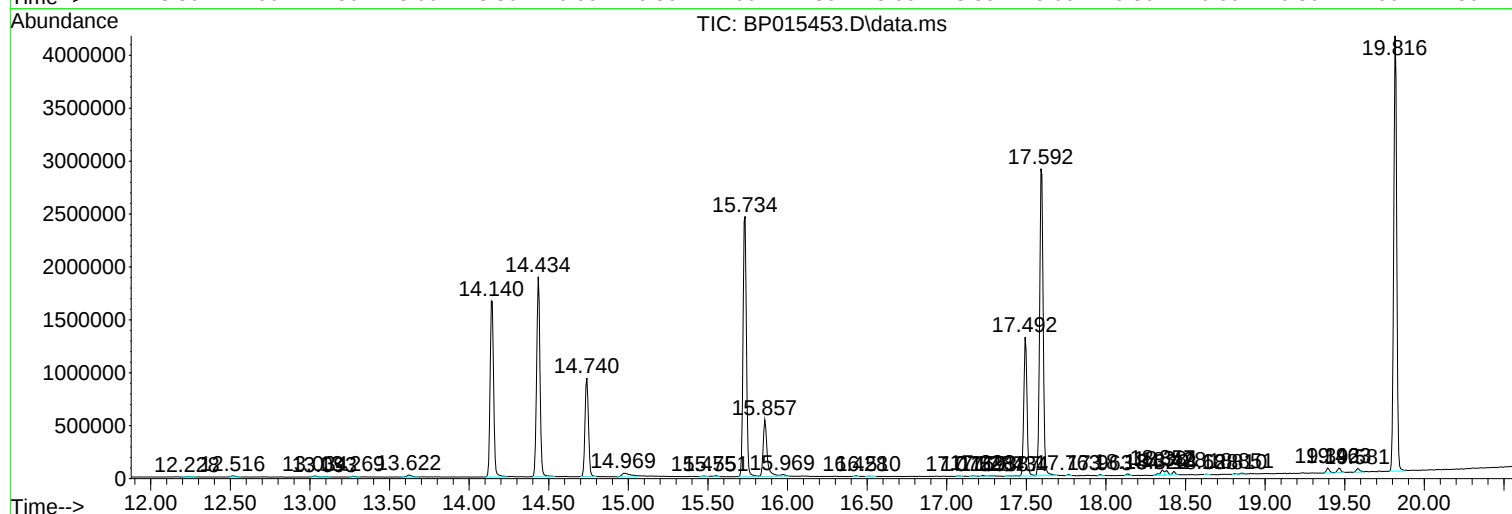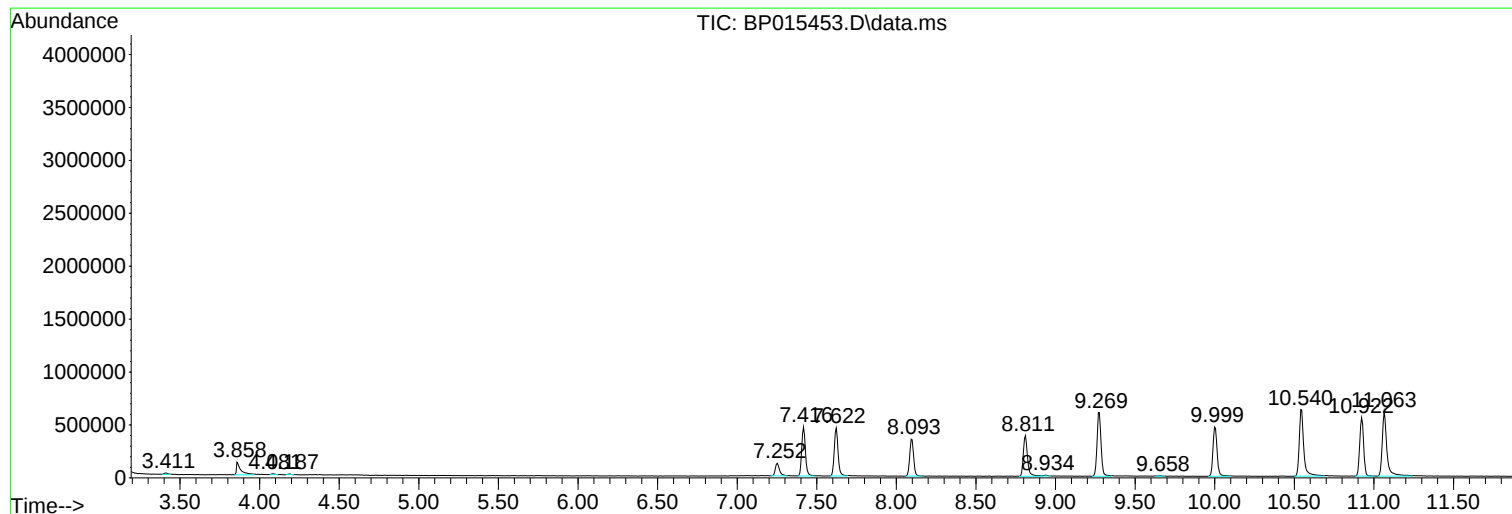

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015453.D
Acq On : 09 Jun 2023 15:45
Operator : MA/JU
Sample : 03097-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015453.D
Acq On : 09 Jun 2023 15:45
Operator : MA/JU
Sample : 03097-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc