

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
 Data File : BP015456.D
 Acq On : 09 Jun 2023 17:26
 Operator : MA/JU
 Sample : 03097-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015456.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	28	32	37	rBV	108535	165512	3.00%	0.347%
2	3.858	111	114	132	rBV	180120	331656	6.01%	0.695%
3	4.081	149	152	159	rVB2	10484	18294	0.33%	0.038%
4	4.187	167	170	173	rVB	6745	7205	0.13%	0.015%
5	7.252	684	691	702	rBV	131872	240262	4.35%	0.503%
6	7.416	712	719	732	rBV	550010	875961	15.86%	1.835%
7	7.622	747	754	766	rBV	529196	890547	16.13%	1.866%
8	8.093	824	834	844	rBV	478857	794012	14.38%	1.663%
9	8.810	948	956	970	rBV	449928	798093	14.45%	1.672%
10	9.275	1027	1035	1045	rBV	732723	1234499	22.35%	2.586%
11	9.657	1095	1100	1107	rVB5	6701	14510	0.26%	0.030%
12	9.999	1151	1158	1174	rBV	599620	1047831	18.97%	2.195%
13	10.540	1243	1250	1272	rBV	798490	1528656	27.68%	3.202%
14	10.922	1308	1315	1329	rVB	736620	1242279	22.50%	2.602%
15	11.063	1330	1339	1354	rBV	732953	1401607	25.38%	2.936%
16	12.516	1581	1586	1594	rBV4	12577	27426	0.50%	0.057%
17	13.545	1756	1761	1766	rBV4	7337	11924	0.22%	0.025%
18	13.622	1766	1774	1779	rVV7	6692	11511	0.21%	0.024%
19	14.145	1855	1863	1878	rBV	1925901	2783850	50.41%	5.832%
20	14.257	1878	1882	1887	rVB8	5939	11207	0.20%	0.023%
21	14.434	1905	1912	1929	rBV	2144349	3159210	57.21%	6.618%
22	14.739	1956	1964	1972	rBV	1211759	1783514	32.30%	3.736%
23	14.963	1996	2002	2016	rBV6	54072	177791	3.22%	0.372%
24	15.145	2029	2033	2037	rVB7	6974	9818	0.18%	0.021%
25	15.734	2126	2133	2147	rBV	2784351	3977092	72.02%	8.332%
26	15.857	2148	2154	2169	rVV	689025	1102015	19.96%	2.309%
27	15.969	2170	2173	2182	rVB4	15807	27120	0.49%	0.057%
28	16.098	2189	2195	2202	rBV	112909	172429	3.12%	0.361%
29	16.516	2264	2266	2272	rVB7	4625	6135	0.11%	0.013%
30	17.169	2373	2377	2383	rBV9	5083	7093	0.13%	0.015%
31	17.381	2408	2413	2417	rBV7	6235	13947	0.25%	0.029%
32	17.492	2424	2432	2442	rBV	1569982	2317368	41.96%	4.855%
33	17.592	2443	2449	2464	rVV2	3018664	4475612	81.04%	9.376%
34	17.769	2476	2479	2484	rVB4	6202	9896	0.18%	0.021%
35	18.139	2539	2542	2547	rVB5	10103	12522	0.23%	0.026%
36	18.351	2573	2578	2586	rBV	144437	209942	3.80%	0.440%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015456.D
Acq On : 09 Jun 2023 17:26
Operator : MA/JU
Sample : 03097-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEN7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Title : SVOA CALIBRATION

37	18.428	2588	2591	2596	rVB	21999	28012	0.51%	0.059%
38	19.392	2752	2755	2760	rVB2	41762	53571	0.97%	0.112%
39	19.463	2764	2767	2773	rVB	53452	73381	1.33%	0.154%
40	19.575	2783	2786	2796	rBV	75739	107639	1.95%	0.225%
41	19.816	2821	2827	2838	rBV	4048919	5522464	100.00%	11.569%
42	21.257	3068	3072	3080	rBV	261459	450160	8.15%	0.943%
43	21.574	3121	3126	3136	rBV	1973359	2662794	48.22%	5.578%
44	23.963	3524	3532	3544	rVB2	2573043	5431464	98.35%	11.379%
45	24.127	3553	3560	3569	rVB	1163297	2506508	45.39%	5.251%




Sum of corrected areas: 47734339

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015456.D
Acq On : 09 Jun 2023 17:26
Operator : MA/JU
Sample : 03097-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEN7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

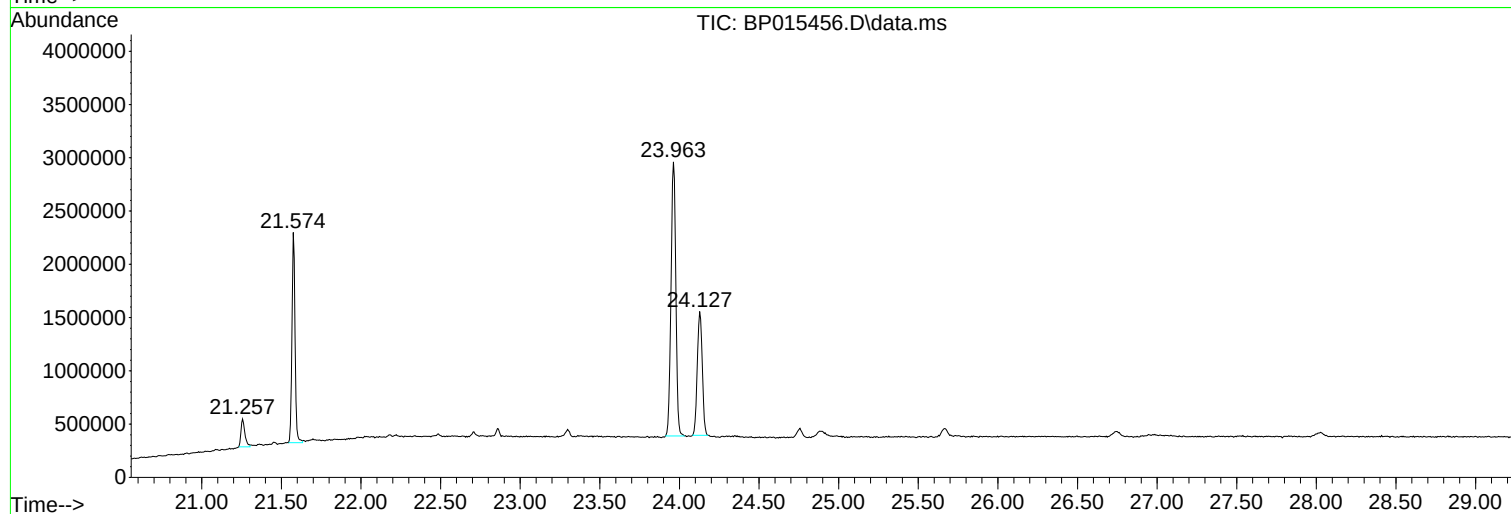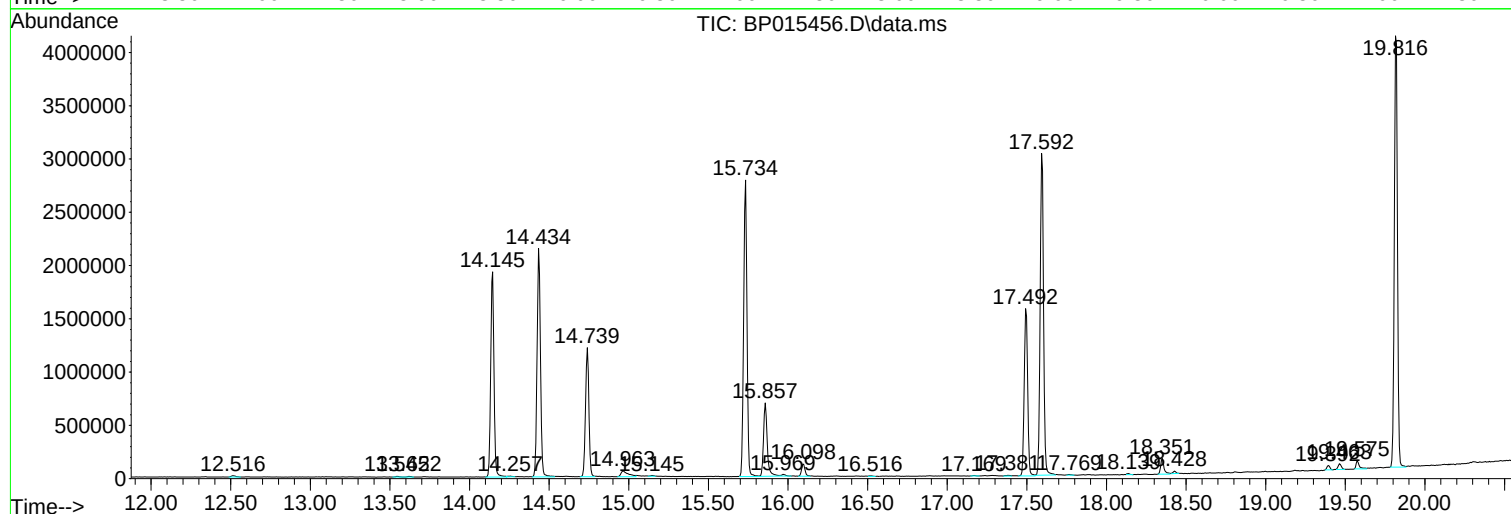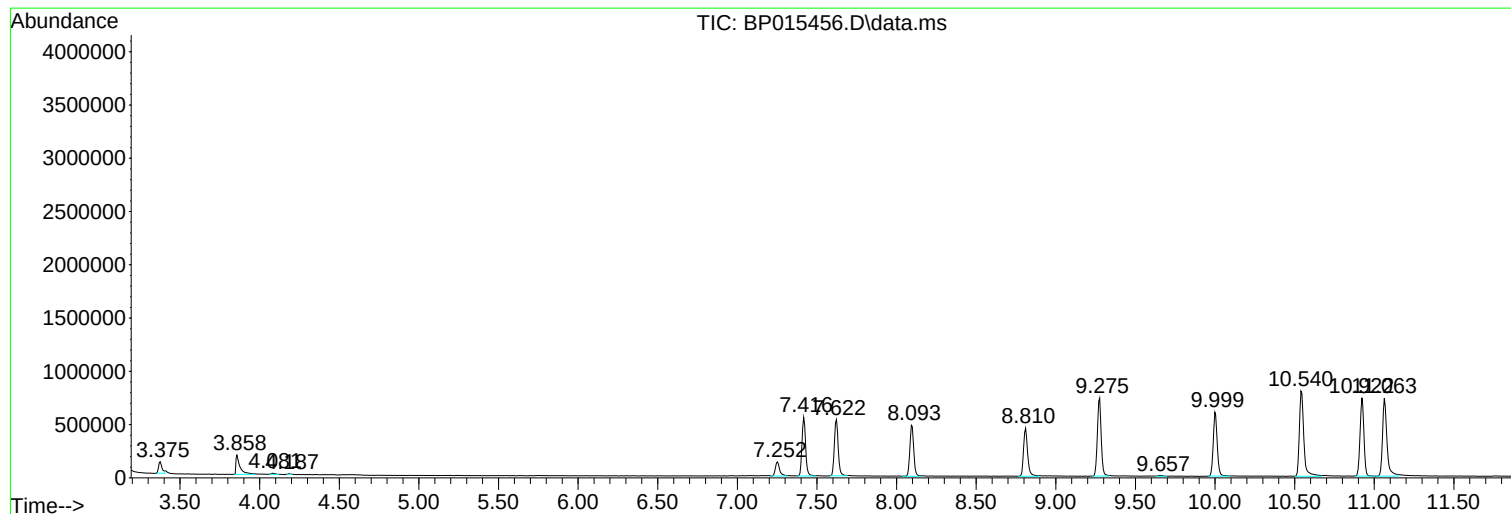

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015456.D
Acq On : 09 Jun 2023 17:26
Operator : MA/JU
Sample : 03097-14
Misc :
ALS Vial : 10 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
EZEN7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.257	3.38 ng/ul	450160	Chrysene-d12	21.574	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	5-Eicosene, (E)-	280	C20H40	074685-30-6	99
2	3-Eicosene, (E)-	280	C20H40	074685-33-9	96
3	E-14-Hexadecenal	238	C16H30O	330207-53-9	95
4	Heptafluorobutyric acid, n-tetra...	410	C18H29F7O2	007365-36-8	94
5	Behenic alcohol	326	C22H46O	000661-19-8	94

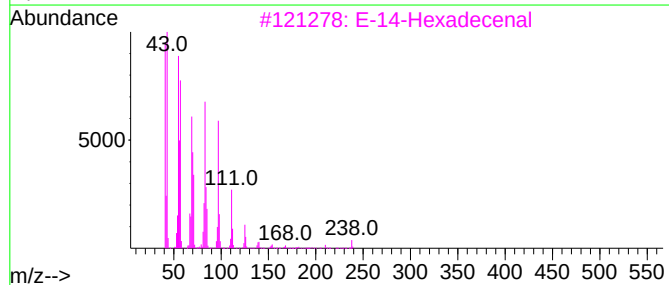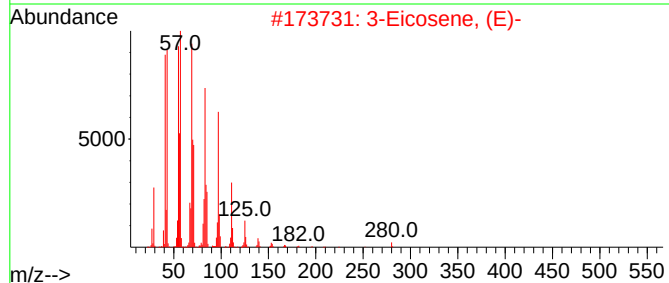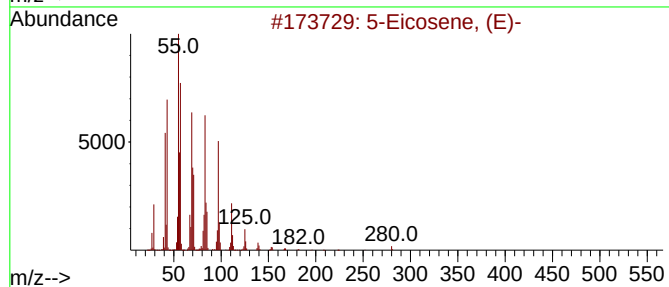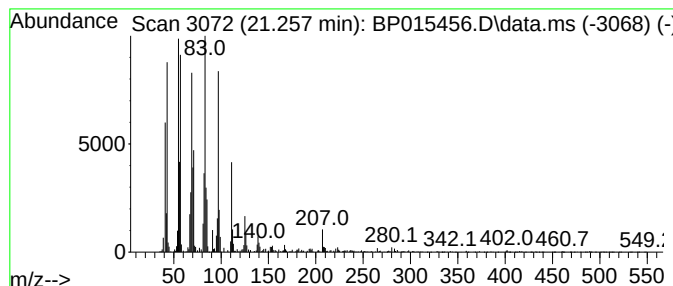

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015456.D
Acq On : 09 Jun 2023 17:26
Operator : MA/JU
Sample : 03097-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEN7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.257	3.4	ng/u1	450160	5	21.574	2662790	20.0