

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
 Data File : BP015457.D
 Acq On : 09 Jun 2023 18:00
 Operator : MA/JU
 Sample : 03097-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015457.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	28	32	35	rBV	33754	44390	0.84%	0.088%
2	3.410	35	38	42	rVB2	14593	19549	0.37%	0.039%
3	3.510	52	55	59	rBV2	10171	12320	0.23%	0.025%
4	3.858	112	114	131	rBV	106339	206282	3.90%	0.411%
5	4.087	149	153	159	rVB3	10720	16076	0.30%	0.032%
6	4.187	165	170	177	rBV4	11486	19883	0.38%	0.040%
7	7.251	685	691	706	rVB	115892	208935	3.95%	0.416%
8	7.416	713	719	732	rBV	500627	816261	15.44%	1.626%
9	7.622	746	754	764	rBV	484038	799791	15.13%	1.594%
10	8.093	827	834	849	rBV	628792	1062610	20.10%	2.117%
11	8.810	947	956	976	rBV	390511	697456	13.19%	1.390%
12	9.275	1027	1035	1051	rBV	671005	1150352	21.76%	2.292%
13	9.657	1093	1100	1108	rVB5	7630	16784	0.32%	0.033%
14	9.998	1152	1158	1176	rBV	551493	963056	18.22%	1.919%
15	10.545	1244	1251	1272	rBV	679045	1341786	25.38%	2.673%
16	10.687	1274	1275	1282	rVB7	3643	5638	0.11%	0.011%
17	10.922	1307	1315	1325	rBV	1005330	1665220	31.50%	3.318%
18	11.063	1330	1339	1360	rBV	614492	1236240	23.39%	2.463%
19	11.745	1449	1455	1464	rBV	5310	15866	0.30%	0.032%
20	12.334	1549	1555	1561	rBV6	7124	13739	0.26%	0.027%
21	12.510	1581	1585	1592	rBV2	13343	24757	0.47%	0.049%
22	13.092	1680	1684	1688	rBV7	4119	6136	0.12%	0.012%
23	13.345	1721	1727	1731	rBV6	7682	11244	0.21%	0.022%
24	13.545	1757	1761	1764	rBV7	4650	7037	0.13%	0.014%
25	13.622	1769	1774	1780	rBV3	21164	36081	0.68%	0.072%
26	14.145	1854	1863	1872	rBV	1825796	2701087	51.09%	5.382%
27	14.433	1905	1912	1928	rBV2	1980732	2975875	56.29%	5.929%
28	14.739	1955	1964	1981	rBV	1684129	2510329	47.49%	5.002%
29	14.975	1997	2004	2017	rBV3	34118	127382	2.41%	0.254%
30	15.145	2029	2033	2046	rVB3	9187	20274	0.38%	0.040%
31	15.245	2046	2050	2055	rVB8	3278	5839	0.11%	0.012%
32	15.516	2090	2096	2099	rBV	11254	17350	0.33%	0.035%
33	15.551	2099	2102	2107	rVB3	9768	12944	0.24%	0.026%
34	15.727	2126	2132	2148	rVV	2472731	3824954	72.35%	7.621%
35	15.857	2148	2154	2170	rVV	881154	1331308	25.18%	2.652%
36	15.975	2171	2174	2179	rVB3	14489	20485	0.39%	0.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
 Data File : BP015457.D
 Acq On : 09 Jun 2023 18:00
 Operator : MA/JU
 Sample : 03097-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

37	16.092	2189	2194	2203	rVB	81163	125502	2.37%	0.250%
38	16.510	2261	2265	2271	rVB8	3864	7039	0.13%	0.014%
39	16.880	2324	2328	2330	rBV5	4342	5601	0.11%	0.011%
40	17.174	2373	2378	2381	rBV7	4152	7601	0.14%	0.015%
41	17.286	2393	2397	2401	rVV4	5449	8375	0.16%	0.017%
42	17.392	2409	2415	2421	rBV8	8302	16485	0.31%	0.033%
43	17.492	2426	2432	2442	rBV	2201144	3217354	60.86%	6.410%
44	17.592	2442	2449	2464	rVV	2975885	4310128	81.53%	8.587%
45	17.763	2474	2478	2488	rVB4	9418	16794	0.32%	0.033%
46	18.133	2537	2541	2546	rBV	24435	33895	0.64%	0.068%
47	18.351	2573	2578	2585	rBV	109799	154792	2.93%	0.308%
48	18.427	2587	2591	2597	rVB	25705	36536	0.69%	0.073%
49	18.539	2608	2610	2613	rBV3	7996	6780	0.13%	0.014%
50	18.810	2653	2656	2662	rBV	22111	24359	0.46%	0.049%
51	19.392	2751	2755	2760	rBV2	47289	61756	1.17%	0.123%
52	19.463	2764	2767	2775	rVB	52064	75061	1.42%	0.150%
53	19.574	2783	2786	2793	rBV4	46337	67074	1.27%	0.134%
54	19.815	2821	2827	2837	rBV	4003699	5286459	100.00%	10.533%
55	21.251	3067	3071	3080	rBV2	152010	310398	5.87%	0.618%
56	21.574	3121	3126	3136	rBV2	2593353	3627922	68.63%	7.228%
57	23.962	3524	3532	3544	rVB2	2505795	5235428	99.03%	10.431%
58	24.127	3553	3560	3576	rVB	1658502	3610078	68.29%	7.193%




Sum of corrected areas: 50190733

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015457.D
Acq On : 09 Jun 2023 18:00
Operator : MA/JU
Sample : 03097-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

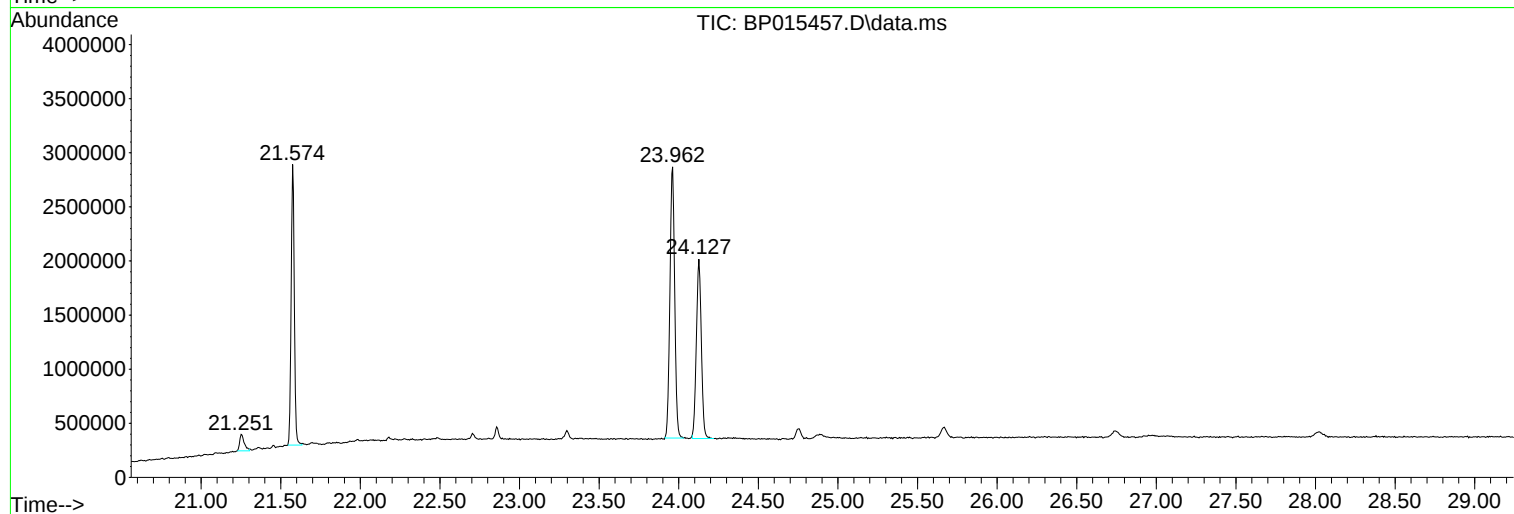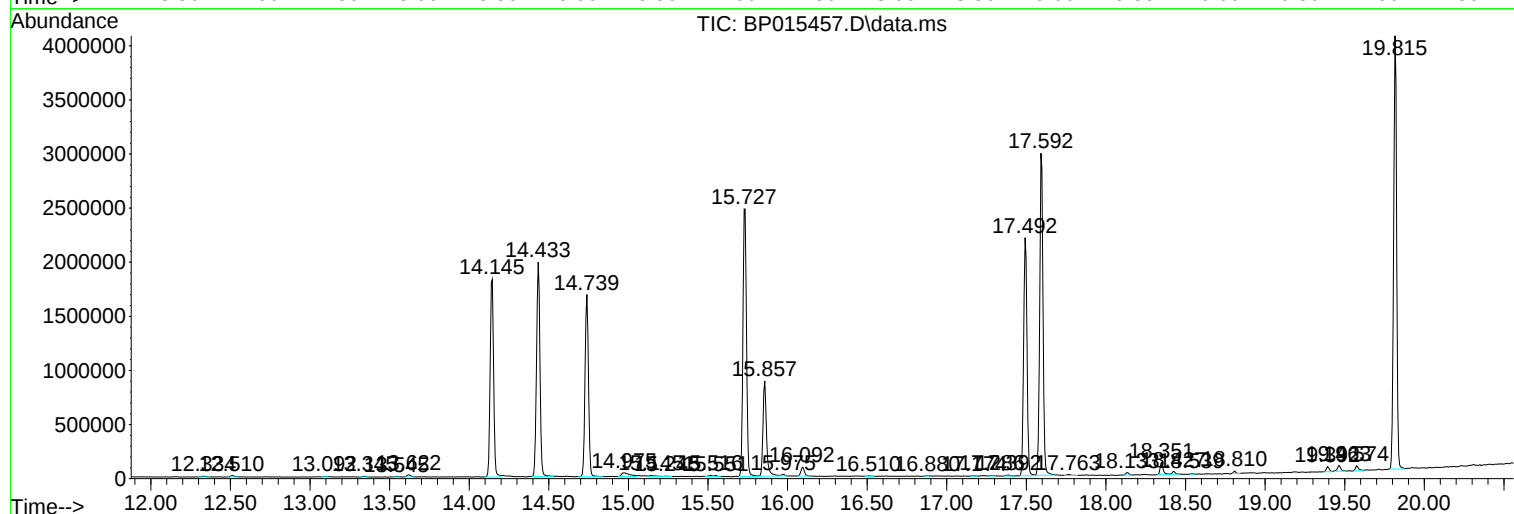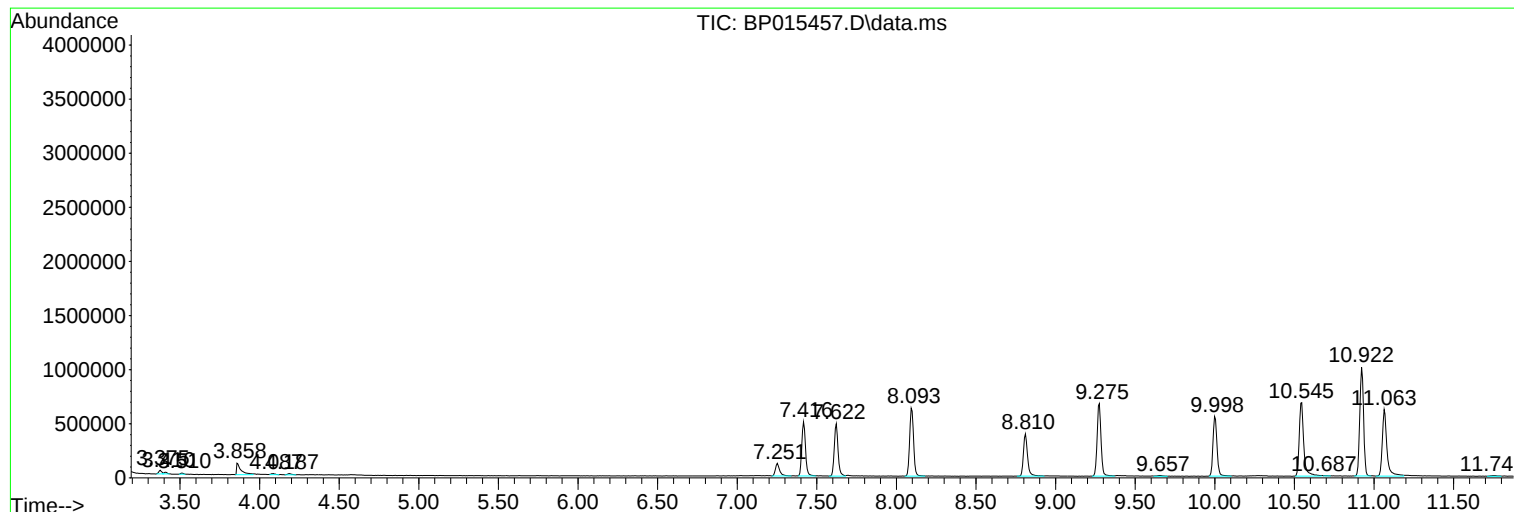

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015457.D
Acq On : 09 Jun 2023 18:00
Operator : MA/JU
Sample : 03097-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015457.D
Acq On : 09 Jun 2023 18:00
Operator : MA/JU
Sample : 03097-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc