

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
 Data File : BP015458.D
 Acq On : 09 Jun 2023 18:34
 Operator : MA/JU
 Sample : 03097-17
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015458.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.411	35	38	44	rVB3	13804	17780	0.34%	0.040%
2	3.858	112	114	124	rBV	108847	178368	3.38%	0.402%
3	4.087	149	153	158	rVB	7730	12510	0.24%	0.028%
4	4.181	167	169	177	rVB4	7370	12589	0.24%	0.028%
5	7.252	685	691	701	rBV	107261	200133	3.79%	0.451%
6	7.416	713	719	729	rBV	474579	760457	14.40%	1.715%
7	7.622	747	754	763	rBV	453867	762890	14.45%	1.720%
8	8.093	828	834	847	rBV	438989	734675	13.92%	1.657%
9	8.810	947	956	972	rBV	372521	661426	12.53%	1.491%
10	9.275	1027	1035	1049	rBV	606700	1076394	20.39%	2.427%
11	9.652	1093	1099	1107	rVB4	6965	14032	0.27%	0.032%
12	9.722	1109	1111	1117	rVB7	4190	6625	0.13%	0.015%
13	9.999	1151	1158	1170	rBV	523694	905637	17.15%	2.042%
14	10.540	1242	1250	1270	rBV	639302	1277920	24.21%	2.882%
15	10.922	1307	1315	1324	rBV	702600	1168919	22.14%	2.636%
16	11.063	1330	1339	1365	rBV	505772	1071196	20.29%	2.415%
17	12.516	1581	1586	1595	rVB2	10855	23221	0.44%	0.052%
18	13.340	1721	1726	1731	rBV8	4151	6288	0.12%	0.014%
19	13.545	1756	1761	1766	rBV7	7366	11646	0.22%	0.026%
20	13.622	1769	1774	1780	rVV2	20077	33651	0.64%	0.076%
21	13.722	1784	1791	1795	rVB10	3204	6897	0.13%	0.016%
22	14.140	1854	1862	1875	rBV	1662247	2490872	47.18%	5.617%
23	14.251	1879	1881	1891	rVB	5566	10868	0.21%	0.025%
24	14.434	1905	1912	1930	rBV2	1807104	2760703	52.29%	6.225%
25	14.610	1940	1942	1948	rVB7	3729	5580	0.11%	0.013%
26	14.739	1957	1964	1974	rBV	1177478	1723166	32.64%	3.886%
27	14.969	1997	2003	2020	rBV5	41701	155547	2.95%	0.351%
28	15.151	2029	2034	2042	rVB5	6879	13268	0.25%	0.030%
29	15.557	2098	2103	2108	rVB4	5127	9715	0.18%	0.022%
30	15.734	2126	2133	2147	rBV	2375458	3567031	67.57%	8.043%
31	15.857	2147	2154	2169	rVV	835052	1302768	24.68%	2.938%
32	15.969	2170	2173	2179	rVB3	14566	23143	0.44%	0.052%
33	16.092	2189	2194	2207	rVB	105438	167213	3.17%	0.377%
34	16.516	2263	2266	2271	rVB7	4430	5805	0.11%	0.013%
35	16.886	2325	2329	2335	rVB9	4499	7677	0.15%	0.017%
36	17.233	2385	2388	2392	rBV6	4855	5922	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
 Data File : BP015458.D
 Acq On : 09 Jun 2023 18:34
 Operator : MA/JU
 Sample : 03097-17
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

37	17.392	2410	2415	2422	rVB8	9168	16368	0.31%	0.037%
38	17.492	2426	2432	2442	rBV	1556934	2261025	42.83%	5.098%
39	17.592	2443	2449	2462	rVV2	2775894	4108990	77.83%	9.265%
40	17.763	2476	2478	2483	rVB3	9417	12036	0.23%	0.027%
41	18.133	2537	2541	2546	rVB2	15795	21468	0.41%	0.048%
42	18.351	2573	2578	2586	rBV	139084	200264	3.79%	0.452%
43	18.428	2587	2591	2604	rVB	32444	52900	1.00%	0.119%
44	18.539	2608	2610	2614	rBV4	6616	7168	0.14%	0.016%
45	18.810	2653	2656	2661	rVB	12319	15046	0.29%	0.034%
46	19.233	2726	2728	2732	rBV5	7333	8549	0.16%	0.019%
47	19.392	2751	2755	2760	rBV	43444	59708	1.13%	0.135%
48	19.463	2764	2767	2771	rVV	48374	59723	1.13%	0.135%
49	19.575	2783	2786	2793	rBV3	54994	74009	1.40%	0.167%
50	19.816	2821	2827	2838	rBV	4035698	5266566	99.76%	11.875%
51	21.251	3067	3071	3083	rBV3	216014	448903	8.50%	1.012%
52	21.574	3121	3126	3137	rBV	1939720	2610882	49.46%	5.887%
53	23.963	3524	3532	3544	rVB2	2475647	5279230	100.00%	11.904%
54	24.127	3553	3560	3578	rVB	1224145	2653004	50.25%	5.982%




Sum of corrected areas: 44348371

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015458.D
Acq On : 09 Jun 2023 18:34
Operator : MA/JU
Sample : 03097-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEQ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

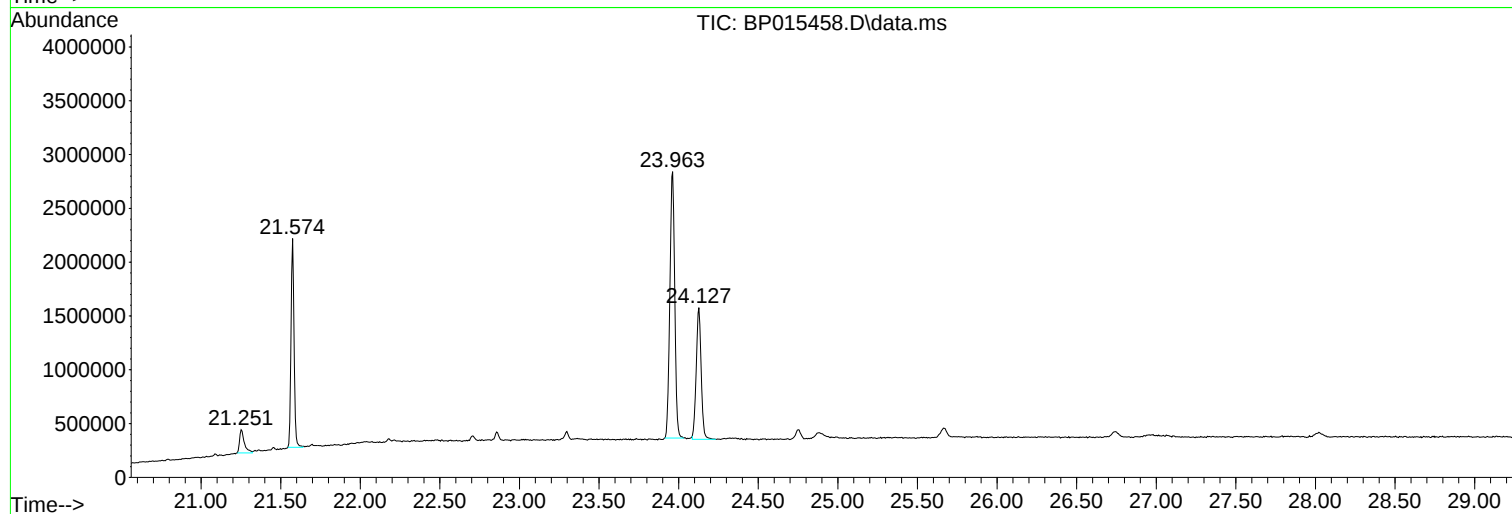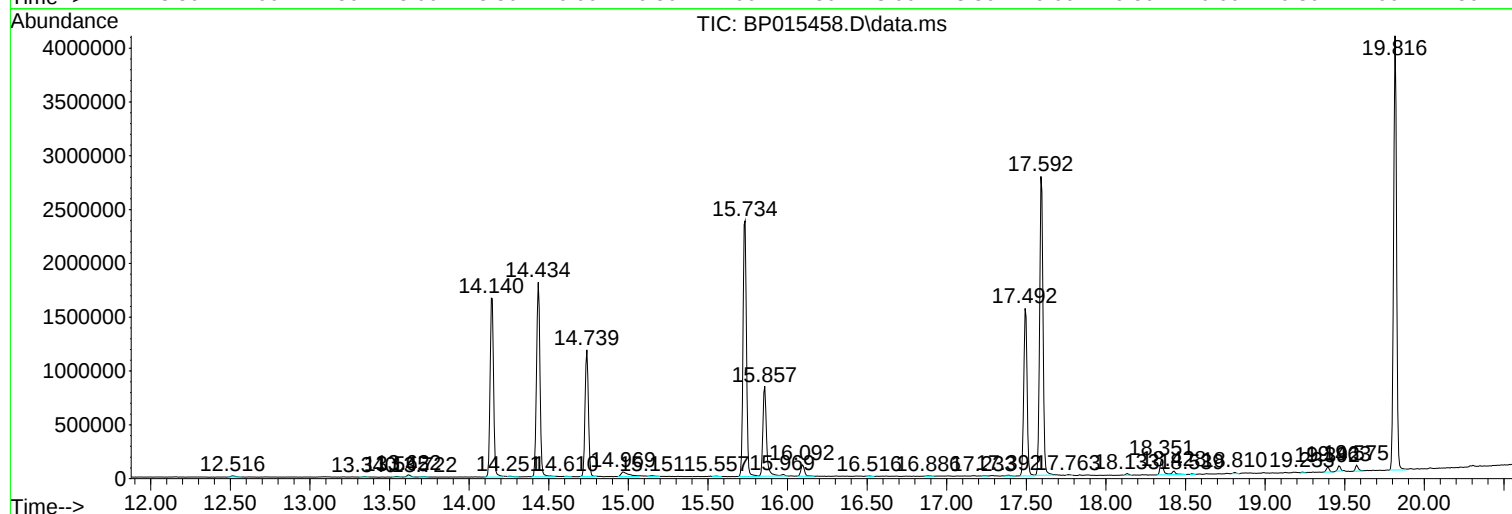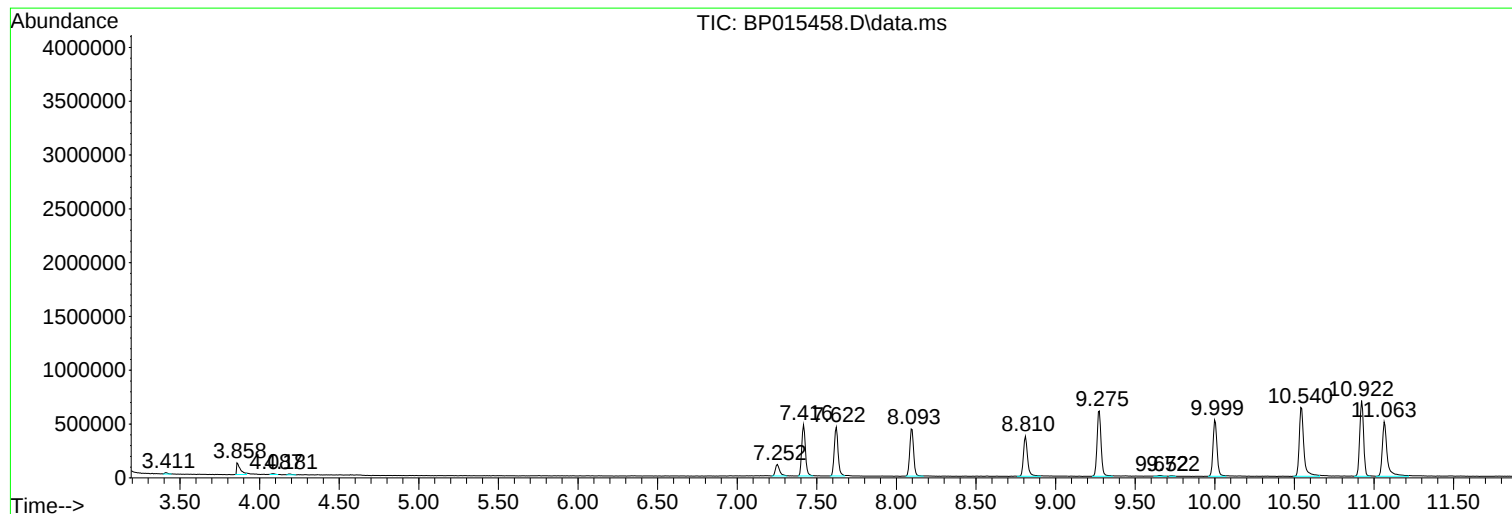

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015458.D
Acq On : 09 Jun 2023 18:34
Operator : MA/JU
Sample : 03097-17
Misc :
ALS Vial : 12 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
EZEQ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.251	3.44 ng/ul	448903	Chrysene-d12	21.574	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	5-Eicosene, (E)-	280	C20H40	074685-30-6	98
2	3-Eicosene, (E)-	280	C20H40	074685-33-9	97
3	Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94
4	Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	94
5	Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	94

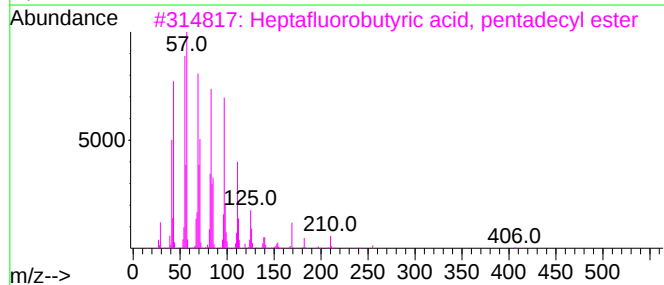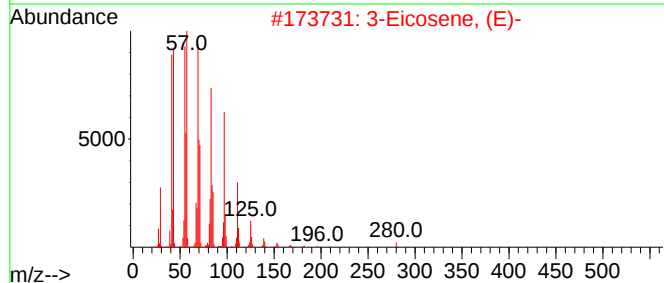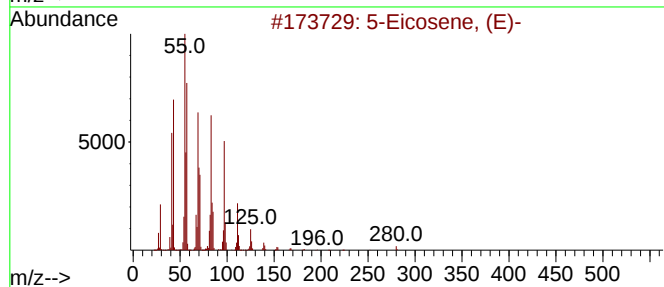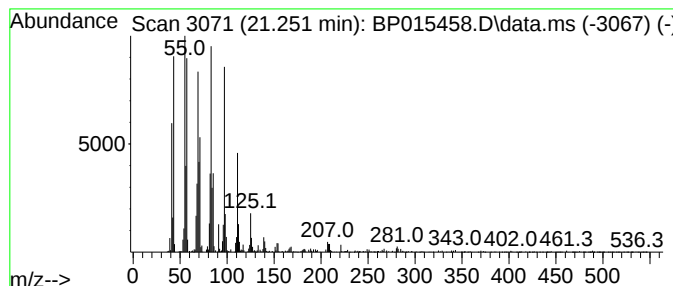

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015458.D
Acq On : 09 Jun 2023 18:34
Operator : MA/JU
Sample : 03097-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEQ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.251	3.4	ng/u1	448903	5	21.574	2610880	20.0