

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
 Data File : BP015460.D
 Acq On : 09 Jun 2023 20:15
 Operator : MA/JU
 Sample : PB153325BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.410	34	38	44	rVB	30019	41585	0.96%	0.097%
2	3.852	111	113	127	rBV	352898	620059	14.28%	1.447%
3	4.193	166	171	174	rBV5	6496	10847	0.25%	0.025%
4	7.246	683	690	709	rBV	488107	868905	20.01%	2.028%
5	7.416	713	719	729	rVV	414890	658173	15.16%	1.536%
6	7.622	747	754	769	rBV	519757	876929	20.19%	2.047%
7	8.093	827	834	845	rBV	485042	806465	18.57%	1.882%
8	8.804	948	955	971	rBV	639480	1157143	26.65%	2.701%
9	9.275	1026	1035	1048	rBV	526250	942526	21.70%	2.200%
10	9.998	1145	1158	1170	rBV	473838	836412	19.26%	1.952%
11	10.539	1243	1250	1276	rBV	603365	1217398	28.03%	2.842%
12	10.922	1307	1315	1325	rBV	786667	1287427	29.65%	3.005%
13	11.063	1329	1339	1372	rBV	591882	1260805	29.03%	2.943%
14	12.528	1582	1588	1593	rBV4	7425	16274	0.37%	0.038%
15	13.622	1767	1774	1782	rBV	22073	36183	0.83%	0.084%
16	13.716	1788	1790	1798	rVB9	3263	5111	0.12%	0.012%
17	14.139	1855	1862	1878	rBV	1521717	2202869	50.73%	5.142%
18	14.433	1905	1912	1933	rBV	1620697	2413917	55.59%	5.634%
19	14.739	1956	1964	1974	rBV	1315145	1971979	45.41%	4.603%
20	14.945	1992	1999	2019	rBV2	309392	882333	20.32%	2.059%
21	15.727	2126	2132	2144	rBV	2072188	3063454	70.54%	7.150%
22	15.857	2148	2154	2170	rVV	626847	1026307	23.63%	2.395%
23	15.969	2170	2173	2184	rVB5	14432	29768	0.69%	0.069%
24	17.280	2392	2396	2403	rBV3	4591	9543	0.22%	0.022%
25	17.492	2425	2432	2443	rBV	1814297	2583031	59.48%	6.029%
26	17.592	2443	2449	2470	rVB	2512685	3560391	81.99%	8.310%
27	18.145	2540	2543	2547	rVB6	3395	5003	0.12%	0.012%
28	19.392	2751	2755	2759	rBV2	36495	48350	1.11%	0.113%
29	19.463	2764	2767	2771	rVB	29021	35751	0.82%	0.083%
30	19.815	2821	2827	2837	rBV	3290014	4342701	100.00%	10.136%
31	21.574	3121	3126	3137	rBV	2081869	2928702	67.44%	6.836%
32	23.956	3523	3531	3543	rBV2	2010853	4272980	98.39%	9.973%
33	24.121	3552	3559	3569	rBV	1259227	2824040	65.03%	6.592%




Sum of corrected areas: 42843361

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015460.D
Acq On : 09 Jun 2023 20:15
Operator : MA/JU
Sample : PB153325BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

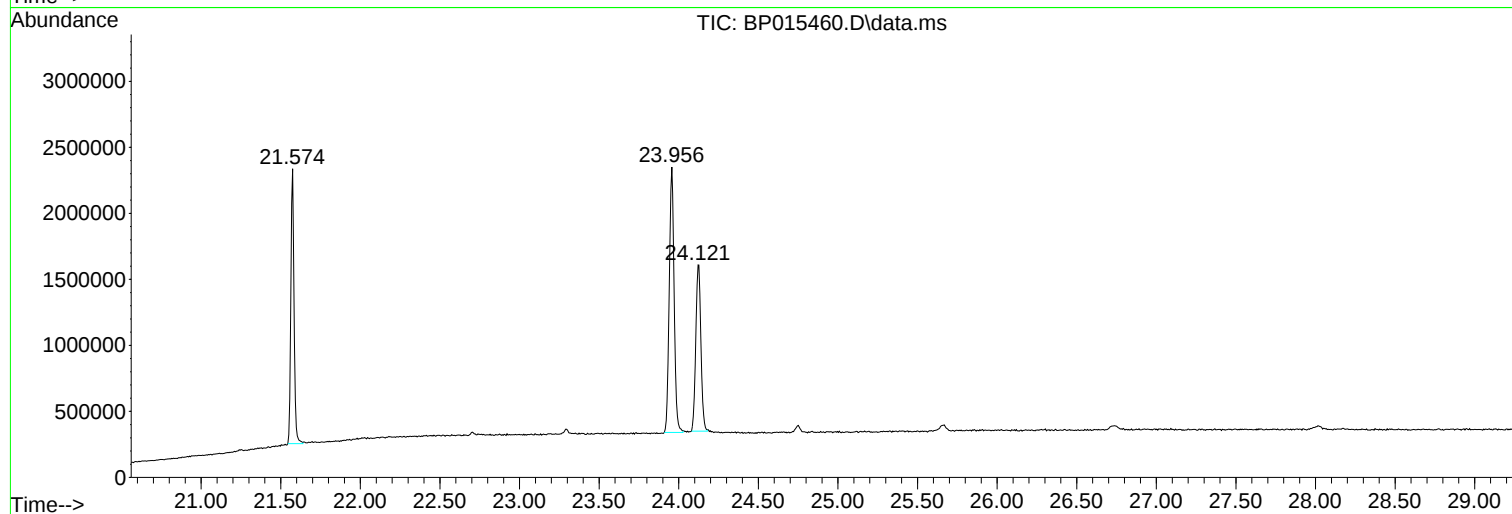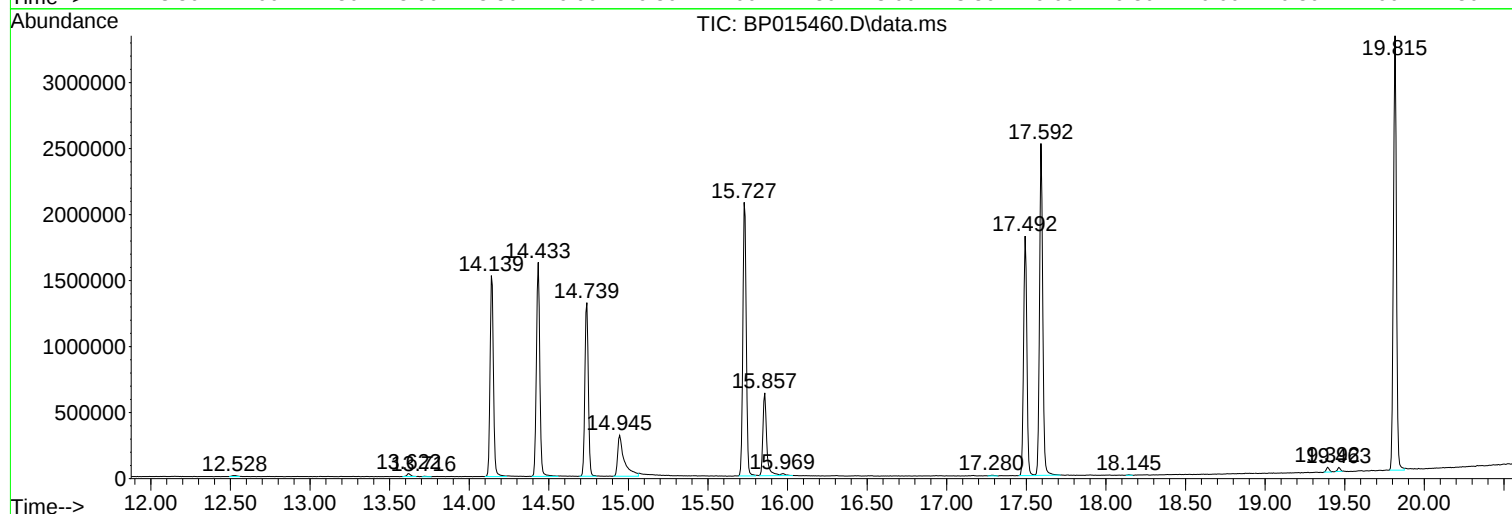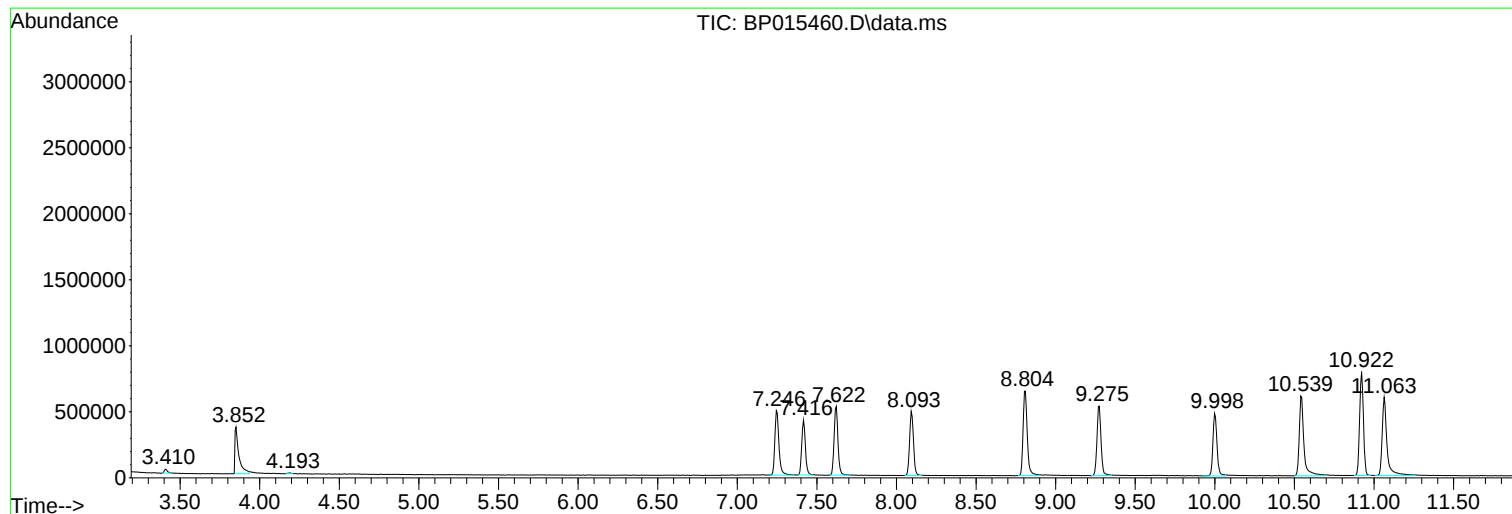

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015460.D
Acq On : 09 Jun 2023 20:15
Operator : MA/JU
Sample : PB153325BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015460.D
Acq On : 09 Jun 2023 20:15
Operator : MA/JU
Sample : PB153325BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc