

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
 Data File : BP015467.D
 Acq On : 10 Jun 2023 00:44
 Operator : MA/JU
 Sample : 03097-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.411	35	38	44	rBV	14815	17753	0.29%	0.037%
2	3.864	112	115	126	rBV	77512	157925	2.58%	0.330%
3	4.081	150	152	158	rVB5	8080	11070	0.18%	0.023%
4	4.181	167	169	175	rVB4	7546	11134	0.18%	0.023%
5	7.252	685	691	704	rBV	122220	226654	3.71%	0.474%
6	7.416	711	719	734	rBV	534463	857942	14.03%	1.794%
7	7.622	747	754	771	rBV	488292	861591	14.09%	1.801%
8	8.093	826	834	843	rBV	437905	713338	11.66%	1.491%
9	8.805	949	955	969	rBV	400891	727302	11.89%	1.521%
10	8.934	973	977	982	rVB4	8516	13848	0.23%	0.029%
11	9.269	1027	1034	1049	rBV	712544	1216008	19.88%	2.542%
12	9.652	1097	1099	1104	rVB6	5509	7043	0.12%	0.015%
13	9.999	1150	1158	1174	rBV	583812	1023019	16.72%	2.139%
14	10.540	1243	1250	1276	rBV	729333	1418792	23.19%	2.966%
15	10.922	1307	1315	1330	rVB	660975	1134437	18.55%	2.372%
16	11.063	1330	1339	1359	rBV	650799	1294145	21.16%	2.706%
17	11.610	1427	1432	1440	rBV	4289	8286	0.14%	0.017%
18	12.228	1532	1537	1540	rBV6	6629	10733	0.18%	0.022%
19	12.510	1576	1585	1594	rBV3	12726	26952	0.44%	0.056%
20	13.028	1668	1673	1678	rBV3	15722	25099	0.41%	0.052%
21	13.269	1710	1714	1721	rVB	11383	18562	0.30%	0.039%
22	13.340	1721	1726	1729	rVB7	5328	6932	0.11%	0.014%
23	13.622	1768	1774	1782	rVB3	24236	48577	0.79%	0.102%
24	14.140	1851	1862	1877	rBV	1934818	2786104	45.55%	5.825%
25	14.434	1903	1912	1931	rBV	2066247	3098611	50.66%	6.478%
26	14.734	1957	1963	1975	rBV	1093171	1676976	27.41%	3.506%
27	14.963	1996	2002	2016	rBV3	45695	163572	2.67%	0.342%
28	15.145	2030	2033	2042	rVB10	8351	14765	0.24%	0.031%
29	15.475	2084	2089	2092	rBV	7318	10650	0.17%	0.022%
30	15.510	2093	2095	2098	rVV2	5453	6767	0.11%	0.014%
31	15.545	2098	2101	2106	rVB	13743	18460	0.30%	0.039%
32	15.728	2125	2132	2146	rBV	2762413	3969903	64.90%	8.299%
33	15.851	2147	2153	2169	rVV	928395	1442558	23.58%	3.016%
34	15.969	2169	2173	2184	rVB4	18166	39594	0.65%	0.083%
35	16.092	2189	2194	2204	rVB2	21733	45099	0.74%	0.094%
36	16.428	2247	2251	2256	rBV7	5434	7447	0.12%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
 Data File : BP015467.D
 Acq On : 10 Jun 2023 00:44
 Operator : MA/JU
 Sample : 03097-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

37	17.075	2356	2361	2366	rVB5	5171	7662	0.13%	0.016%
38	17.163	2373	2376	2380	rVB6	5291	7543	0.12%	0.016%
39	17.222	2382	2386	2390	rBV2	11724	15480	0.25%	0.032%
40	17.281	2392	2396	2400	rBV5	4450	9025	0.15%	0.019%
41	17.492	2425	2432	2442	rVV	1535216	2195835	35.90%	4.591%
42	17.592	2442	2449	2465	rVV	3277256	4792937	78.35%	10.020%
43	17.763	2475	2478	2484	rVB	17142	23282	0.38%	0.049%
44	17.963	2508	2512	2517	rBV4	10783	15157	0.25%	0.032%
45	18.133	2537	2541	2547	rBV8	17508	22441	0.37%	0.047%
46	18.322	2569	2573	2574	rBV4	18707	20862	0.34%	0.044%
47	18.345	2574	2577	2580	rVV2	60854	85564	1.40%	0.179%
48	18.375	2580	2582	2587	rVV2	42485	60638	0.99%	0.127%
49	18.422	2587	2590	2598	rVB	32611	45160	0.74%	0.094%
50	18.628	2623	2625	2630	rVB5	8121	8343	0.14%	0.017%
51	18.845	2659	2662	2669	rBV8	12633	24644	0.40%	0.052%
52	19.392	2751	2755	2760	rBV2	44989	64836	1.06%	0.136%
53	19.463	2762	2767	2774	rVB	49743	72284	1.18%	0.151%
54	19.575	2782	2786	2792	rBV4	48413	71761	1.17%	0.150%
55	19.816	2821	2827	2838	rBV	4384883	5901507	96.48%	12.338%
56	21.574	3120	3126	3134	rBV	1827561	2624576	42.91%	5.487%
57	23.957	3523	3531	3548	rVB2	2884862	6117033	100.00%	12.788%
58	24.121	3552	3559	3572	rVB	1170545	2528833	41.34%	5.287%




Sum of corrected areas: 47833051

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015467.D
Acq On : 10 Jun 2023 00:44
Operator : MA/JU
Sample : 03097-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEP1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

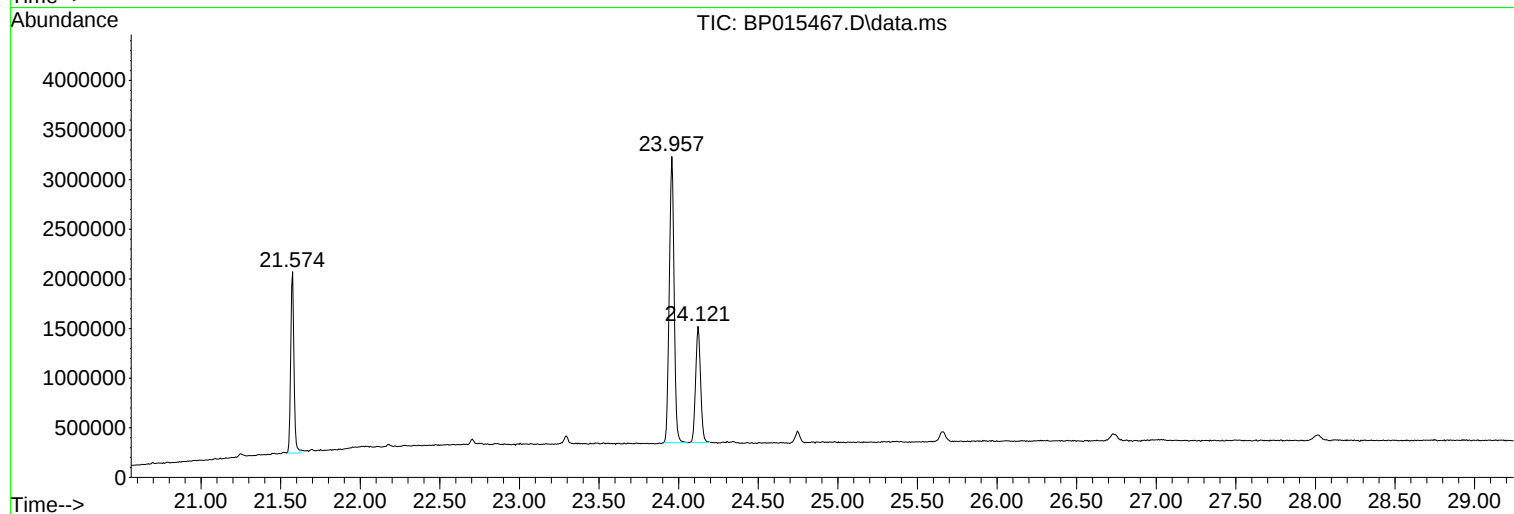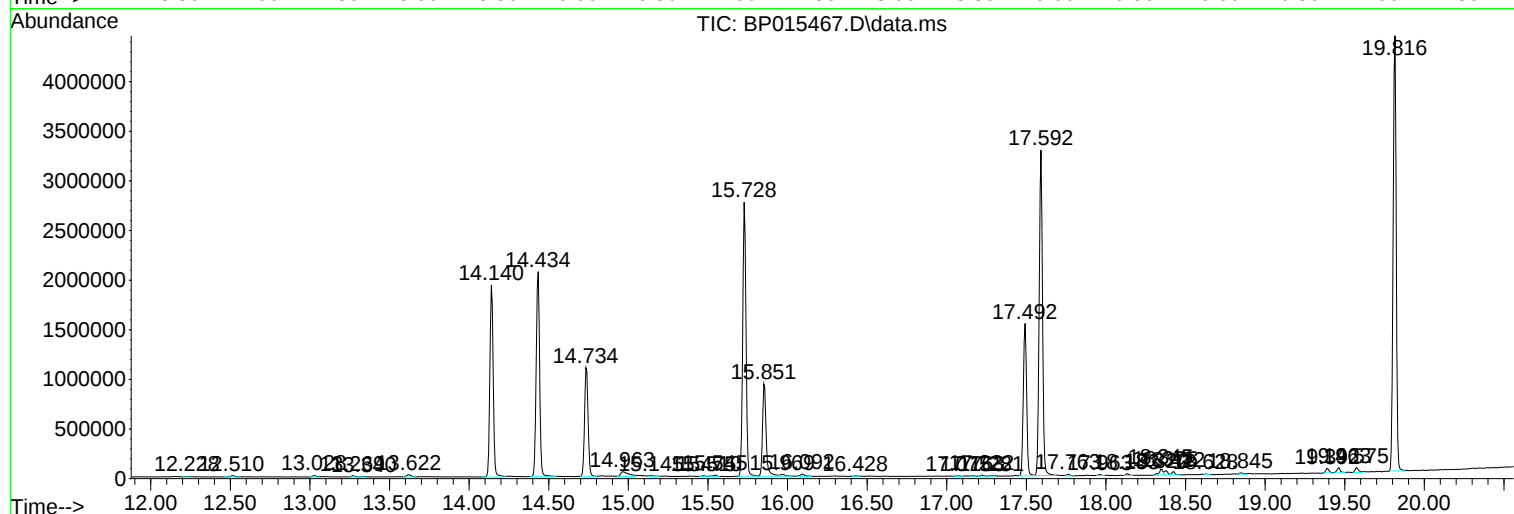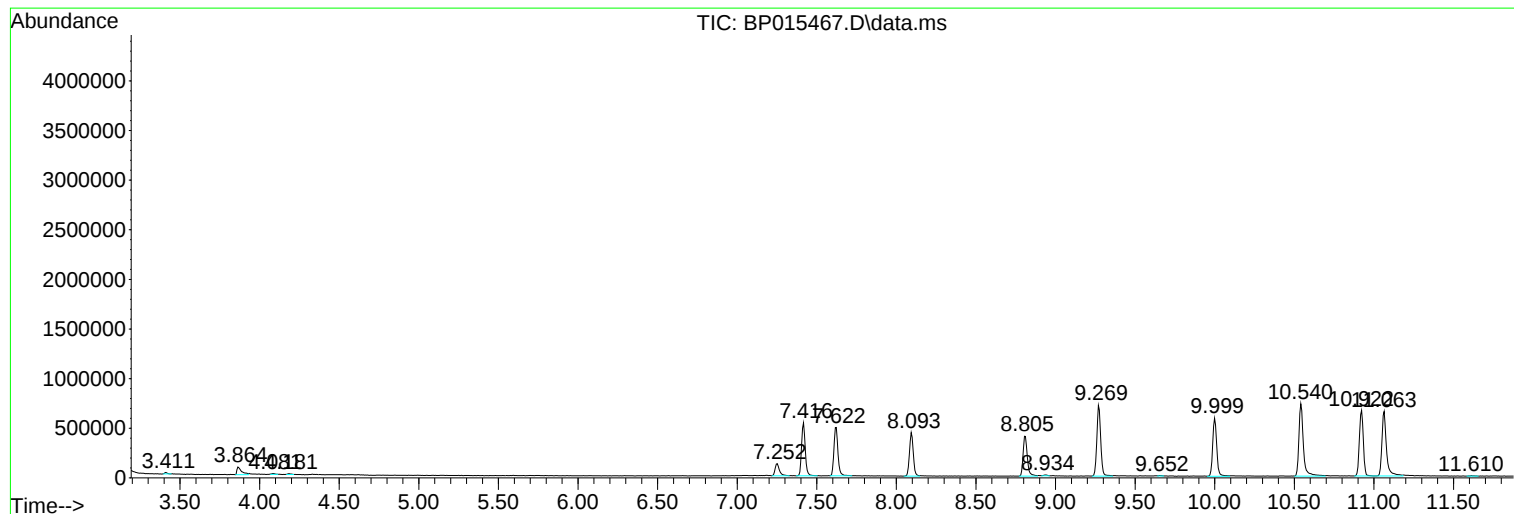

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015467.D
Acq On : 10 Jun 2023 00:44
Operator : MA/JU
Sample : 03097-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEP1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060923\
Data File : BP015467.D
Acq On : 10 Jun 2023 00:44
Operator : MA/JU
Sample : 03097-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEPI

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------