
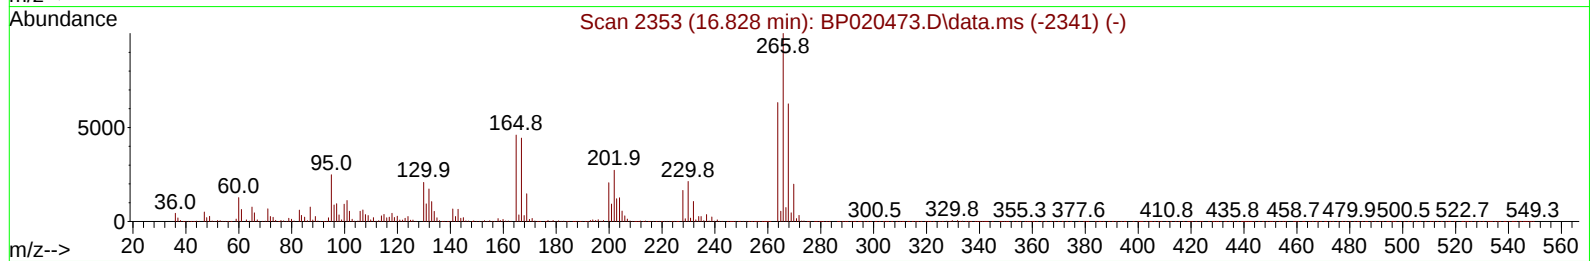
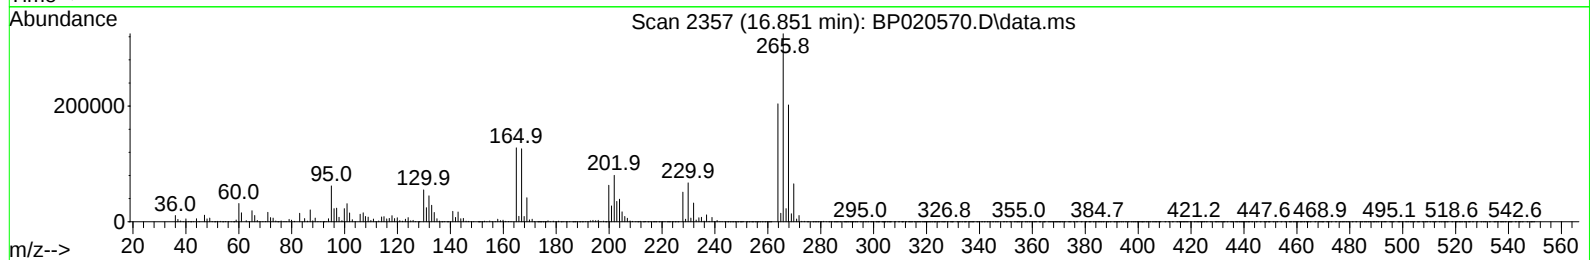


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061024\
Data File : BP020570.D
Acq On : 10 Jun 2024 09:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 11:12:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

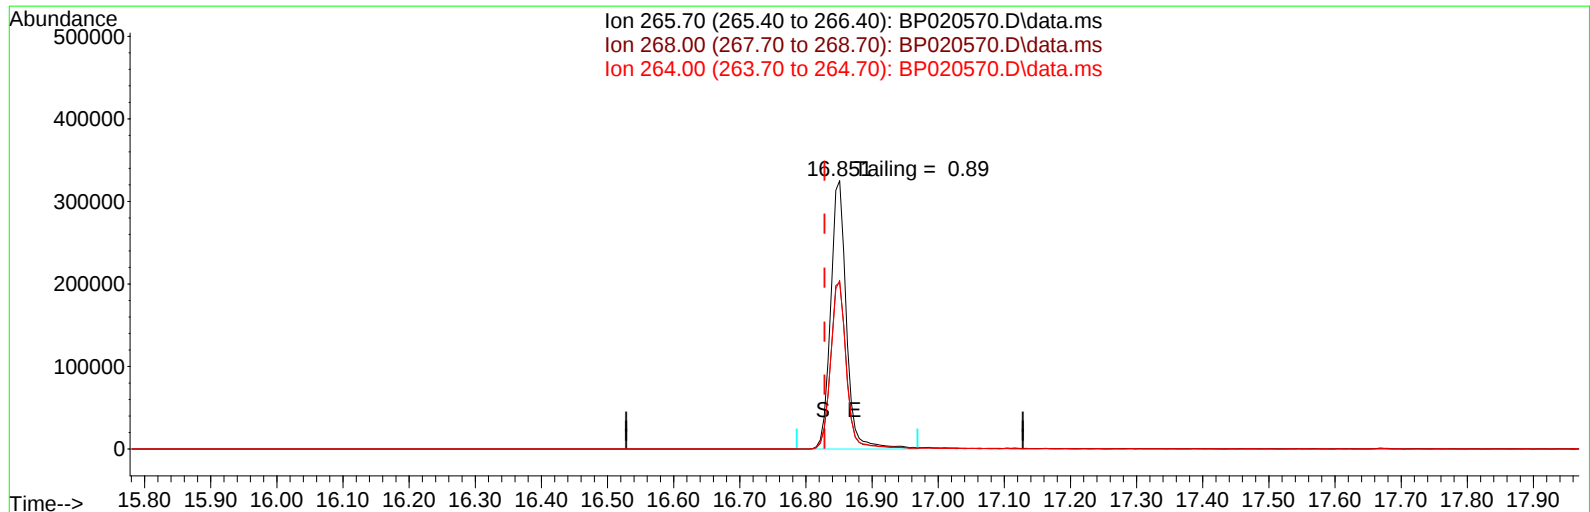

TIC: BP020570.D\data.ms

(70) Pentachlorophenol (C)




16.851min (+ 0.023) 1312903.00 ng

response 537652

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.09
264.00	63.30	62.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061024\
Data File : BP020570.D
Acq On : 10 Jun 2024 09:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 11:12:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

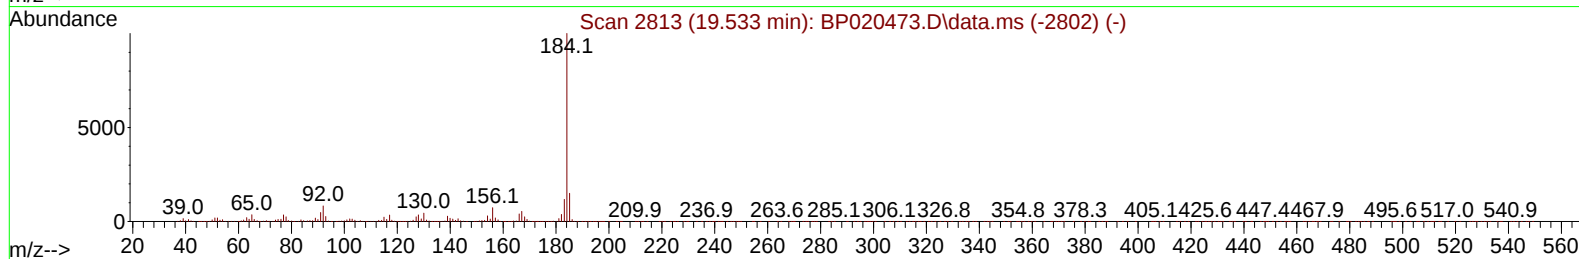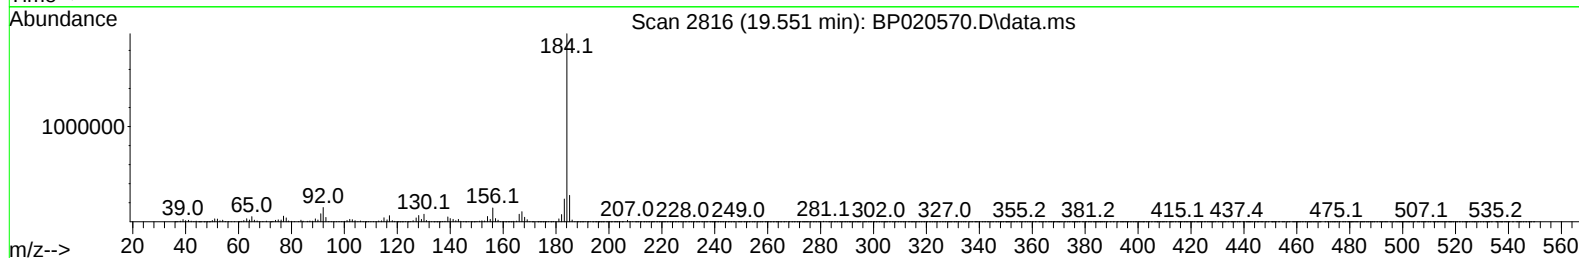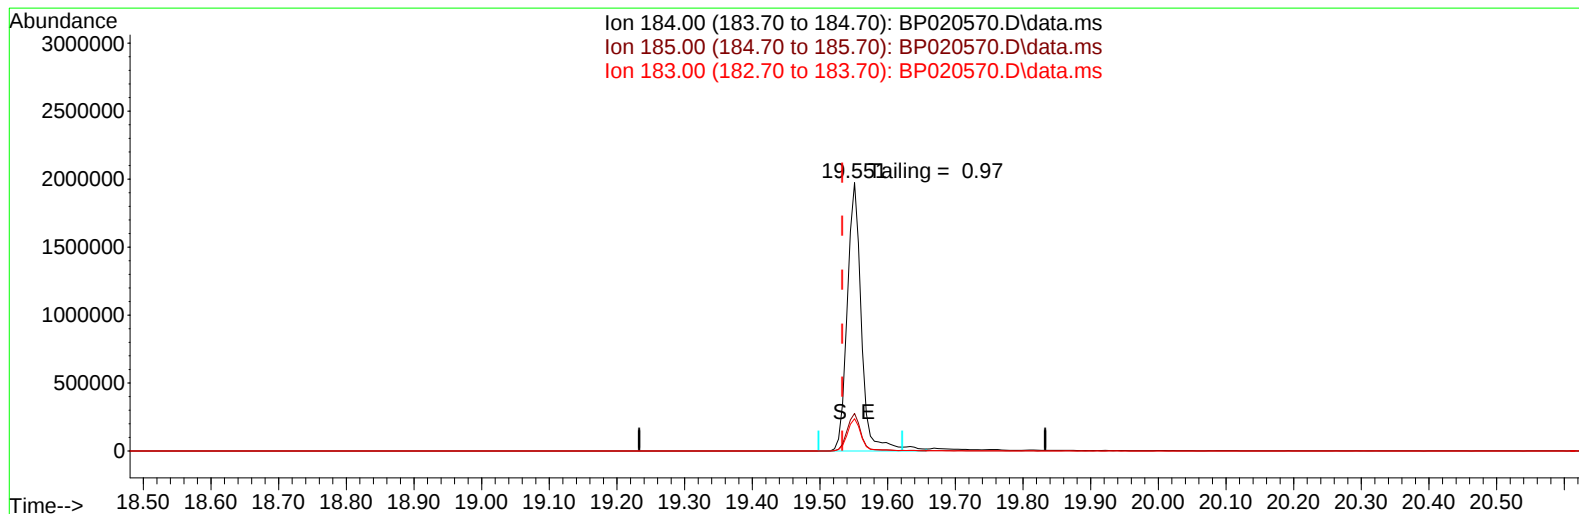

TIC: BP020570.D\data.ms

(77) Benzidine

19.551min (+ 0.018) 228365.55 ng

response 2846489

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.03
183.00	11.70	12.06
0.00	0.00	0.00