
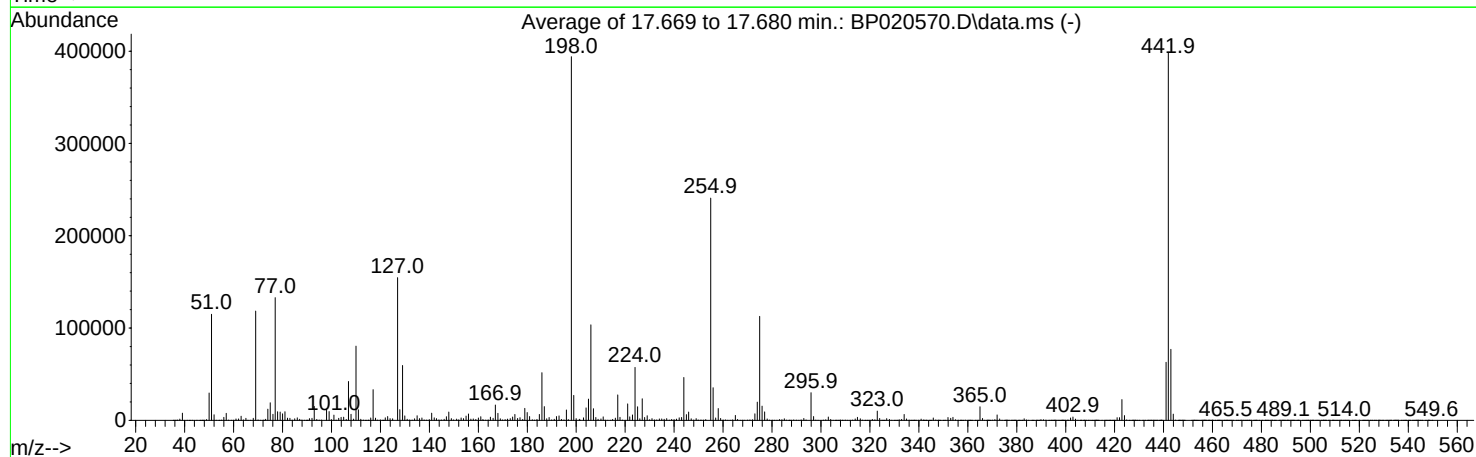


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061024\
Data File : BP020570.D
Acq On : 10 Jun 2024 09:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 30 03:41:03 2024

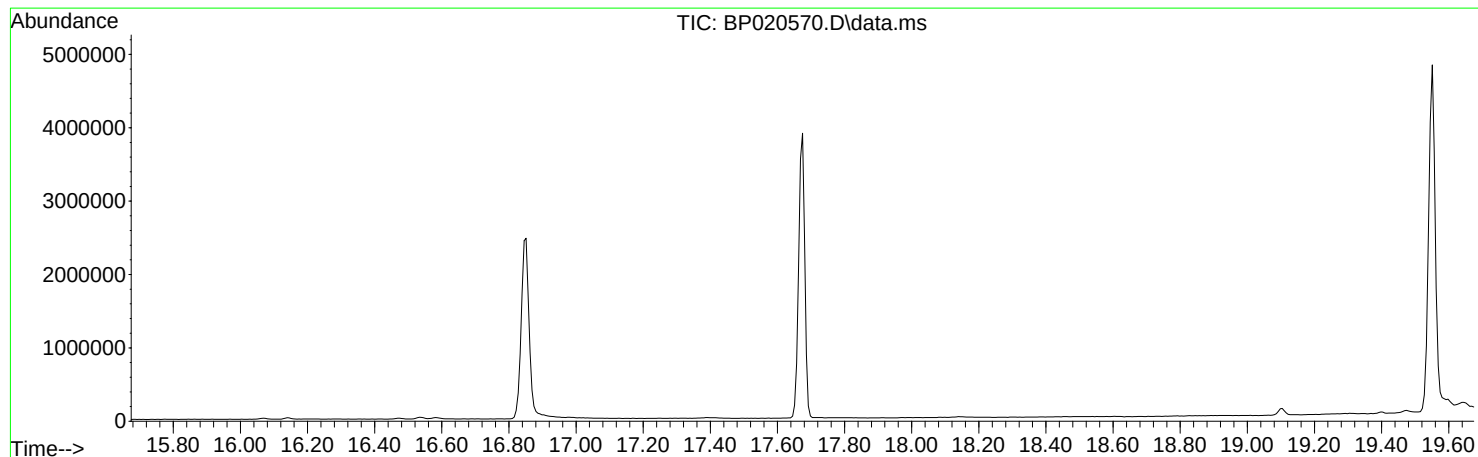

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	114902	PASS
68	69	0.00	2	1.9	2302	PASS
69	198	0.00	100	30.0	118339	PASS
70	69	0.00	2	0.5	595	PASS
127	198	10	80	39.2	154600	PASS
197	198	0.00	2	0.2	835	PASS
198	198	100	100	100.0	394044	PASS
199	198	5	9	6.9	27011	PASS
275	198	10	60	28.6	112682	PASS
365	198	1	100	3.7	14741	PASS
441	198	0.01	100	16.0	62927	PASS
442	442	100	100	100.0	398563	PASS
443	442	15	24	19.3	76944	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/10/2024	BNA_P	<u>BP020570.D</u>
Compound Name	Response	Retention Time
DDT	1334928	20.845
DDD	22779	20.427
DDE	2133	19.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24912	1359840	1.83

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061024\
Data File : BP020570.D
Acq On : 10 Jun 2024 09:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 10 11:12:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

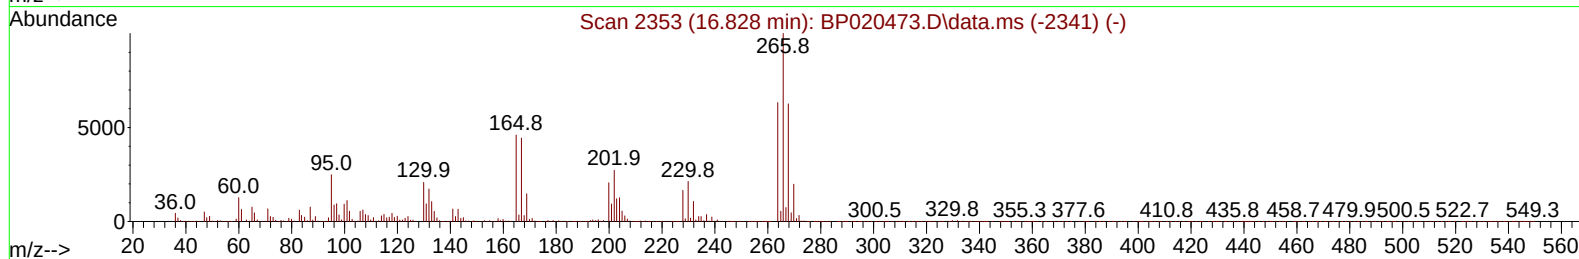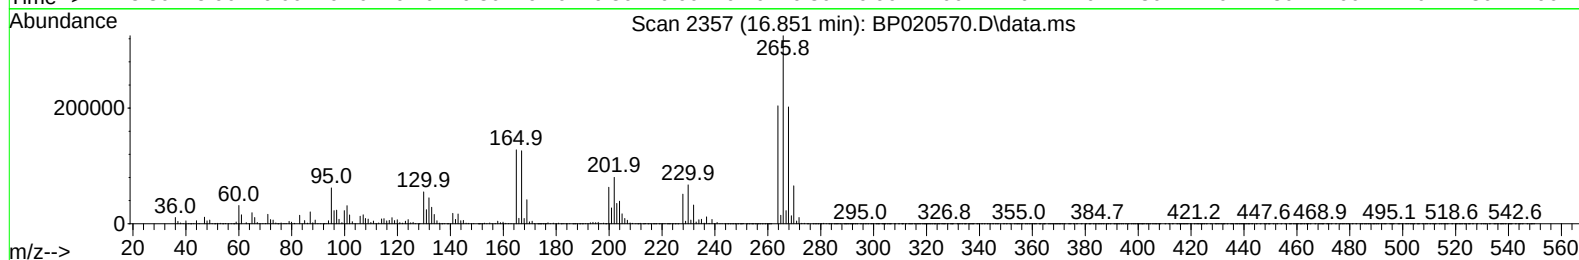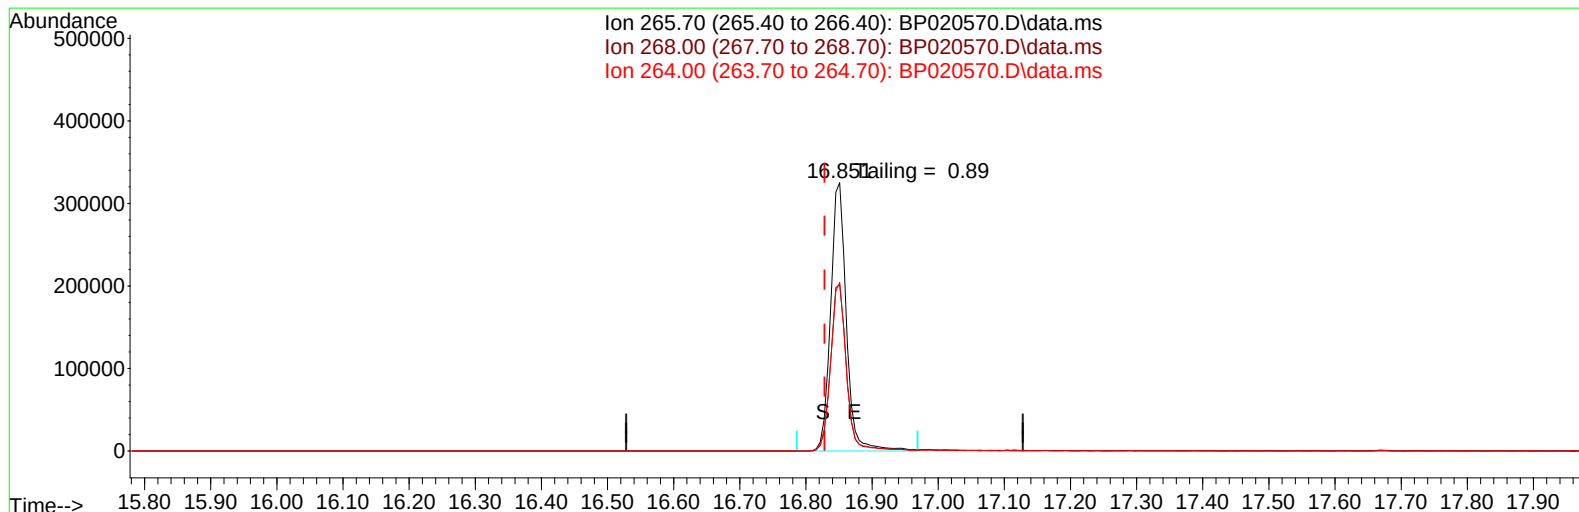

TIC: BP020570.D\data.ms

(70) Pentachlorophenol (C)

16.851min (+ 0.023) 1312903.00 ng




response 537652

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.09
264.00	63.30	62.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061024\
Data File : BP020570.D
Acq On : 10 Jun 2024 09:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 10 11:12:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

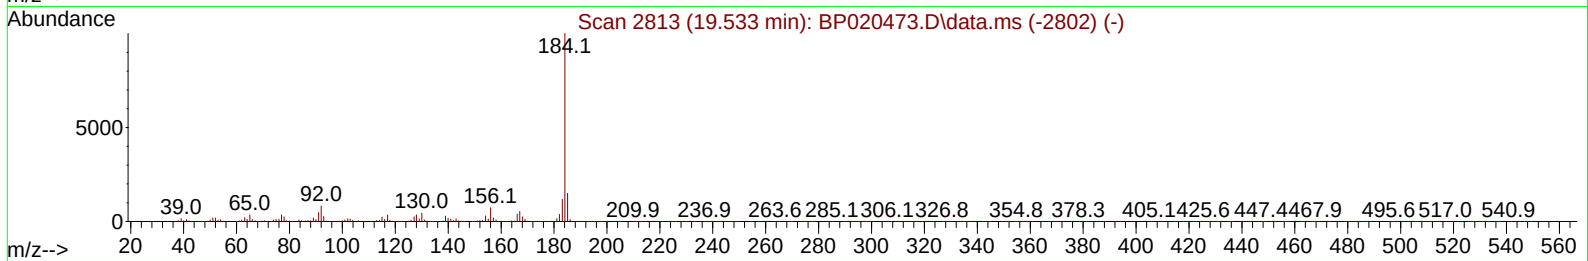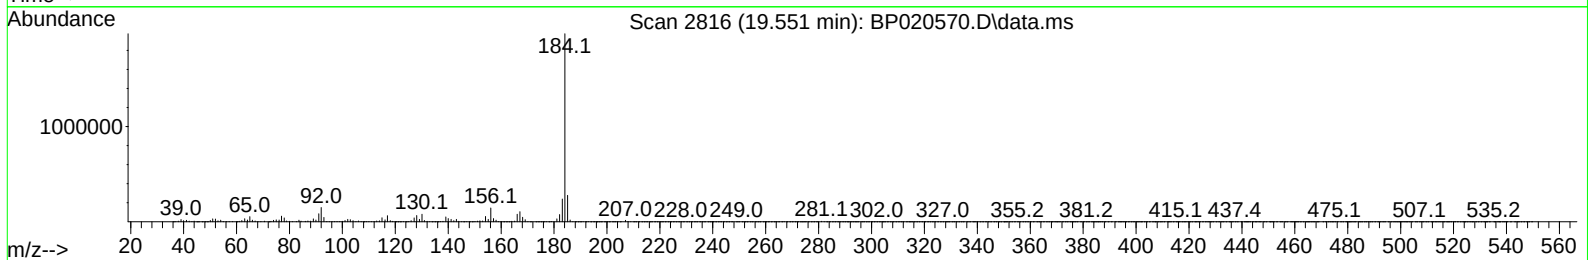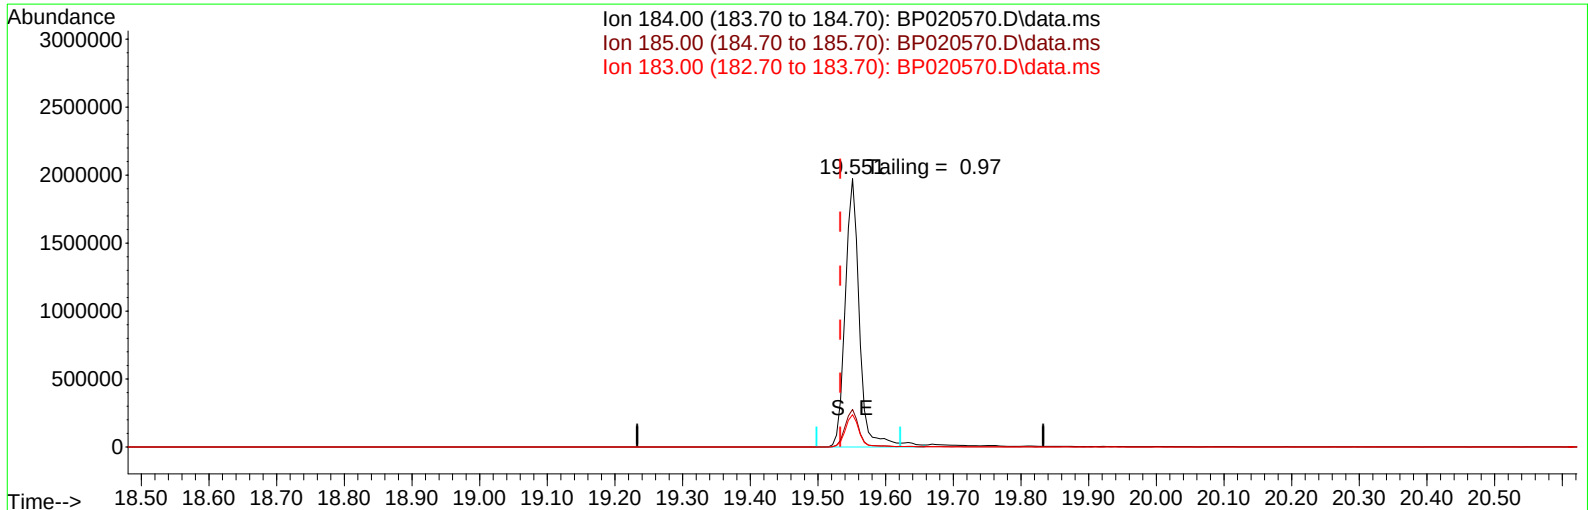

TIC: BP020570.D\data.ms

(77) Benzidine

19.551min (+ 0.018) 228365.55 ng

response 2846489

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.03
183.00	11.70	12.06
0.00	0.00	0.00