


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061124\
Data File : BP020583.D
Acq On : 11 Jun 2024 09:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 30 03:41:03 2024

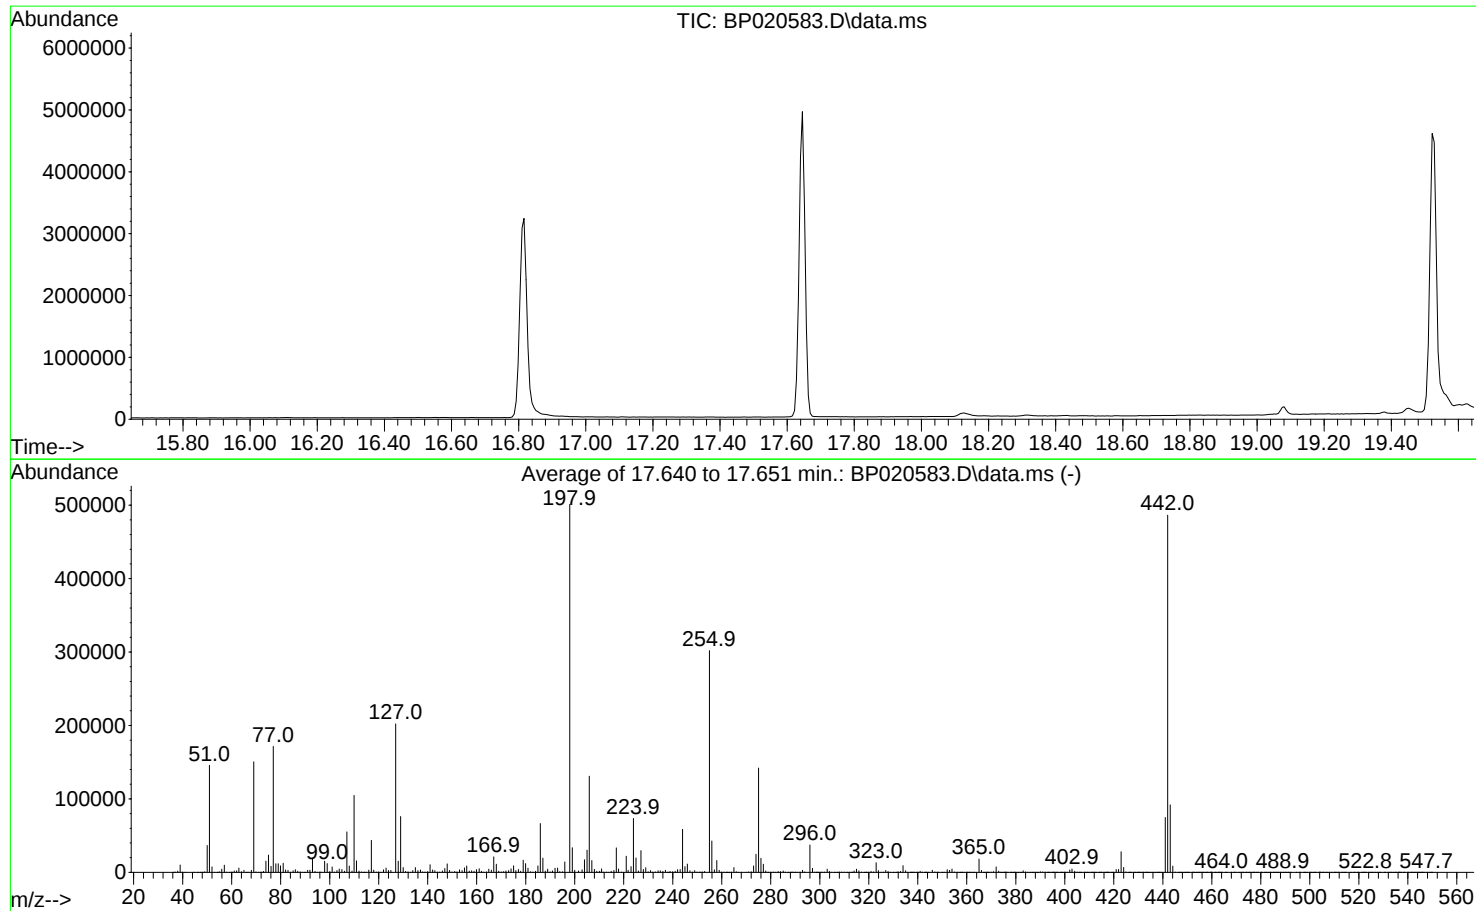

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	145702	PASS
68	69	0.00	2	1.9	2812	PASS
69	198	0.00	100	30.1	150608	PASS
70	69	0.00	2	0.5	748	PASS
127	198	10	80	40.4	202290	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	500912	PASS
199	198	5	9	6.7	33638	PASS
275	198	10	60	28.4	142061	PASS
365	198	1	100	3.6	18037	PASS
441	198	0.01	100	14.9	74787	PASS
442	442	100	100	100.0	486293	PASS
443	442	15	24	18.9	91906	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/11/2024	BNA_P	<u>BP020583.D</u>
Compound Name	Response	Retention Time
DDT	1560265	20.822
DDD	25046	20.41
DDE	3049	19.828
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28095	1588360	1.77

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061124\
Data File : BP020583.D
Acq On : 11 Jun 2024 09:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 11 12:48:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

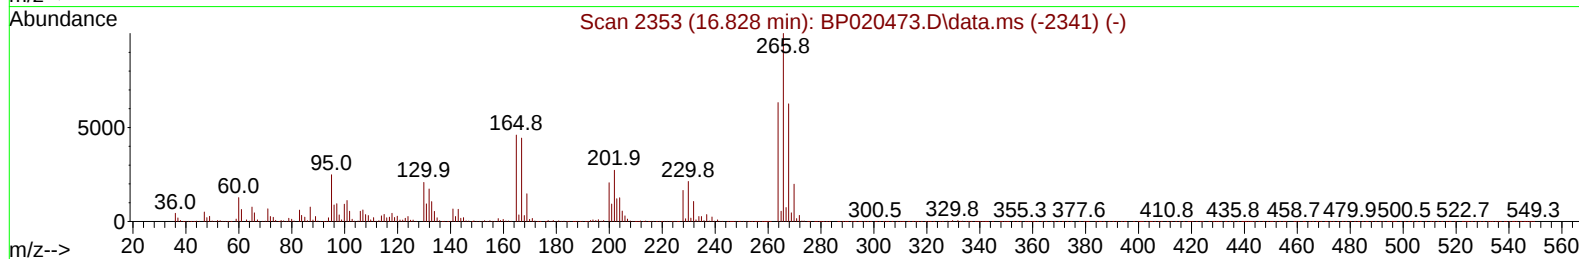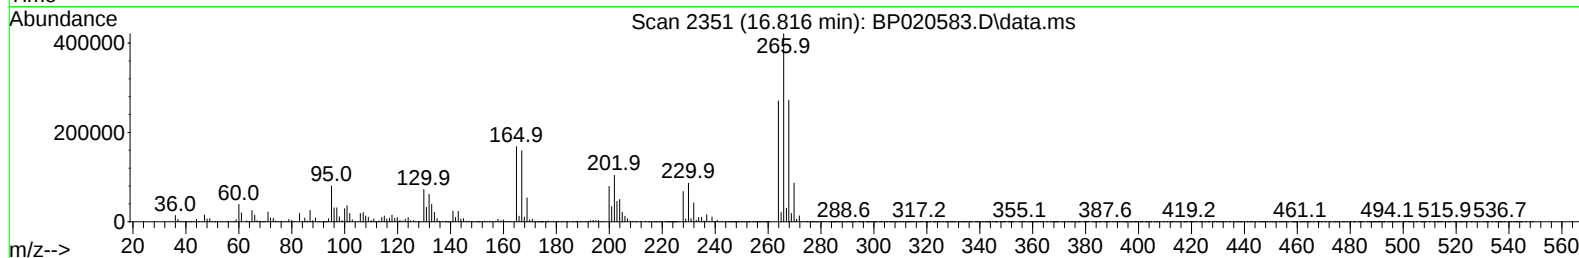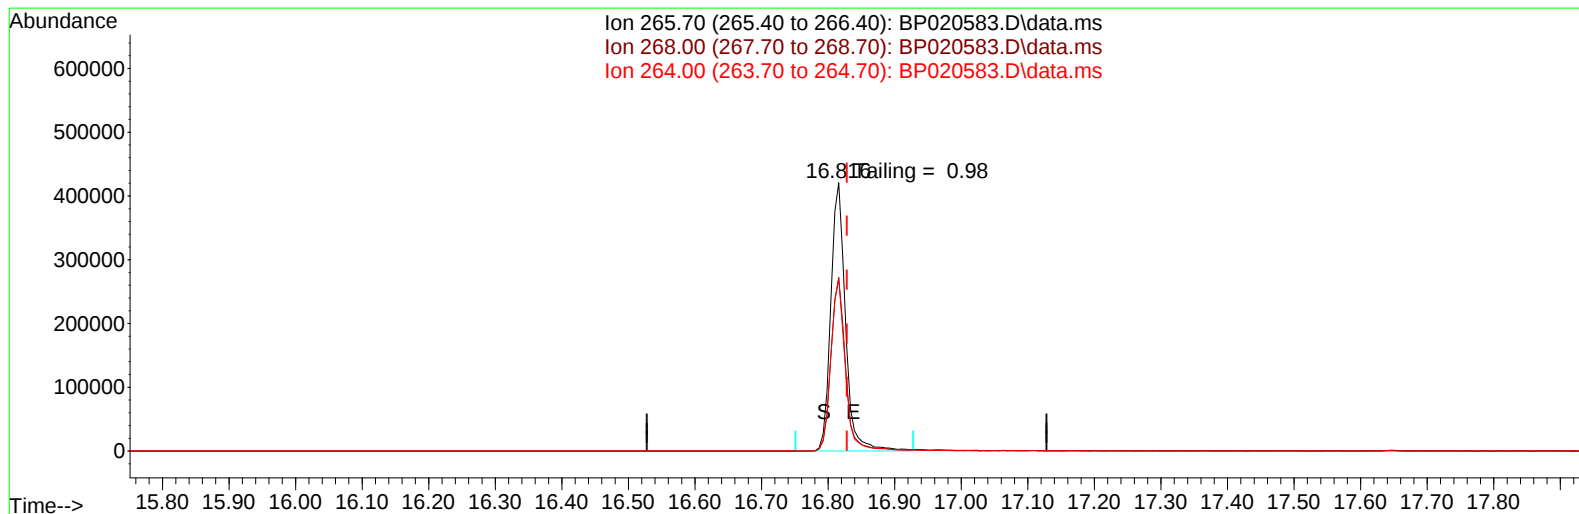

TIC: BP020583.D\data.ms

(70) Pentachlorophenol (C)

16.816min (-0.012) 212989.17 ng




response 647935

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.62
264.00	63.30	64.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061124\
Data File : BP020583.D
Acq On : 11 Jun 2024 09:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 11 12:48:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

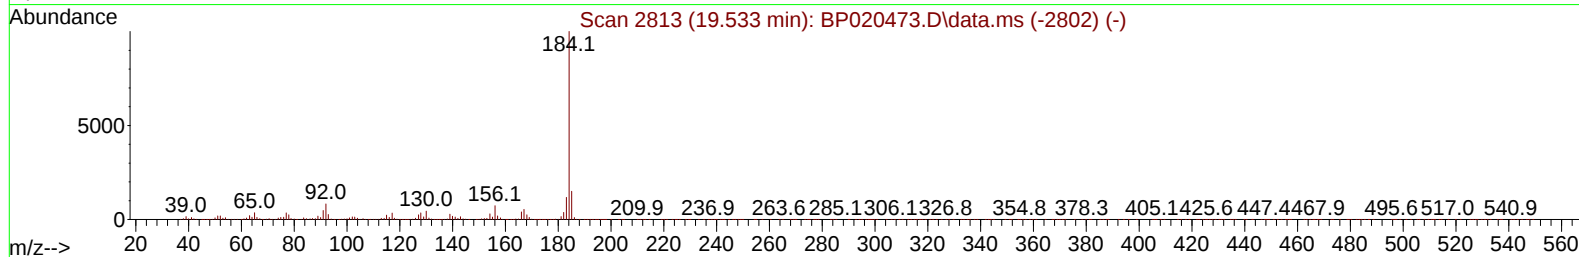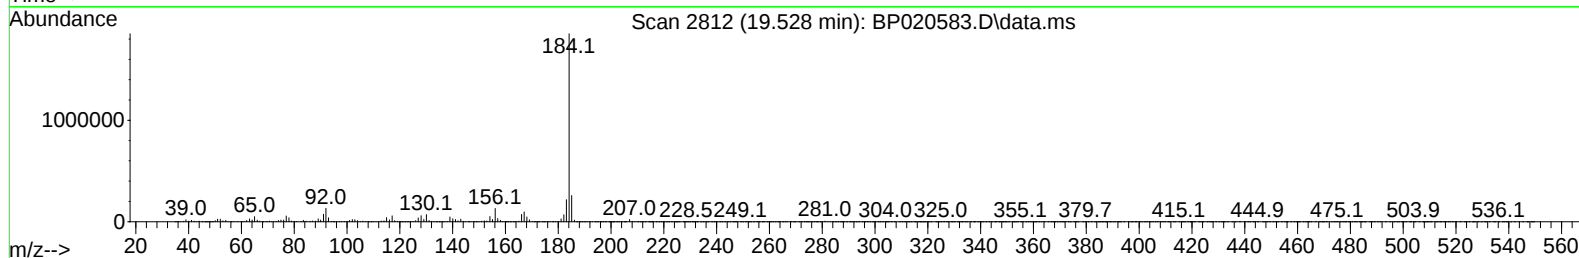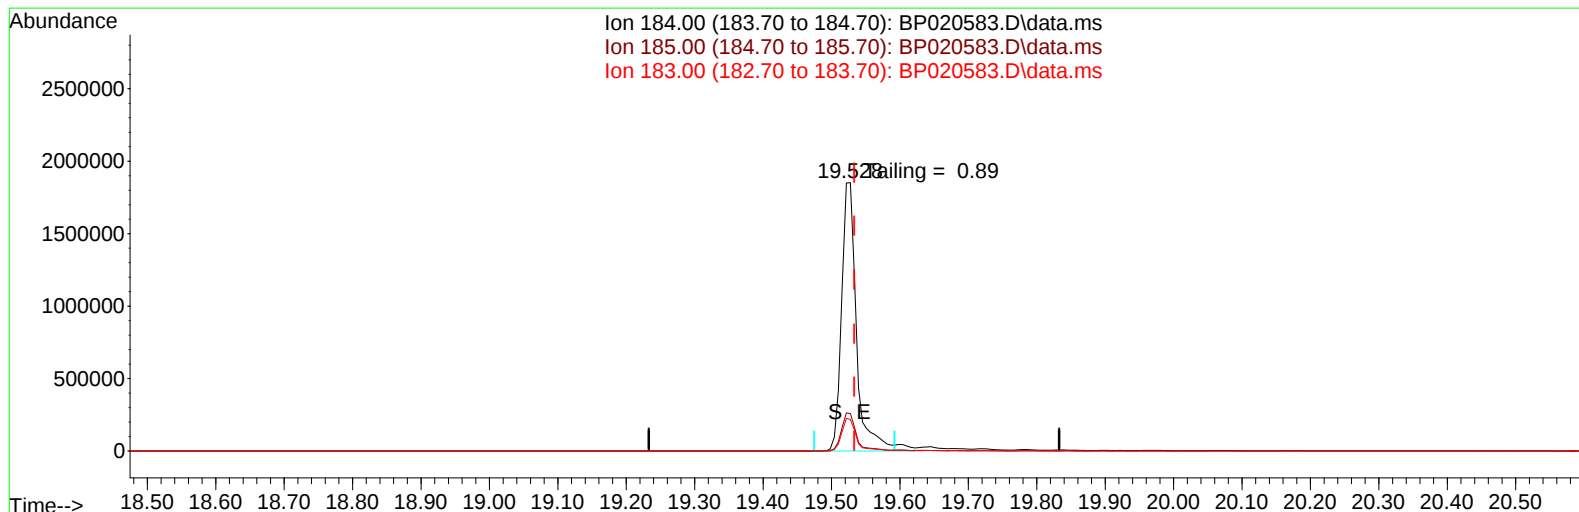

TIC: BP020583.D\data.ms

(77) Benzidine

19.528min (-0.005) 49895.37 ng

response 2795370

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.95
183.00	11.70	11.74
0.00	0.00	0.00