
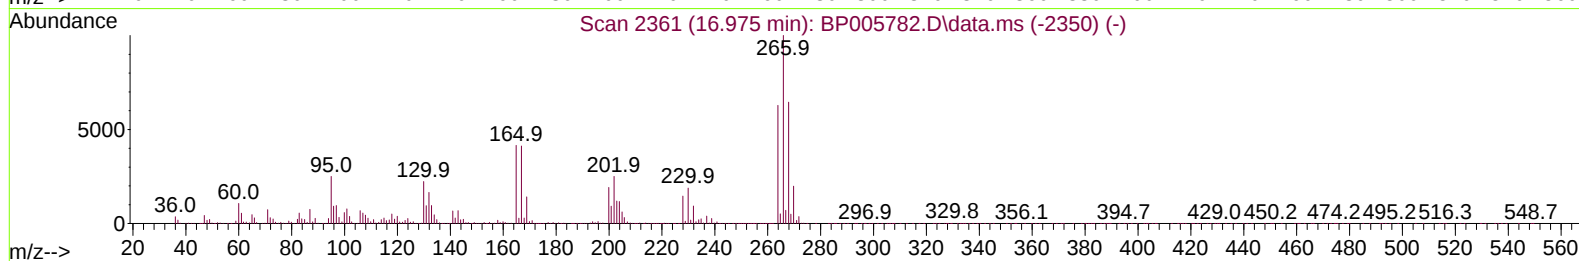
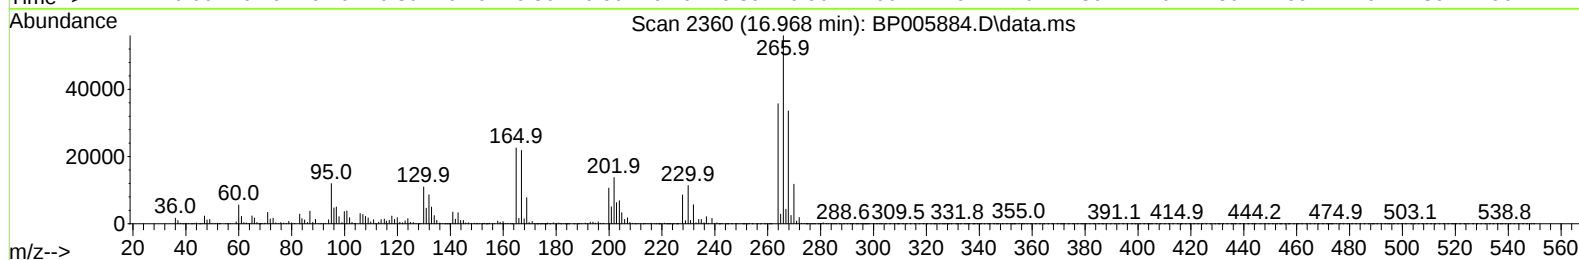


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061221\
 Data File : BP005884.D
 Acq On : 12 Jun 2021 09:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 03:53:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 13:53:36 2021
 Response via : Initial Calibration

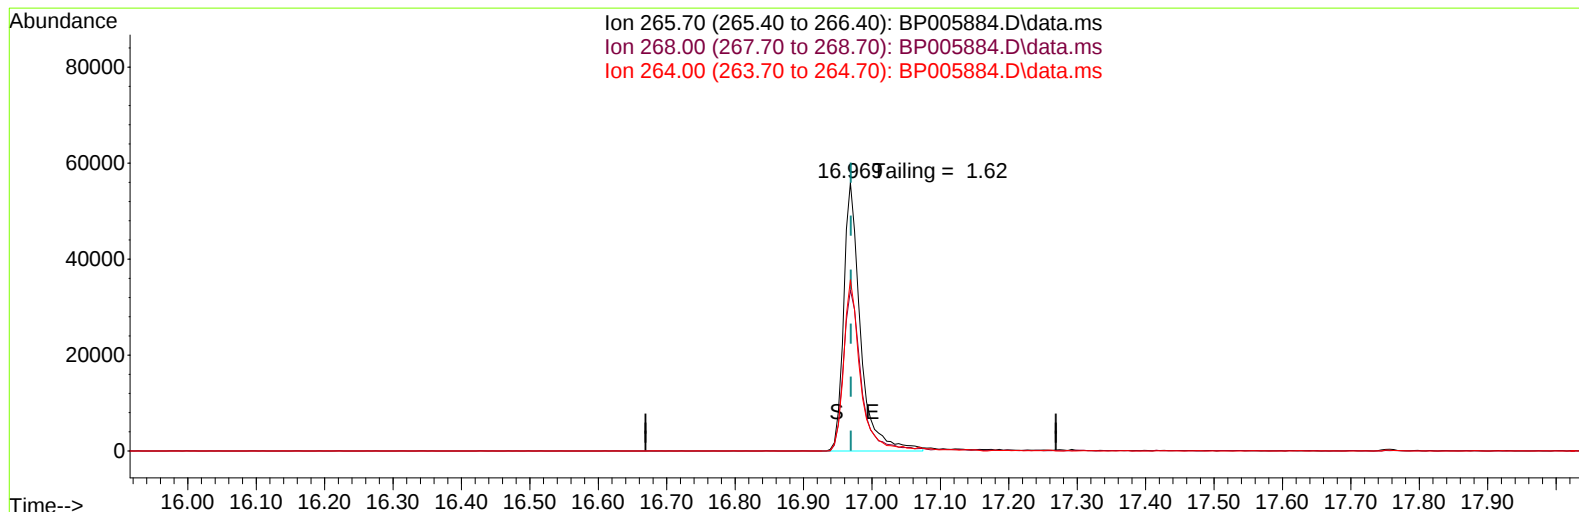

TIC: BP005884.D\data.ms

(70) Pentachlorophenol (C)




16.968min (-0.000) 776258.85 ng

response 92966

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	60.02
264.00	62.90	63.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061221\
 Data File : BP005884.D
 Acq On : 12 Jun 2021 09:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 03:53:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 13:53:36 2021
 Response via : Initial Calibration

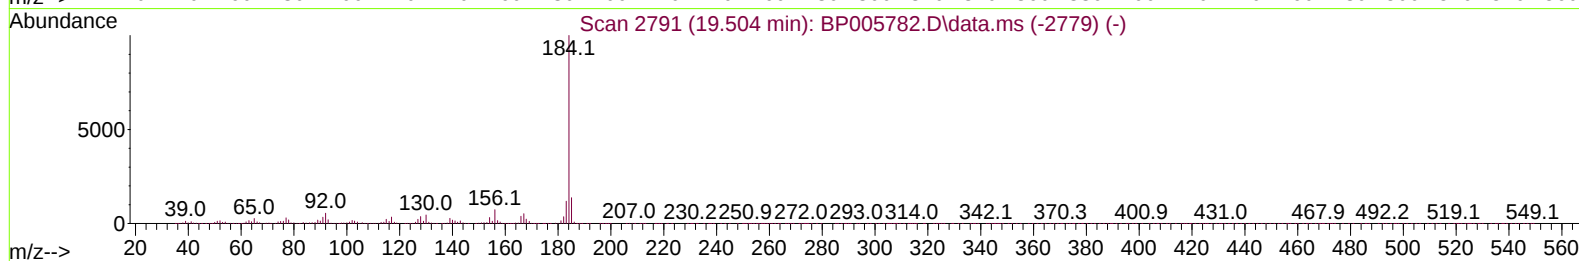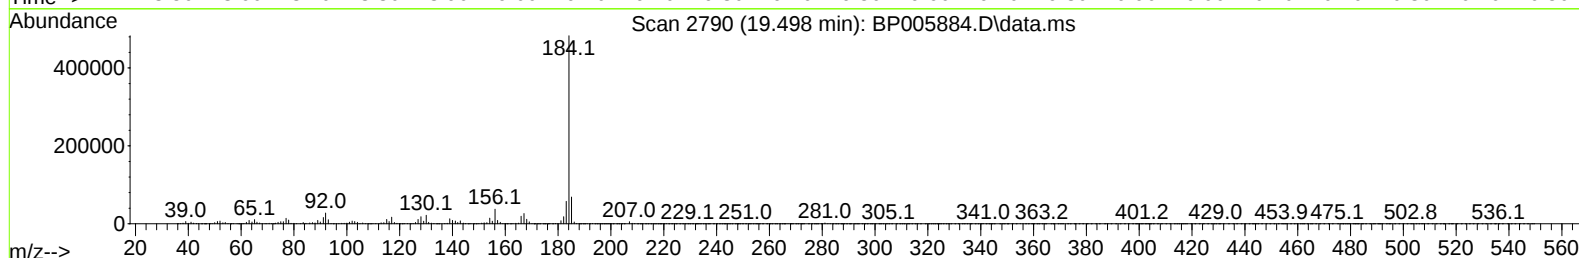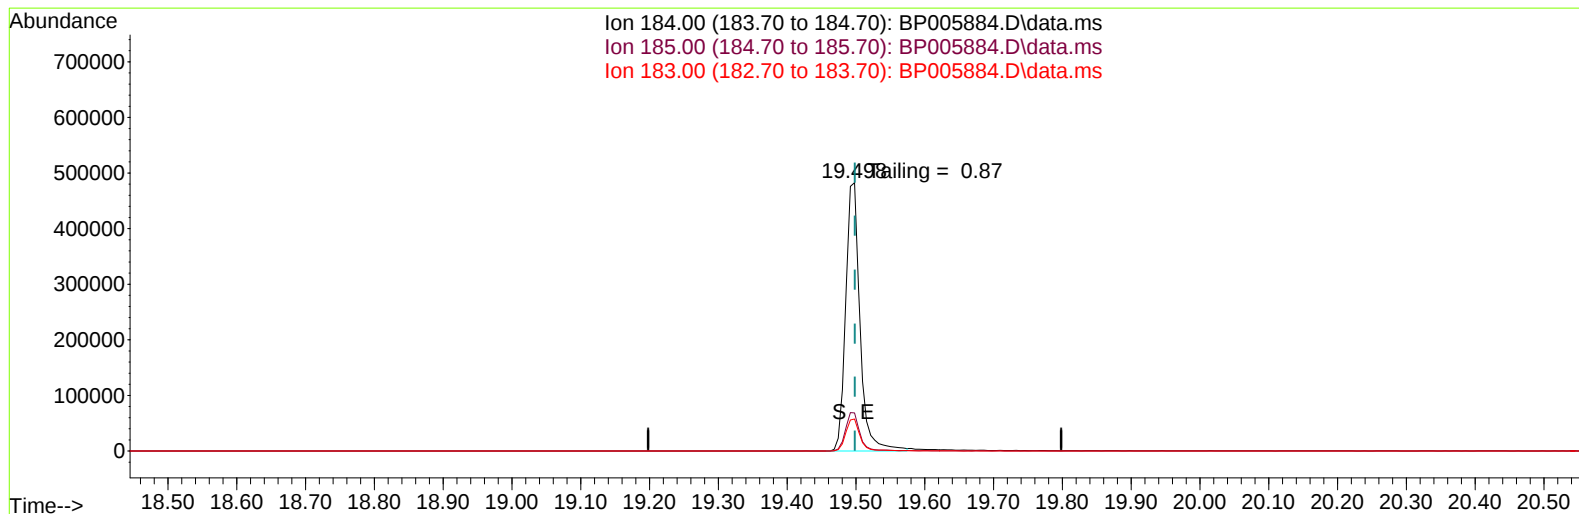

TIC: BP005884.D\data.ms

(77) Benzidine**19.498min (-0.000) 491950.18 ng****response 675609**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.21
183.00	11.90	11.94
0.00	0.00	0.00