

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP061221\  
 Data File : BP005891.D  
 Acq On : 12 Jun 2021 16:31  
 Operator : CG/JU  
 Sample : M2655-01  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 0226-FIELD-BLANK-2

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP060821.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005891.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.511       | 405           | 412         | 425          | rBV      | 1339914        | 1945093       | 41.44%          | 9.850%        |
| 2         | 7.116       | 678           | 685         | 709          | rBV      | 1151243        | 1921369       | 40.93%          | 9.730%        |
| 3         | 7.940       | 818           | 825         | 833          | rBV      | 251950         | 396521        | 8.45%           | 2.008%        |
| 4         | 9.104       | 1015          | 1023        | 1034         | rBV      | 750305         | 1207897       | 25.73%          | 6.117%        |
| 5         | 10.028      | 1172          | 1180        | 1194         | rBV      | 26421          | 73388         | 1.56%           | 0.372%        |
| 6         | 10.746      | 1294          | 1302        | 1314         | rBV      | 305865         | 522193        | 11.13%          | 2.645%        |
| 7         | 13.192      | 1711          | 1718        | 1728         | rBV      | 1862020        | 2823748       | 60.16%          | 14.300%       |
| 8         | 14.563      | 1945          | 1951        | 1960         | rVB      | 465720         | 690336        | 14.71%          | 3.496%        |
| 9         | 16.057      | 2198          | 2205        | 2224         | rBV      | 1706038        | 2514132       | 53.56%          | 12.732%       |
| 10        | 17.310      | 2412          | 2418        | 2425         | rVB      | 596246         | 840810        | 17.91%          | 4.258%        |
| 11        | 19.857      | 2846          | 2851        | 2861         | rVB      | 3805691        | 4693869       | 100.00%         | 23.771%       |
| 12        | 21.380      | 3106          | 3110        | 3115         | rBV      | 865888         | 1060189       | 22.59%          | 5.369%        |
| 13        | 23.798      | 3516          | 3521        | 3527         | rVB2     | 566322         | 1056780       | 22.51%          | 5.352%        |




Sum of corrected areas: 19746325

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP061221\  
Data File : BP005891.D  
Acq On : 12 Jun 2021 16:31  
Operator : CG/JU  
Sample : M2655-01  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
0226-FIELD-BLANK-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP060821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

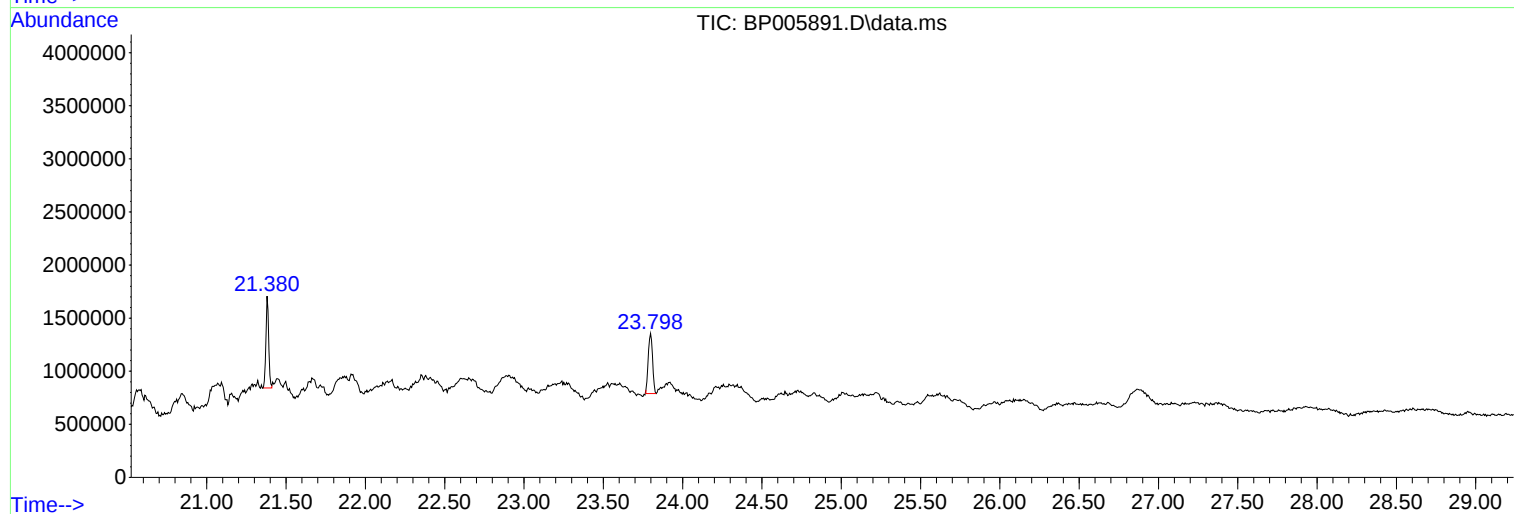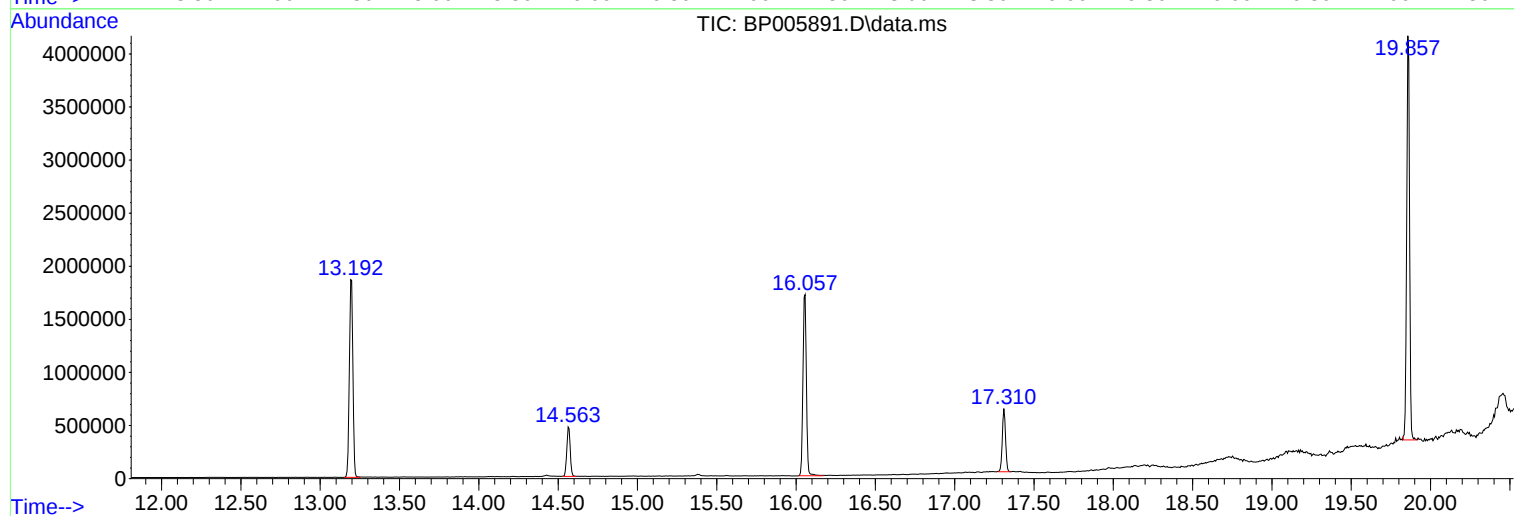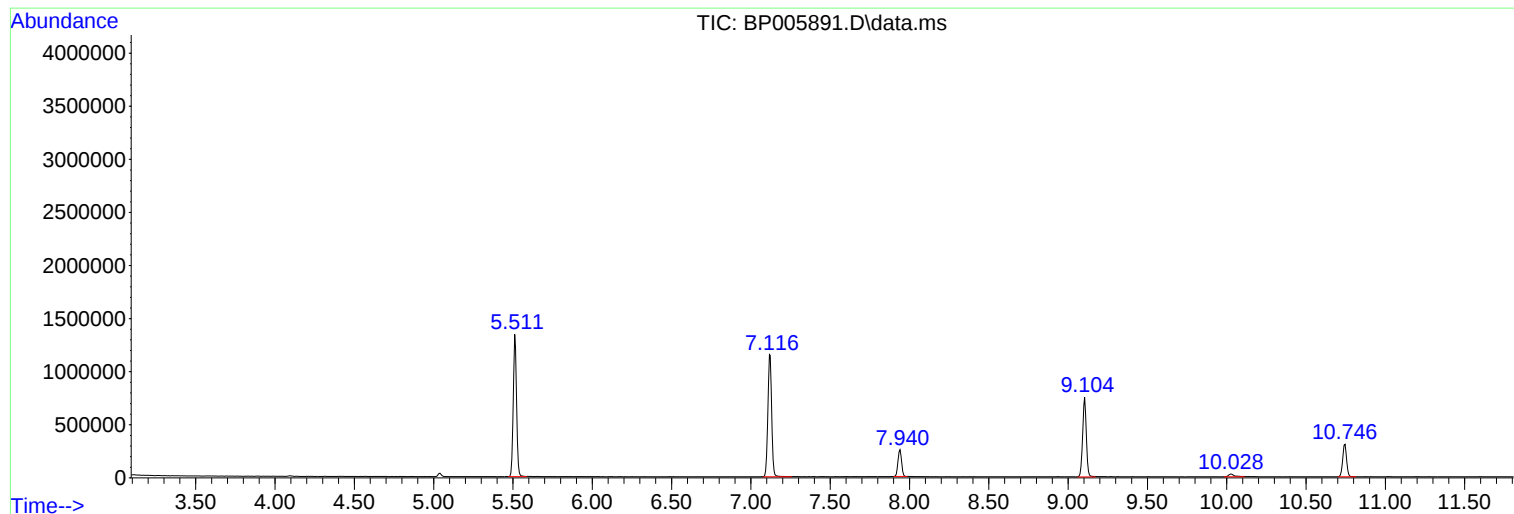

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP061221\  
Data File : BP005891.D  
Acq On : 12 Jun 2021 16:31  
Operator : CG/JU  
Sample : M2655-01  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
0226-FIELD-BLANK-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP060821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP061221\  
Data File : BP005891.D  
Acq On : 12 Jun 2021 16:31  
Operator : CG/JU  
Sample : M2655-01  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
0226-FIELD-BLANK-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP060821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|