


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061221\
 Data File : BP005884.D
 Acq On : 12 Jun 2021 09:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 11 13:53:36 2021

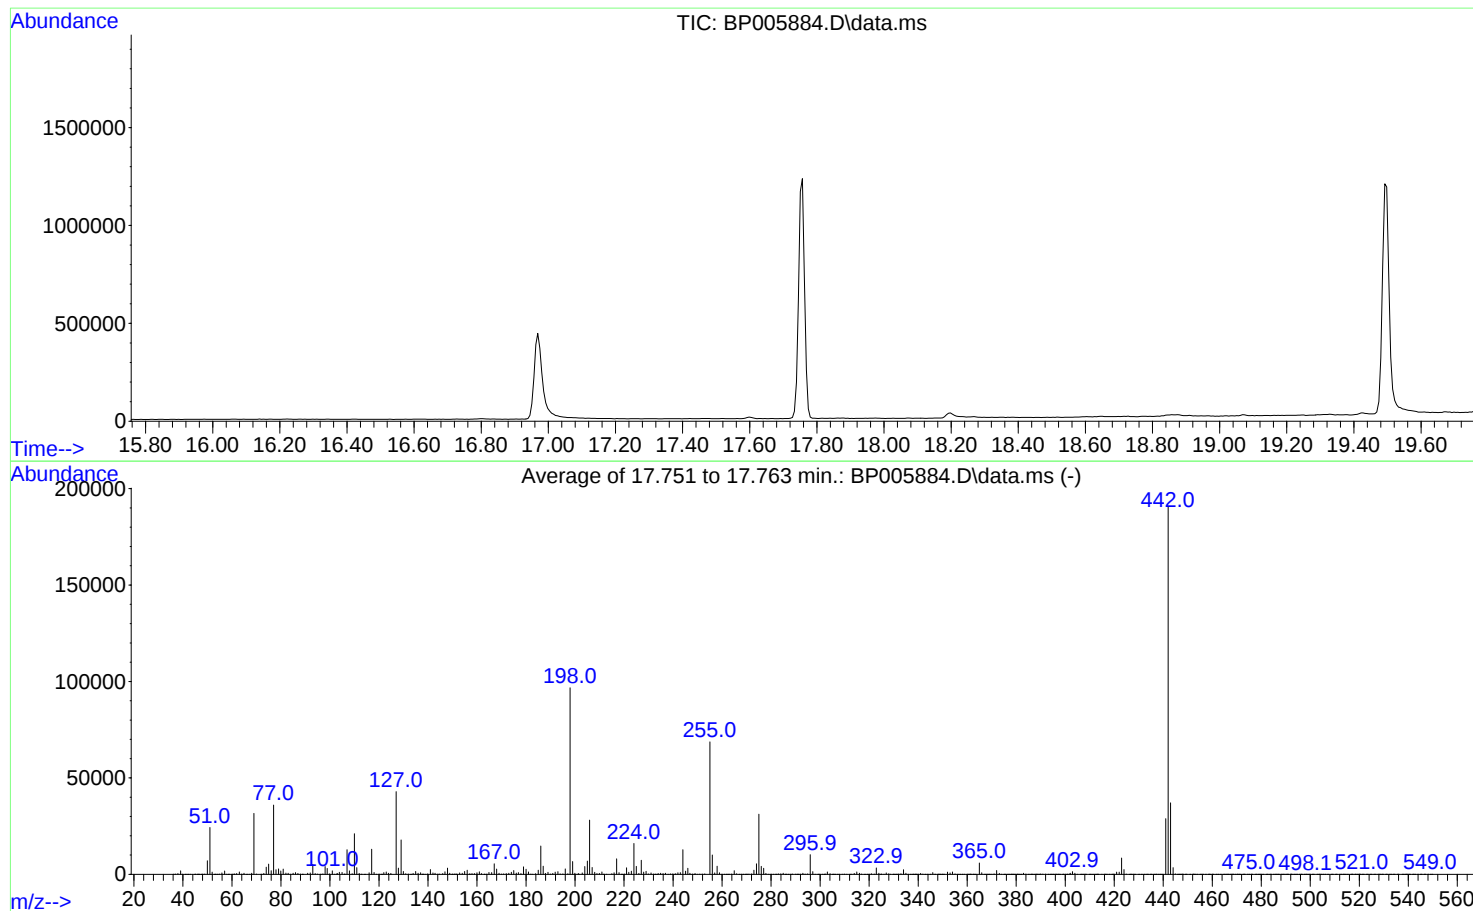




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.1	24293	PASS
68	69	0.00	2	1.9	604	PASS
69	198	0.00	100	32.7	31635	PASS
70	69	0.00	2	0.7	212	PASS
127	198	10	80	44.4	42907	PASS
197	198	0.00	2	0.3	304	PASS
198	198	100	100	100.0	96707	PASS
199	198	5	9	6.9	6641	PASS
275	198	10	60	32.3	31228	PASS
365	198	1	100	6.1	5910	PASS
441	198	0.01	100	29.9	28912	PASS
442	442	100	100	100.0	190733	PASS
443	442	15	24	19.5	37125	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061221\
 Data File : BP005884.D
 Acq On : 12 Jun 2021 09:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 14 03:53:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 13:53:36 2021
 Response via : Initial Calibration

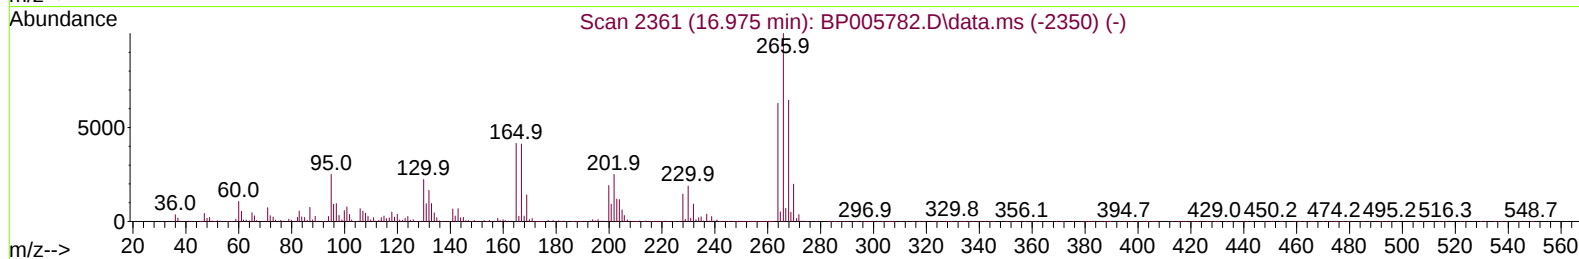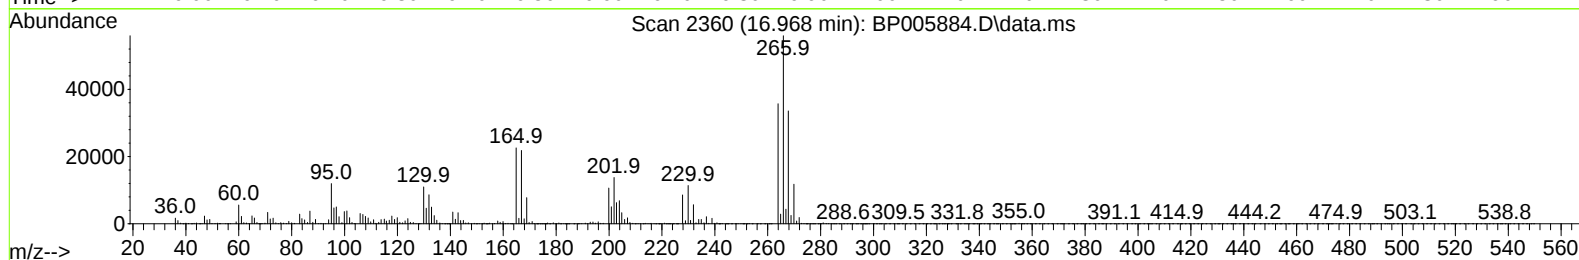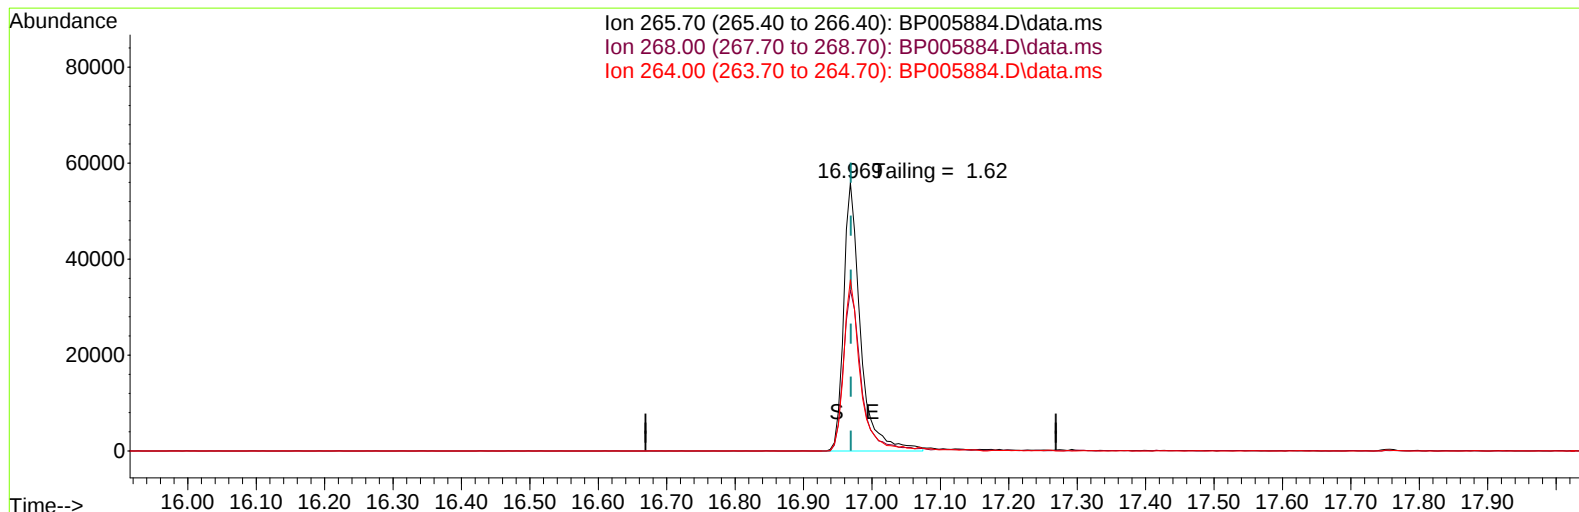

TIC: BP005884.D\data.ms

(70) Pentachlorophenol (C)

16.968min (-0.000) 776258.85 ng




response 92966

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	60.02
264.00	62.90	63.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061221\
 Data File : BP005884.D
 Acq On : 12 Jun 2021 09:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 14 03:53:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 13:53:36 2021
 Response via : Initial Calibration

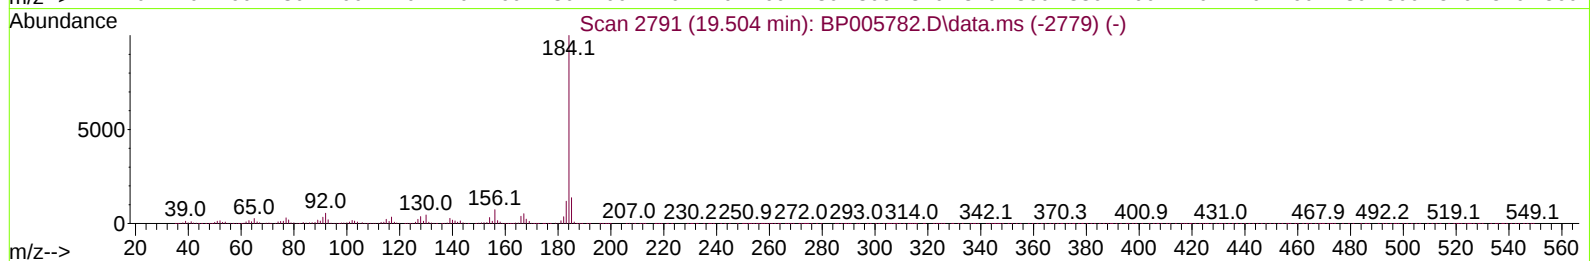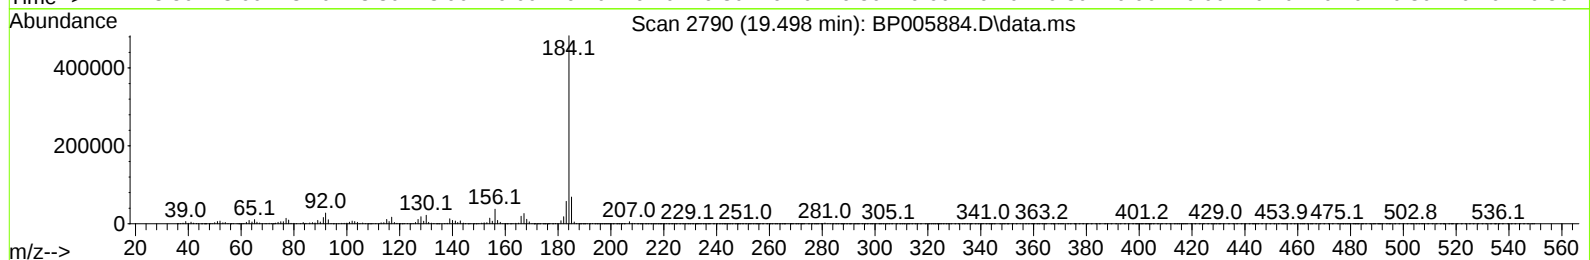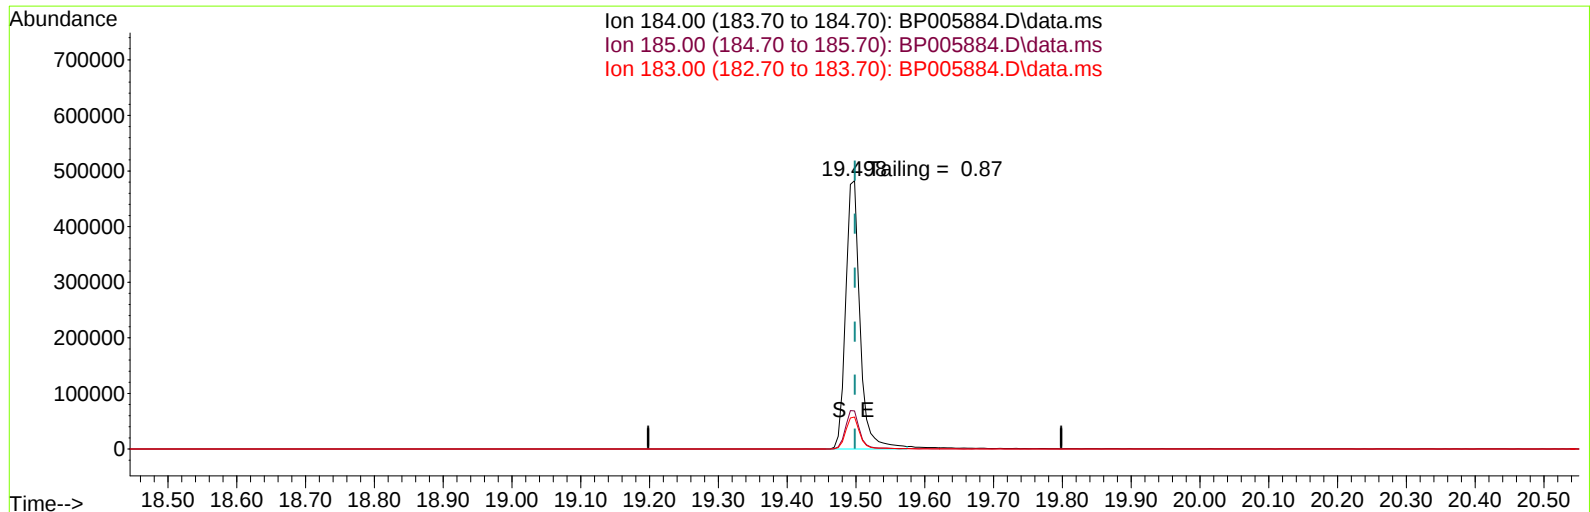

TIC: BP005884.D\data.ms

(77) Benzidine

19.498min (-0.000) 491950.18 ng

response 675609

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.21
183.00	11.90	11.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/12/2021	BNA_P	BP005884.D
Compound Name	Response	Retention Time
DDT	404068	20.692
DDD	6486	20.263
DDE	2495	19.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8981	413049	2.17